
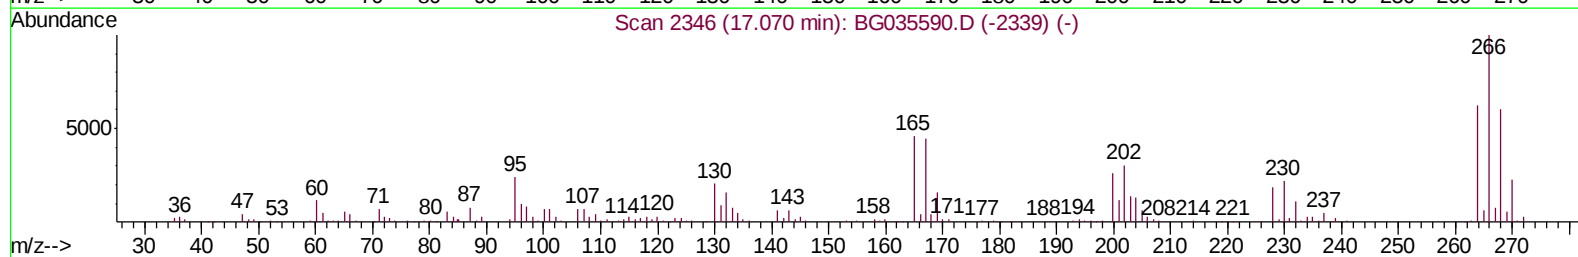
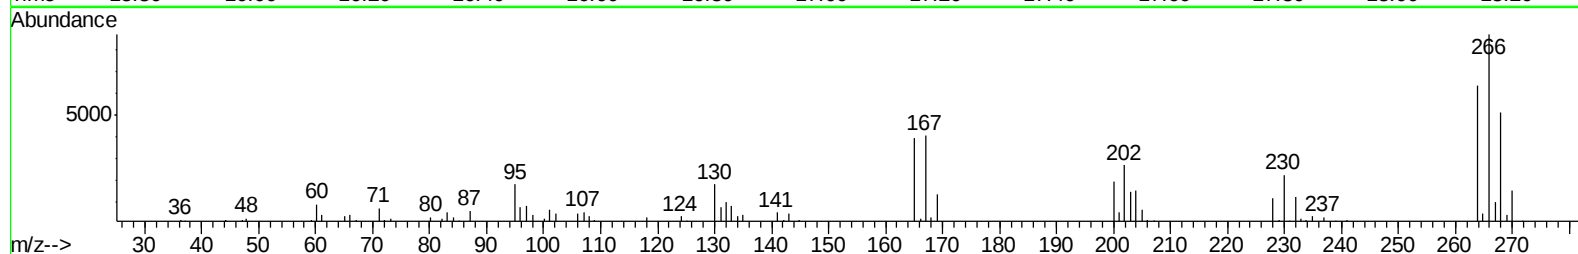


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG080818\
Data File : BG036214.D
Acq On : 9 Aug 2018 2:27
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 08:15:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

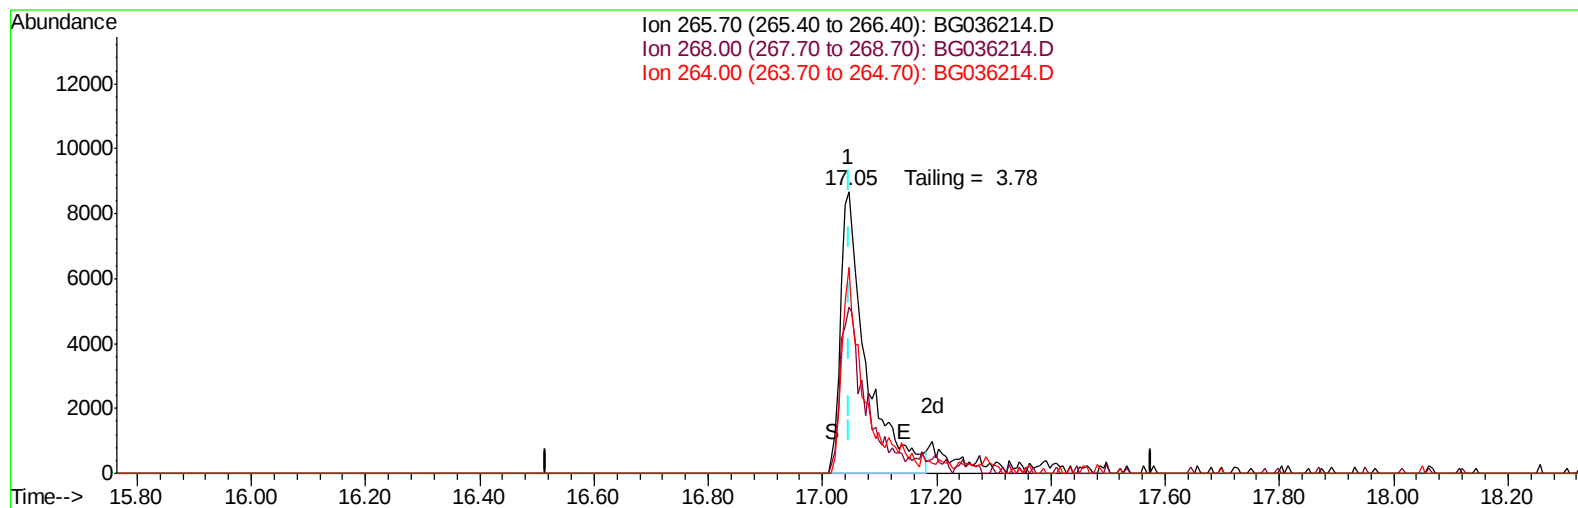

TIC: BG036214.D

(69) Pentachlorophenol (C)




17.045min (-0.002) 0.00ng

response 26759

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.20
264.00	62.00	73.05
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG080818\
Data File : BG036214.D
Acq On : 9 Aug 2018 2:27
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 08:15:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

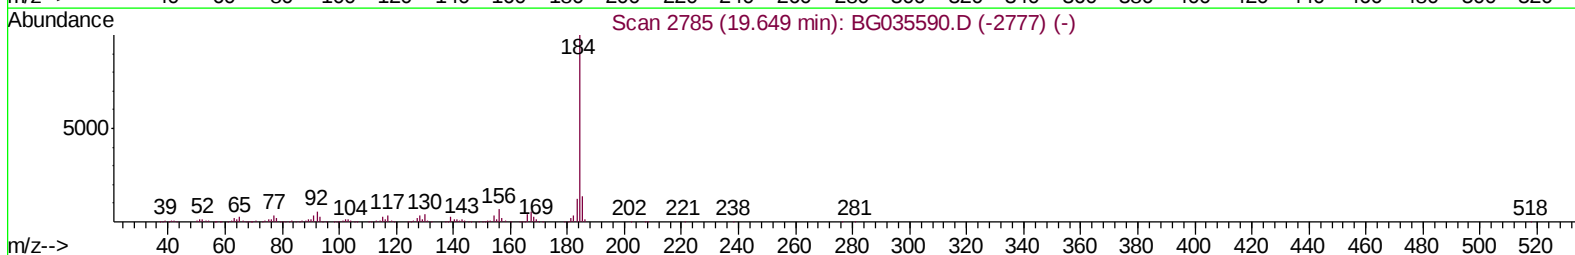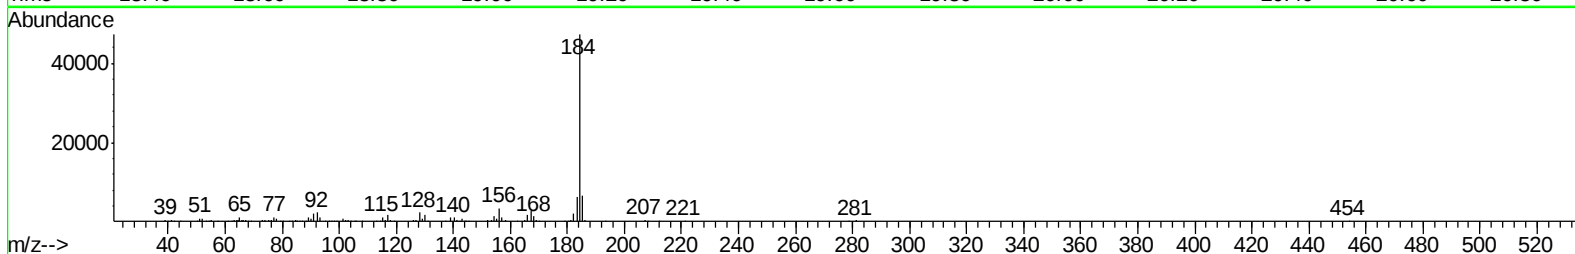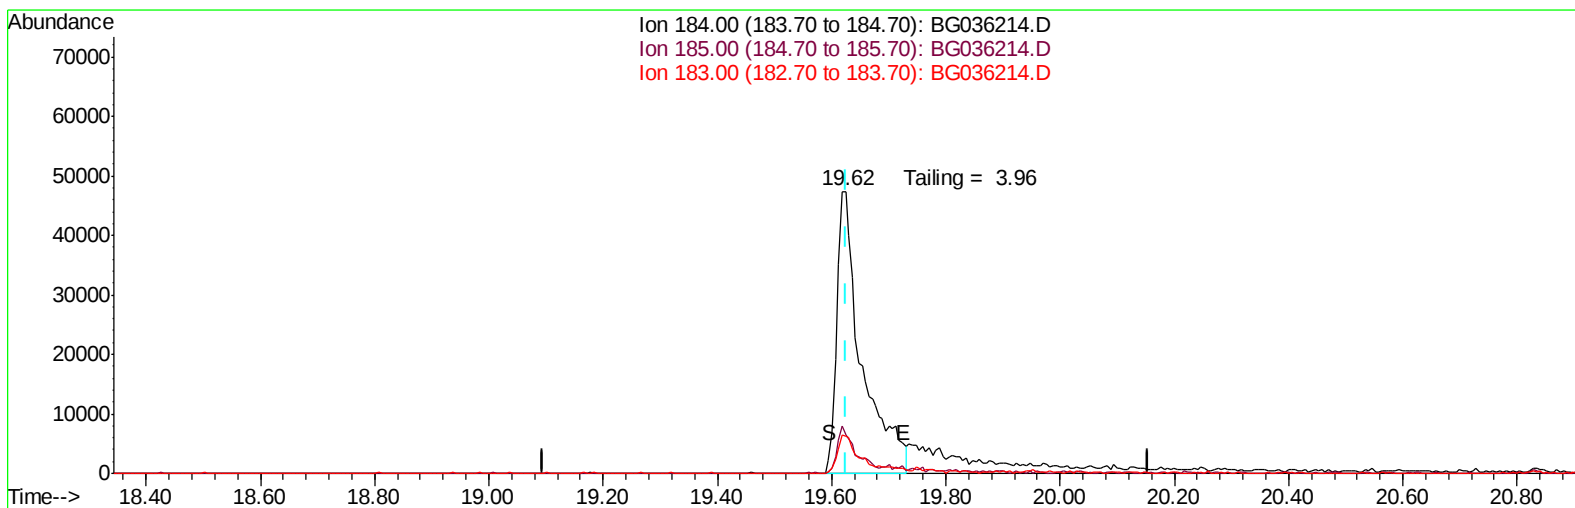

TIC: BG036214.D

(76) Benzidine

19.624min (-0.002) 89352.43ng

response 143295

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.74
183.00	13.30	13.05
0.00	0.00	0.00