


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080818\
 Data File : BG036214.D
 Acq On : 9 Aug 2018 2:27
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 31 12:30:06 2018

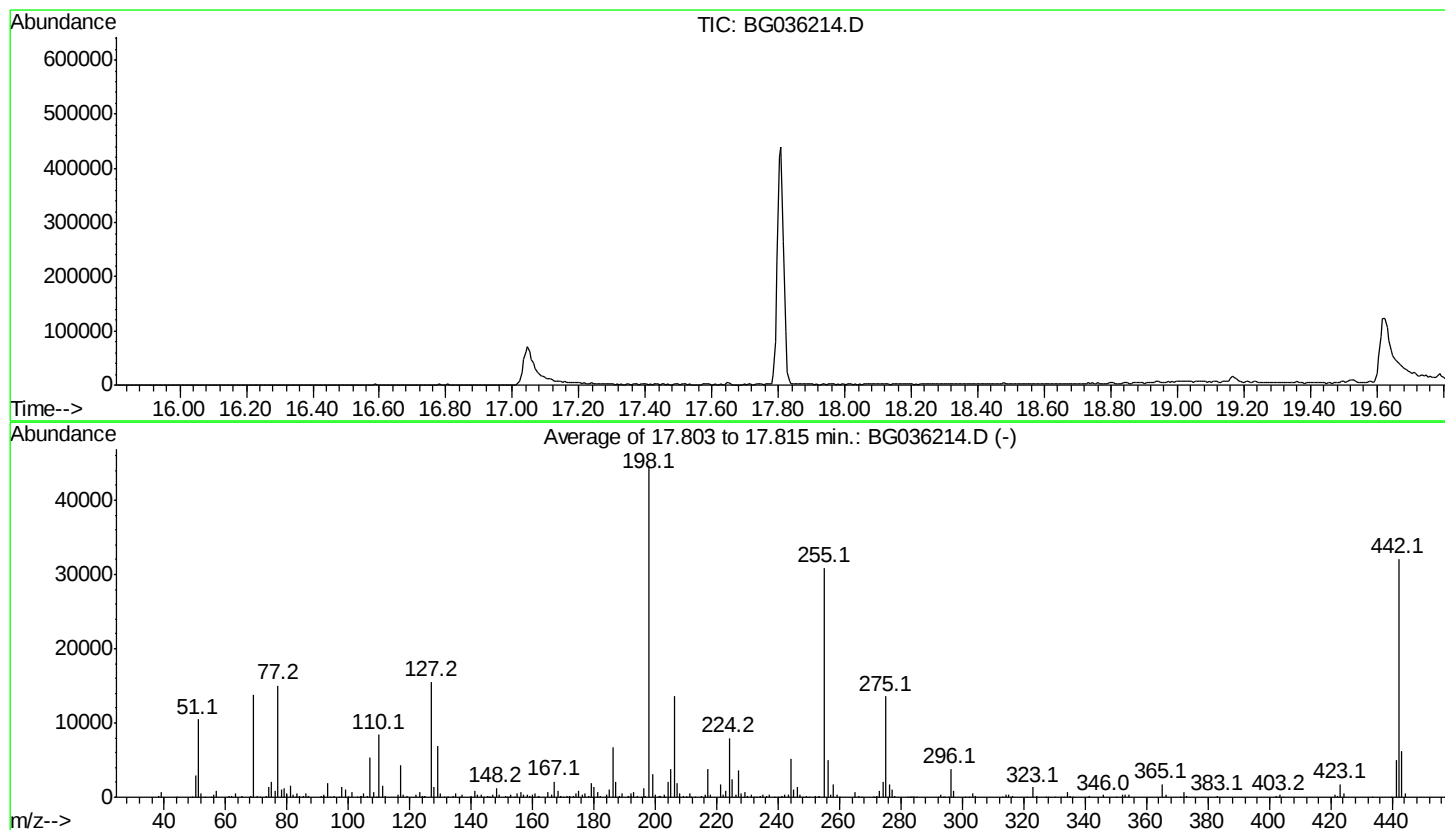

AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.5	10508	PASS
68	69	0.00	2	1.2	162	PASS
69	198	0.00	100	31.0	13850	PASS
70	69	0.00	2	1.2	161	PASS
127	198	10	80	34.8	15561	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	44672	PASS
199	198	5	9	7.0	3135	PASS
275	198	10	60	30.4	13582	PASS
365	198	1	100	4.0	1790	PASS
441	198	0.01	100	11.3	5063	PASS
442	198	50	100	71.9	32122	PASS
443	442	15	24	19.1	6144	PASS