

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG080819\
 Data File : BG042116.D
 Acq On : 10 Aug 2019 00:01
 Operator : HP/JU
 Sample : K4041-11
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BENT5

Manual Integrations
 APPROVED

Sohil
 8/13/2019 8:19:25 AM

Quant Time: Aug 10 04:43:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 09 16:22:05 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.03	152	79657	20.00	ng/ul	0.00
18) Naphthalene-d8	10.85	136	328169	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.69	164	229740	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.44	188	482838	20.00	ng/ul	0.00
77) Chrysene-d12	21.73	240	477794	20.00	ng/ul	0.00
85) Perylene-d12	24.99	264	566208	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.41	96	3782	2.08	ng/uL	0.00
5) Phenol-d5	7.18	99	88408	14.14	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.34	67	48615	13.90	ng/ul	0.00
9) 2-Chlorophenol-d4	7.56	132	88749	16.61	ng/ul	0.00
13) 4-Methylphenol-d8	8.74	113	76470	14.57	ng/ul	0.00
19) Nitrobenzene-d5	9.19	128	44253	17.91	ng/ul	0.00
22) 2-Nitrophenol-d4	9.92	143	55298	19.28	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.47	165	98198	16.96	ng/ul	0.00
29) 4-Chloroaniline-d4	10.99	131	101167	15.75	ng/ul	0.00
43) Dimethylphthalate-d6	14.09	166	307829	17.28	ng/ul	0.00
46) Acenaphthylene-d8	14.38	160	366930	18.03	ng/ul	0.00
51) 4-Nitrophenol-d4	14.89	143	24097m	8.05	ng/ul	0.01
57) Fluorene-d10	15.68	176	281351	17.75	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.80	200	37902	12.24	ng/ul	0.00
70) Anthracene-d10	17.54	188	434024	18.74	ng/ul	0.00
78) Pyrene-d10	19.82	212	494014	18.53	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.76	264	556671	18.82	ng/ul	0.00

Target Compounds

					Ovalue
6) Phenol	7.21	94	13226	2.050 ng/ul	92
44) Dimethylphthalate	14.13	163	65396	3.696 ng/ul	98
69) Phenanthrene	17.48	178	30149	1.141 ng/ul	98
76) Fluoranthene	19.49	202	78440m	2.568 ng/ul	
79) Pyrene	19.85	202	78649	2.447 ng/ul#	96
82) Benzo(a)anthracene	21.70	228	40223	1.214 ng/ul	98
84) Chrysene	21.77	228	44066	1.425 ng/ul	97
87) Benzo(b)fluoranthene	23.95	252	64445	1.814 ng/ul	98
90) Benzo(a)pyrene	24.83	252	44660	1.319 ng/ul	97
93) Benzo(a,h,i)perylene	29.87	276	34070m	1.033 ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG080819\
Data File : BG042116.D
Acq On : 10 Aug 2019 00:01
Operator : HP/JU
Sample : K4041-11
Misc :
ALS Vial : 46 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BENT5

Quant Time: Aug 10 04:43:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 09 16:22:05 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
8/13/2019 8:19:25 AM

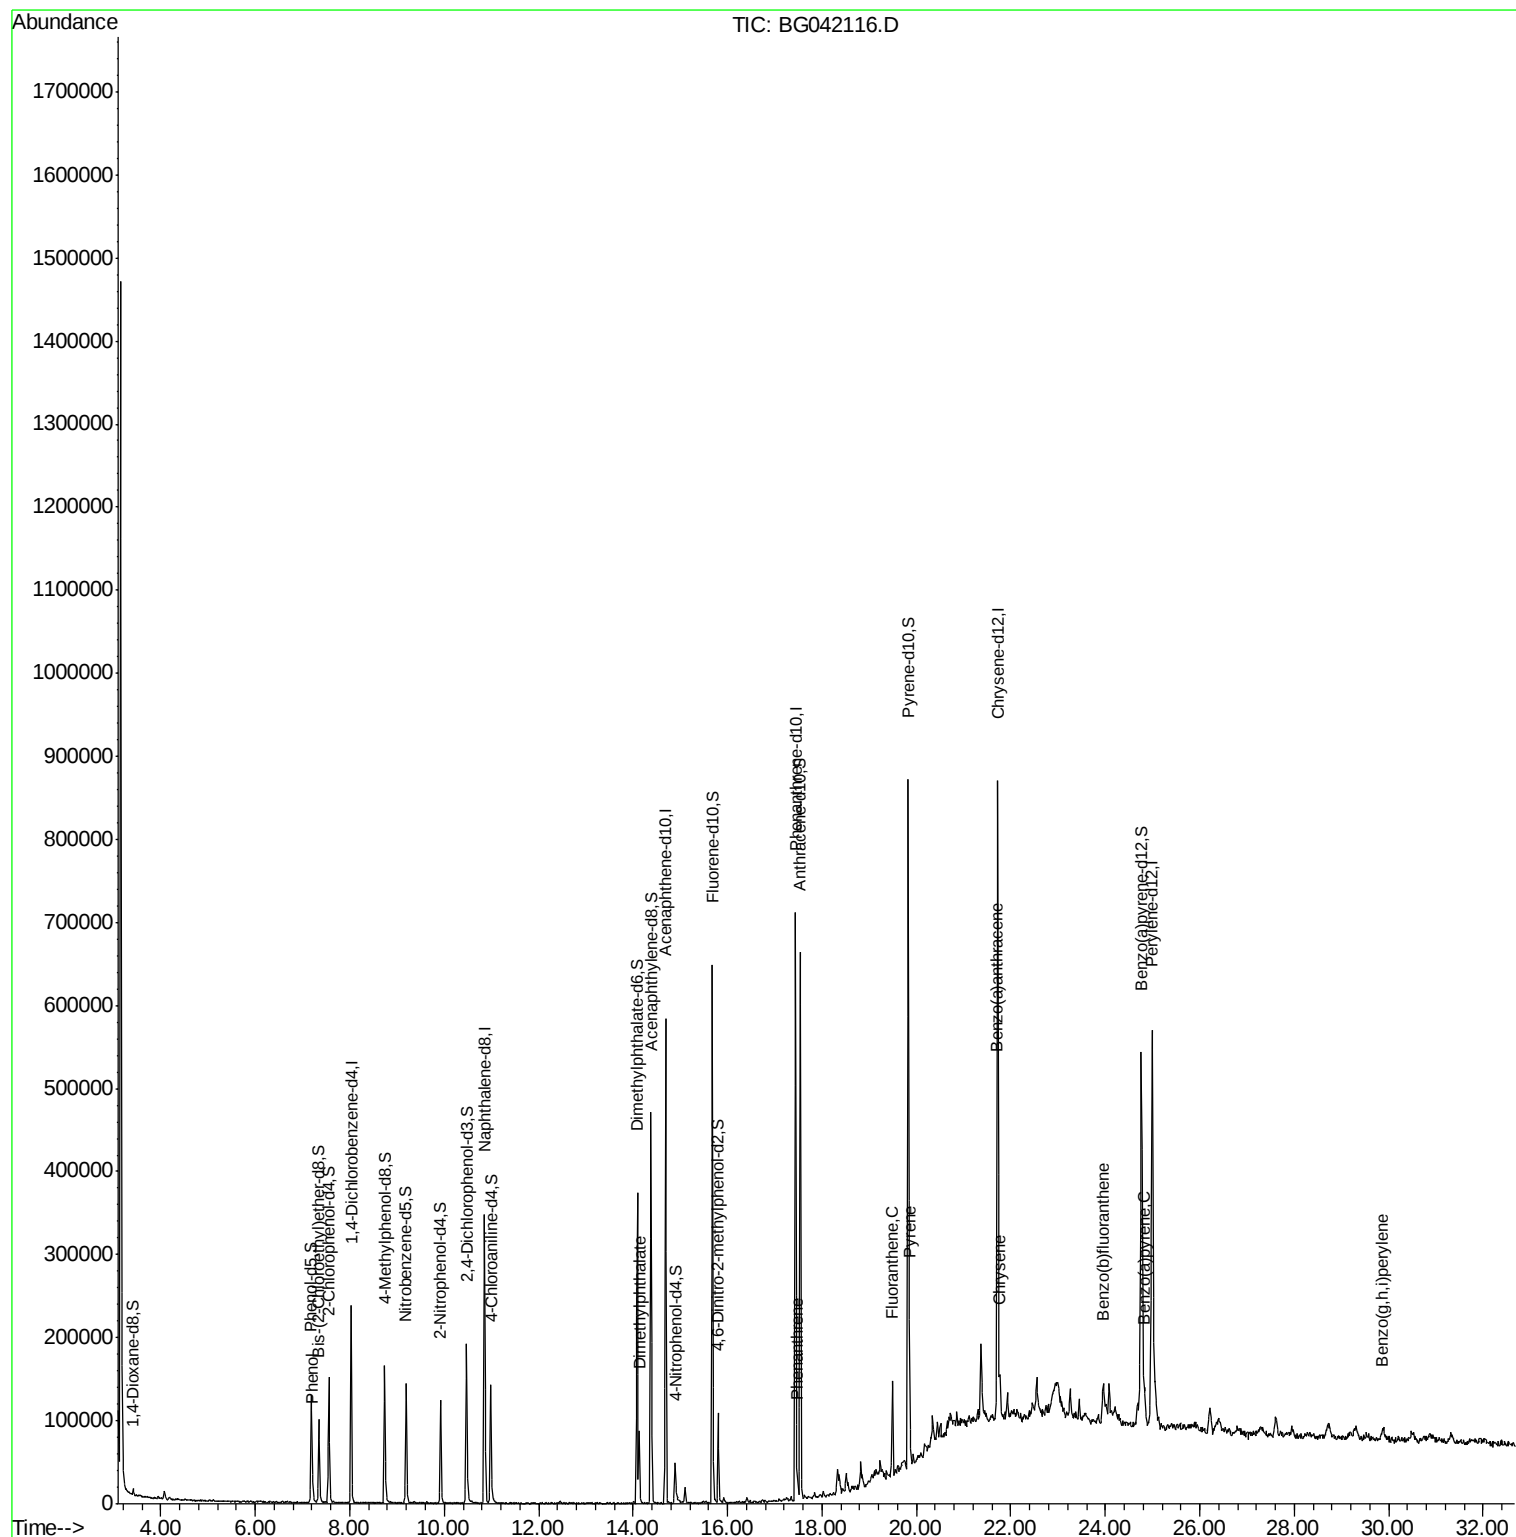

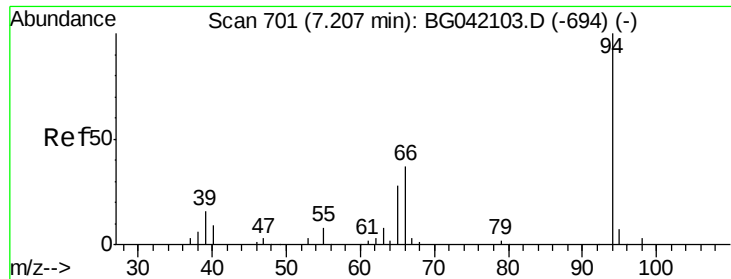

#6

Phenol





Concen: 2.050 ng/ul
 RT: 7.21 min Scan# 702
 Delta R.T. 0.01 min
 Lab File: BG042116.D
 Acq: 10 Aug 2019 00:01

Instrument :
 BNA_G
 ClientSampleId :
 BENT5

Tot Ion	Ion	Ratio	Resp	Lower	Upper
94	100		13226		
65	29.7	25.8	38.6		
66	33.3	31.8	47.8		

Manual Integrations
 APPROVED

Sohil
 8/13/2019 8:19:25 AM

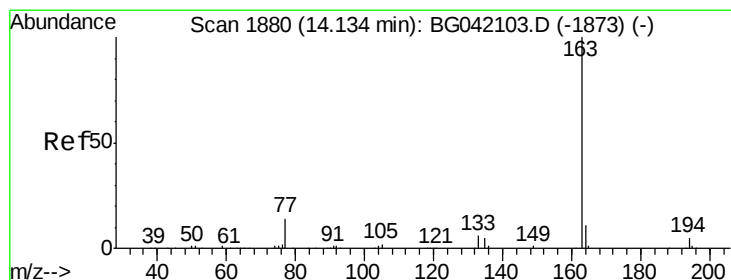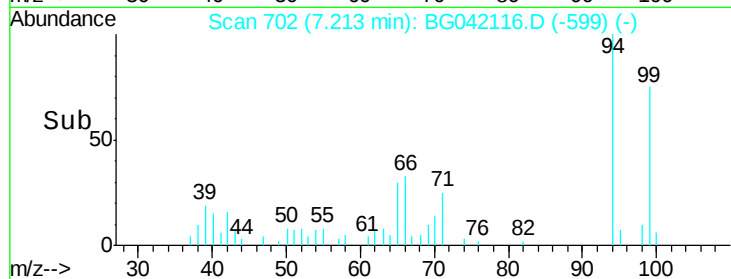
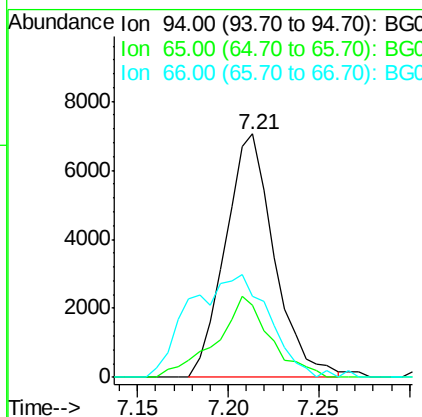
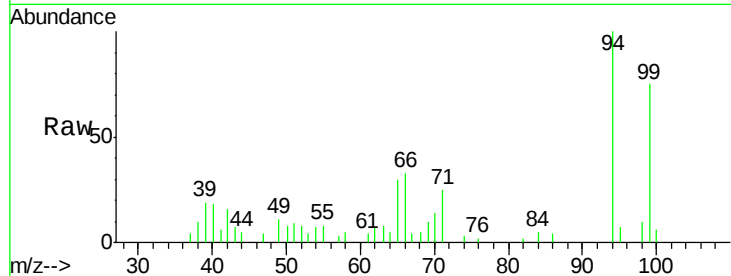



#44

Dimethylphthalate

Concen: 3.696 ng/ul
 RT: 14.13 min Scan# 1880
 Delta R.T. 0.00 min
 Lab File: BG042116.D
 Acq: 10 Aug 2019 00:01

Tgt Ion	Ion	Ratio	Resp	Lower	Upper
163	100		65396		
194	4.6	4.2	6.2		
164	10.6	7.8	11.8		

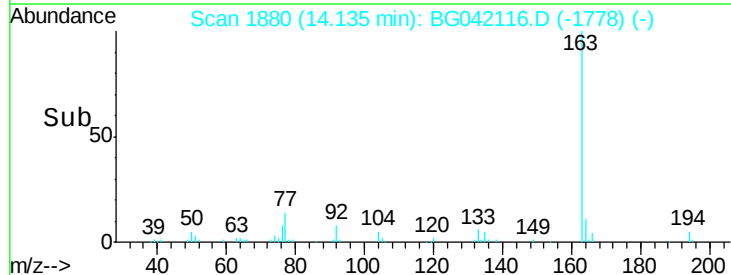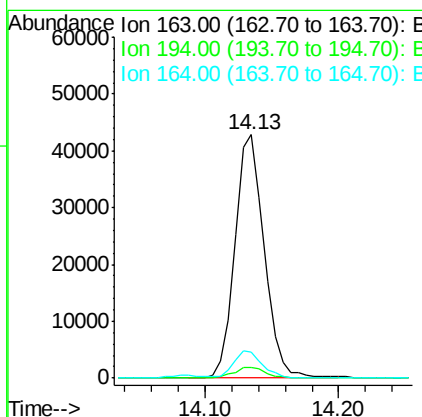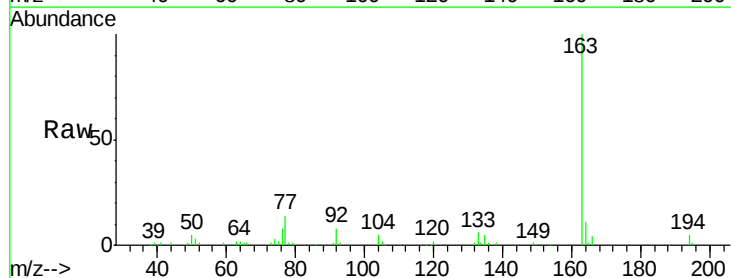

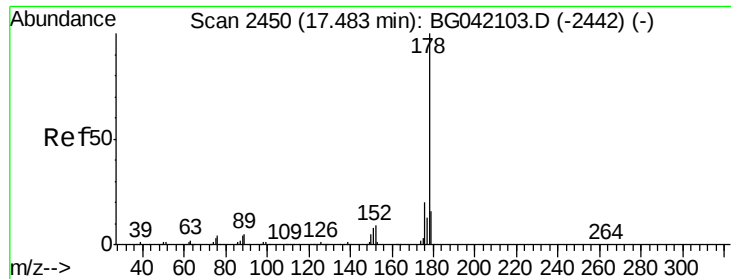


#69
Phenanthrene
Concen: 1.141 ng/ul
RT: 17.48 min Scan# 2450
Delta R.T. 0.00 min
Lab File: BG042116.D
Acq: 10 Aug 2019 00:01

Instrument :
BNA_G
ClientSampled :
BENT5

Tot Ion	Ratio	Lower	Upper
178	100		
179	14.9	12.8	19.2
176	19.6	15.4	23.2

Manual Integrations
APPROVED

Sohil
8/13/2019 8:19:25 AM



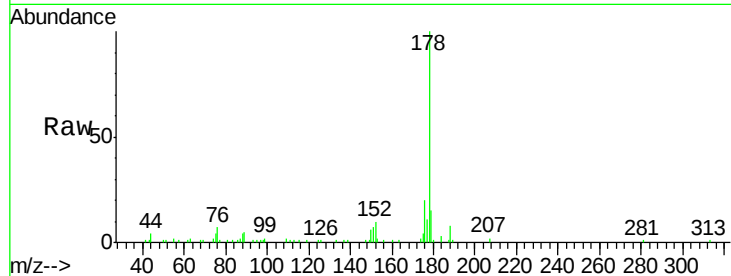


Abundance

Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

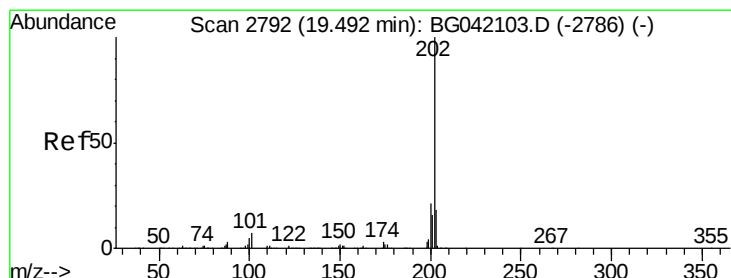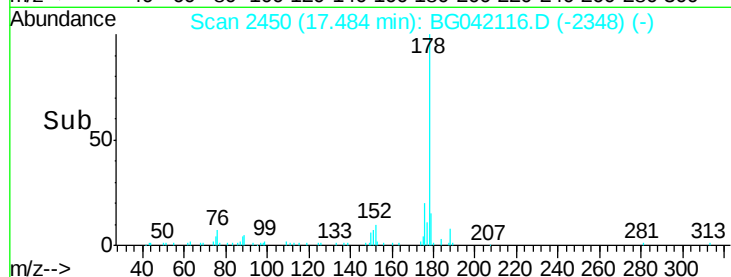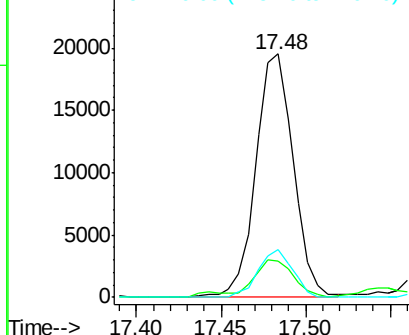

#76
Fluoranthene
Concen: 2.568 ng/ul m
RT: 19.49 min Scan# 2792
Delta R.T. 0.00 min
Lab File: BG042116.D
Acq: 10 Aug 2019 00:01




Tgt Ion	Ratio	Lower	Upper
202	100		
101	6.0	6.7	10.1#
100	5.5	5.3	7.9


Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

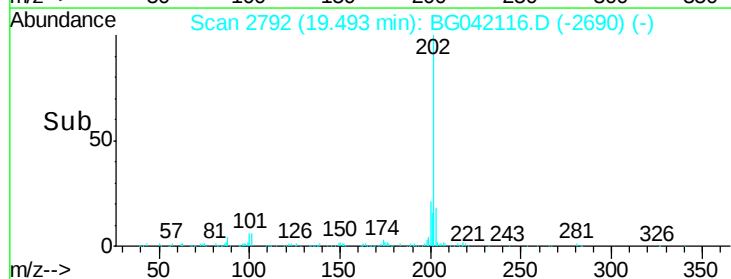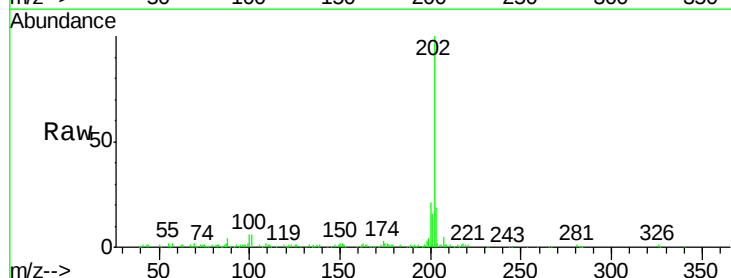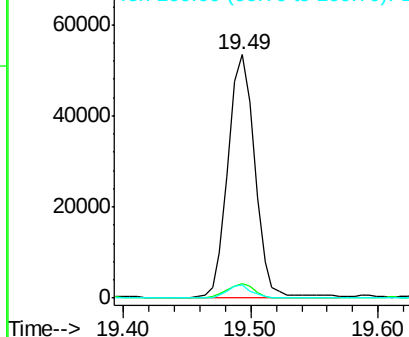

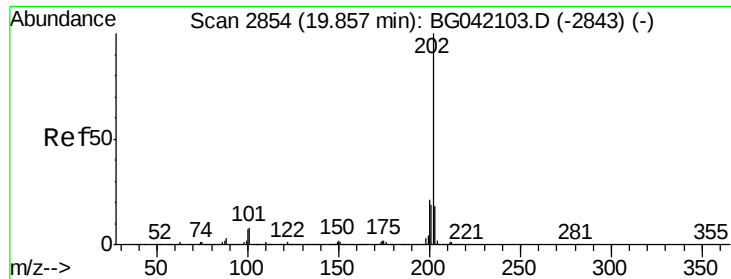

#79

Pvrene

Concen: 2.447 ng/ul

RT: 19.85 min Scan# 2853

Delta R.T. -0.01 min

Lab File: BG042116.D

Acq: 10 Aug 2019 00:01

Instrument :

BNA_G





ClientSampleId :

BENT5

Tot Ion:	202	Resp:	78649
Ion Ratio	Lower	Upper	
202	100		
101	7.5	7.6	11.4#
100	7.4	6.5	9.7

Manual Integrations
APPROVED

Sohil
8/13/2019 8:19:25 AM

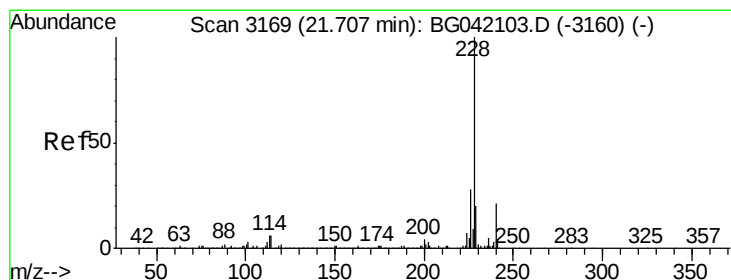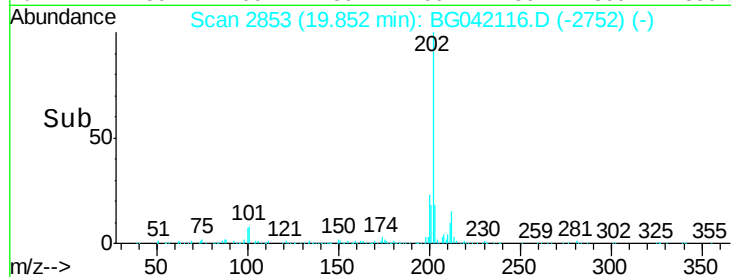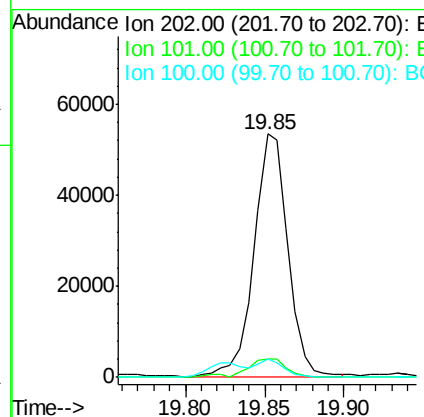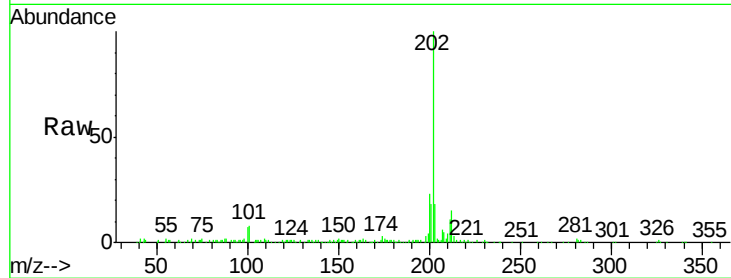

#82

Benzo(a)anthracene

Concen: 1.214 ng/ul




RT: 21.70 min Scan# 3168


Delta R.T. 0.00 min

Lab File: BG042116.D

Acq: 10 Aug 2019 00:01

Tgt Ion:	228	Resp:	40223
Ion Ratio	Lower	Upper	
228	100		
229	23.2	17.0	25.6
226	28.5	23.3	34.9

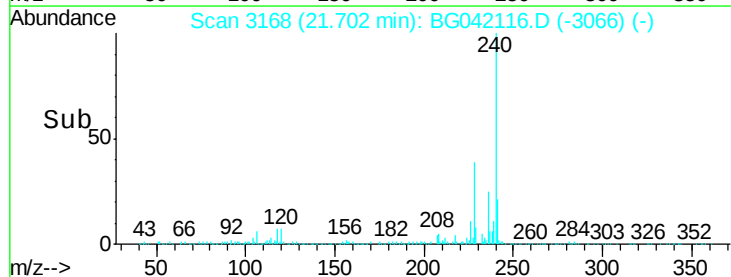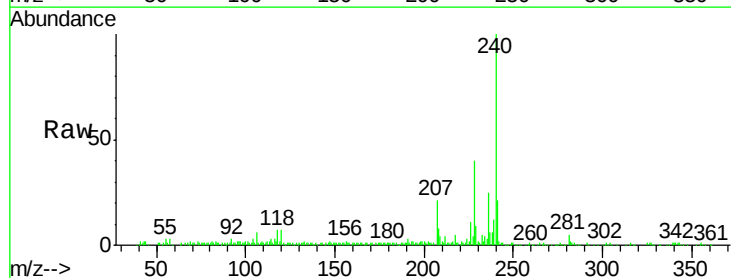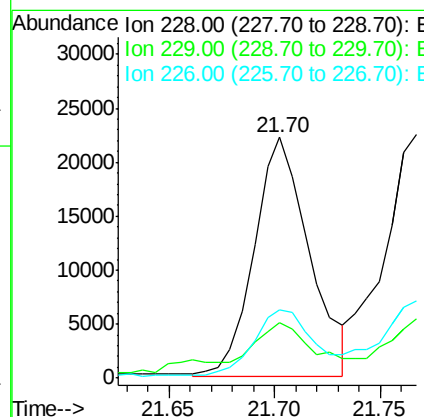

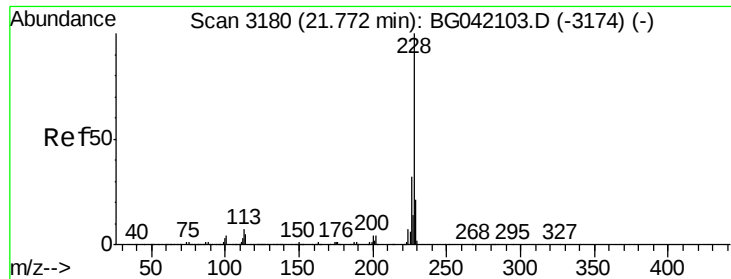





#84
Chrysene
Concen: 1.425 ng/ul
RT: 21.77 min Scan# 3179
Delta R.T. 0.00 min
Lab File: BG042116.D
Acq: 10 Aug 2019 00:01

Instrument :
BNA_G
ClientSampleId :
BENT5

Tot Ion	Ratio	Lower	Upper
228	100		
226	32.0	25.7	38.5
229	24.1	16.6	24.8




Manual Integrations
APPROVED


Sohil
8/13/2019 8:19:25 AM

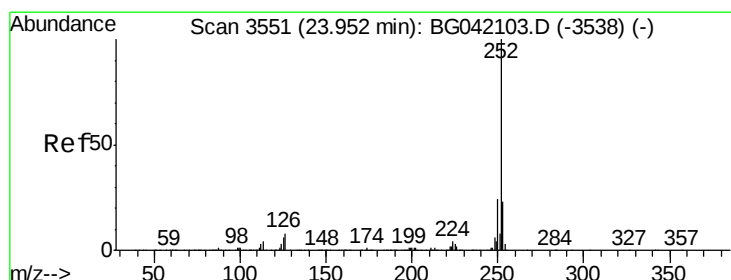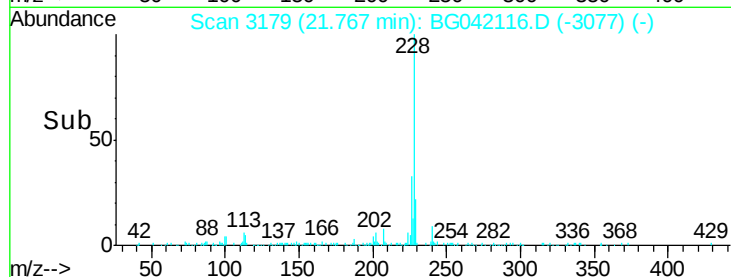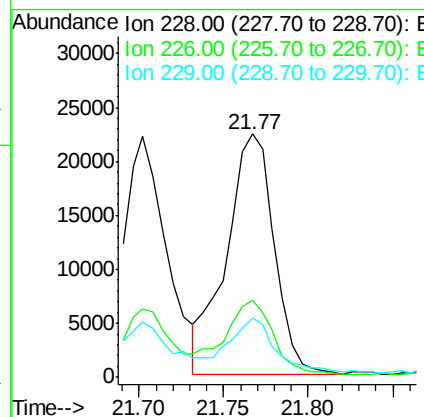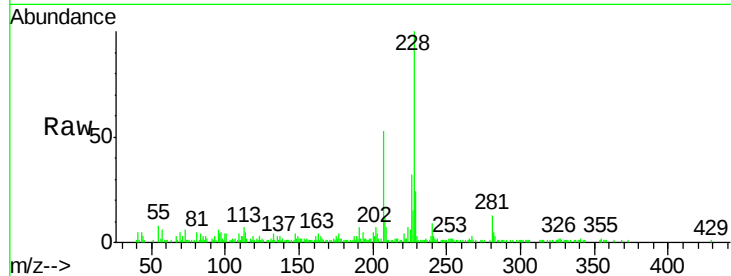

#87
Benzo(b)fluoranthene
Concen: 1.814 ng/ul
RT: 23.95 min Scan# 3551
Delta R.T. 0.01 min
Lab File: BG042116.D
Acq: 10 Aug 2019 00:01

Tgt Ion	Ratio	Lower	Upper
252	100		
253	24.4	18.4	27.6
125	7.6	5.8	8.8

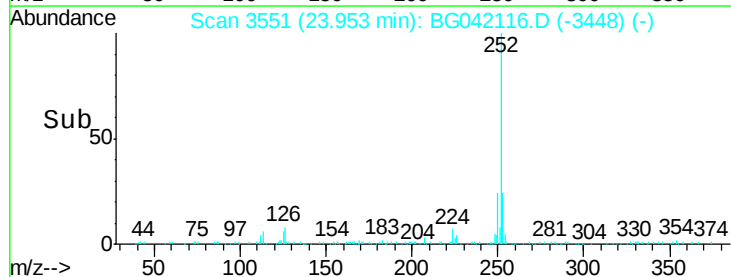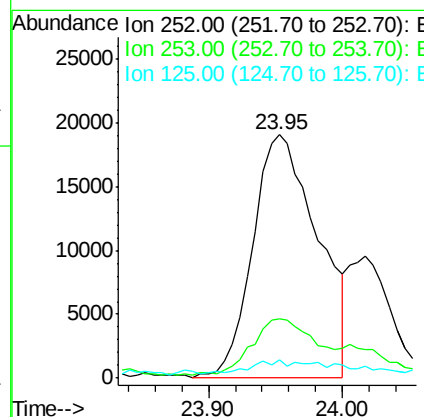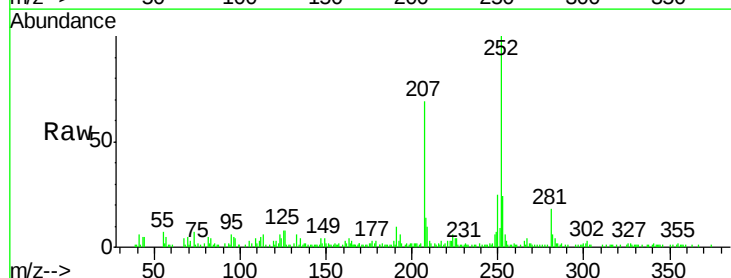

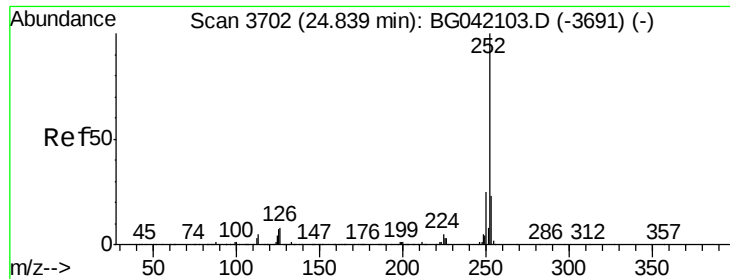





#90
Benzo(a)pyrene
Concen: 1.319 ng/ul
RT: 24.83 min Scan# 3701
Delta R.T. 0.00 min
Lab File: BG042116.D
Acq: 10 Aug 2019 00:01

Instrument :
BNA_G
ClientSampleId :
BENT5

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.8	18.3	27.5
125	6.5	6.5	9.7

Manual Integrations
APPROVED

Sohil
8/13/2019 8:19:25 AM

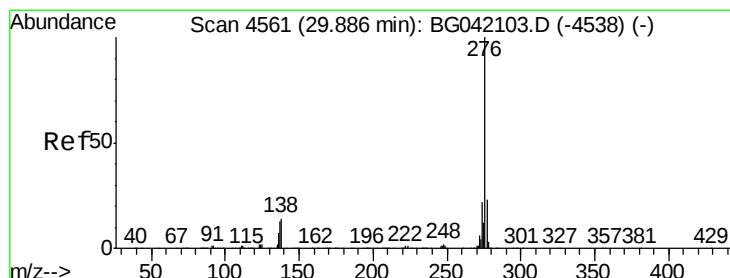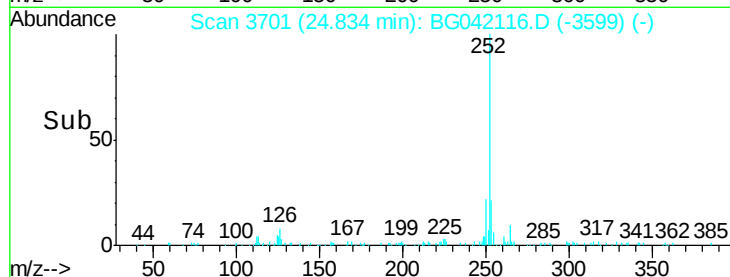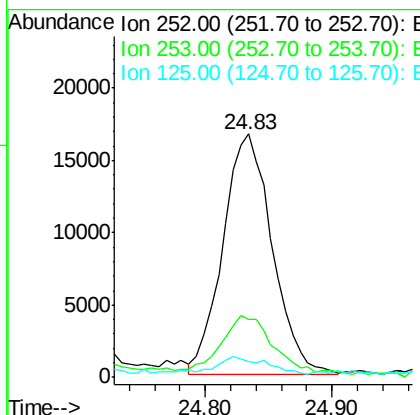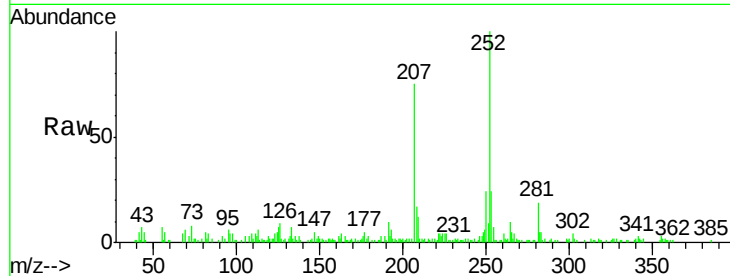

#93
Benzo(g,h,i)perylene
Concen: 1.033 ng/ul m
RT: 29.87 min Scan# 4558
Delta R.T. -0.02 min
Lab File: BG042116.D
Acq: 10 Aug 2019 00:01

Tgt Ion	Ratio	Lower	Upper
276	100		
138	14.1	12.6	18.8
277	25.1	19.2	28.8

