

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080822\
 Data File : BG054548.D
 Acq On : 8 Aug 2022 11:10
 Operator : CG/JU
 Sample : PB146797BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB146797BL

Quant Time: Aug 08 14:51:15 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 08 14:48:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.973	152	17882	20.000	ng	0.00
21) Naphthalene-d8	10.787	136	67981	20.000	ng	# 0.00
39) Acenaphthene-d10	14.618	164	54324	20.000	ng	0.00
64) Phenanthrene-d10	17.362	188	156290	20.000	ng	# 0.00
76) Chrysene-d12	21.633	240	194928	20.000	ng	# 0.00
86) Perylene-d12	24.835	264	199820	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.558	112	133086	155.390	ng	0.00
7) Phenol-d6	7.174	99	173726	148.032	ng	0.00
23) Nitrobenzene-d5	9.142	82	118370	94.822	ng	0.00
42) 2,4,6-Tribromophenol	16.116	330	148786	130.445	ng	0.00
45) 2-Fluorobiphenyl	13.237	172	351686	91.326	ng	0.00
79) Terphenyl-d14	19.976	244	973520	99.076	ng	0.00


Target Compounds Qvalue


 (#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080822\
Data File : BG054548.D
Acq On : 8 Aug 2022 11:10
Operator : CG/JU
Sample : PB146797BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB146797BL

Quant Time: Aug 08 14:51:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 08 14:48:51 2022
Response via : Initial Calibration




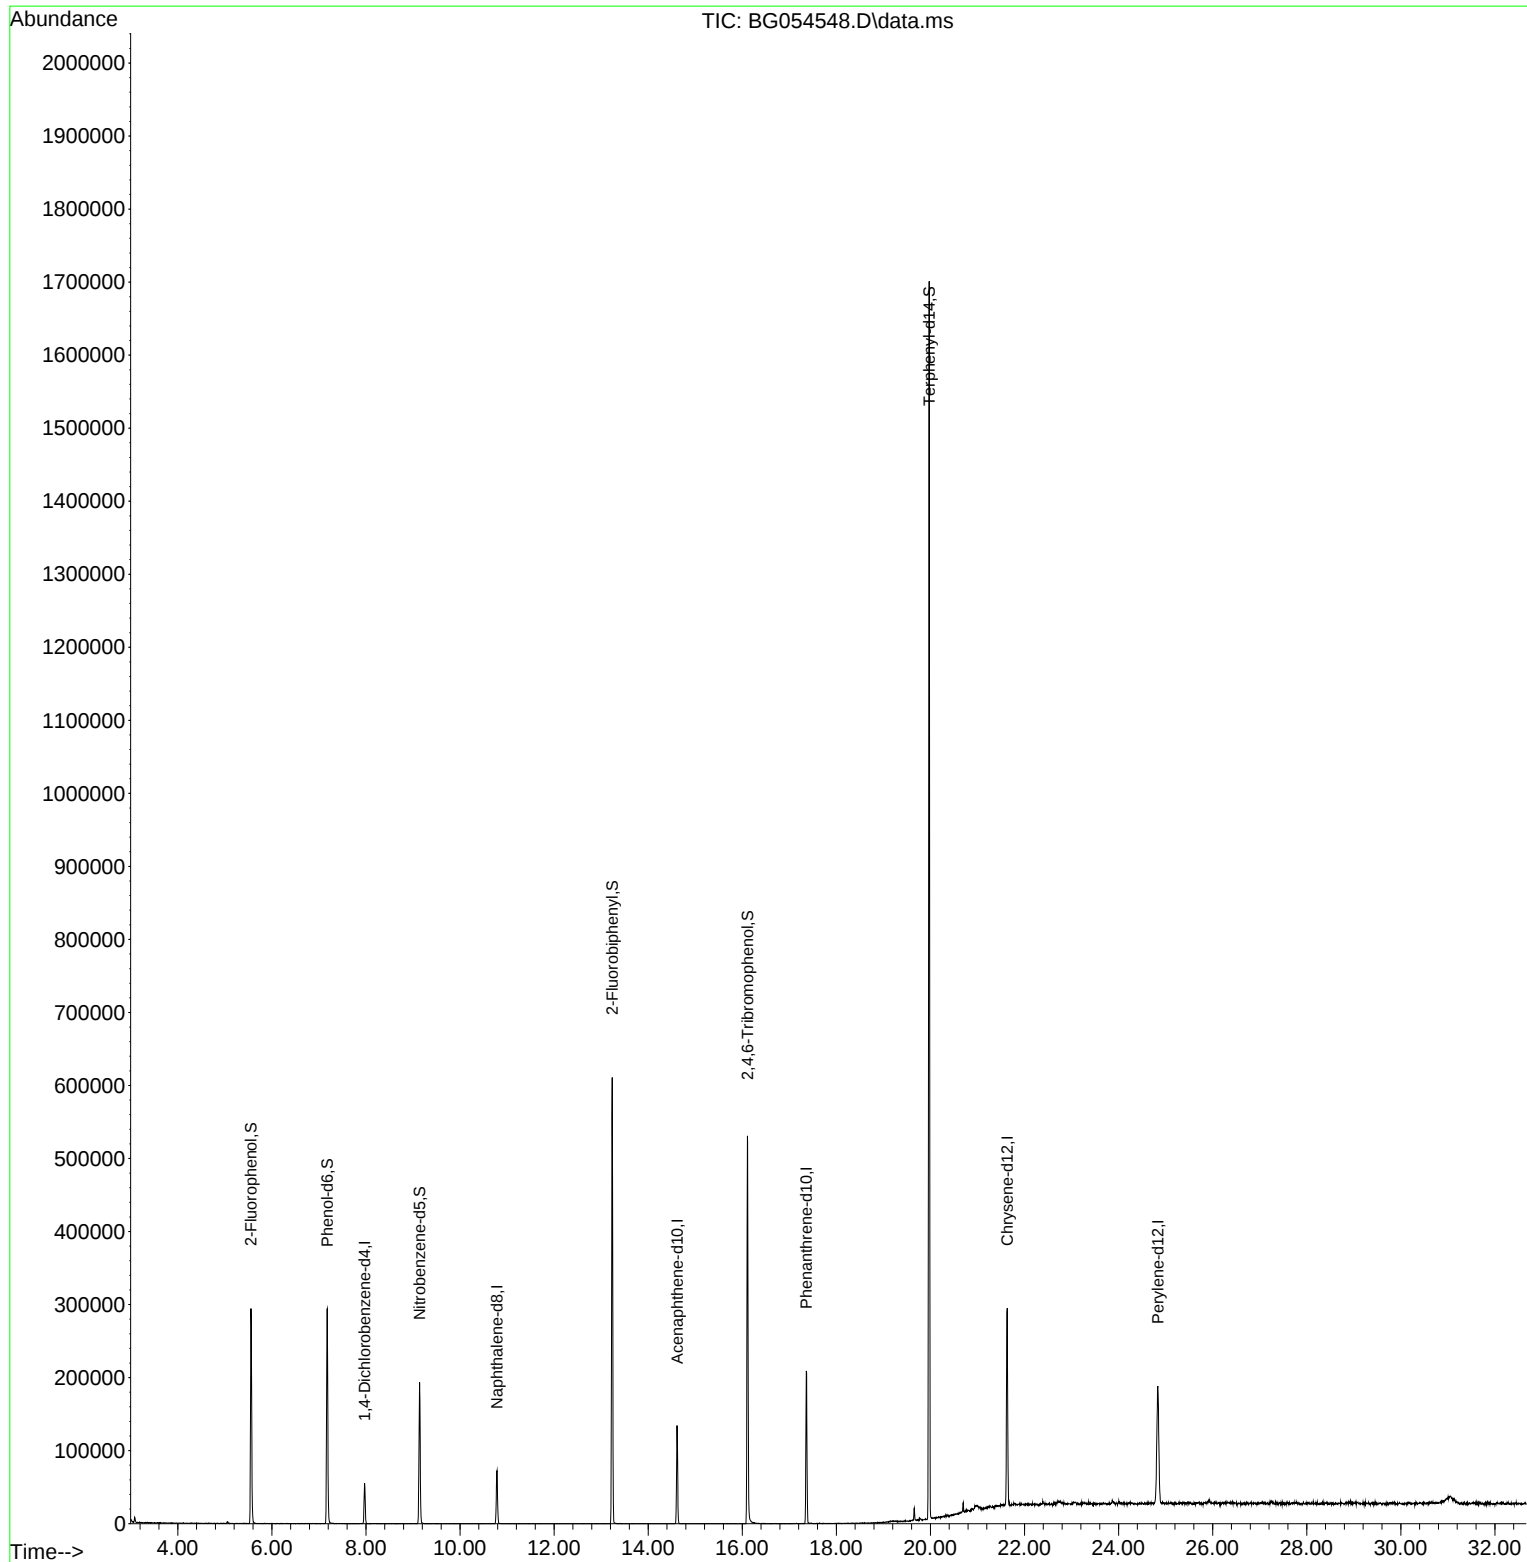


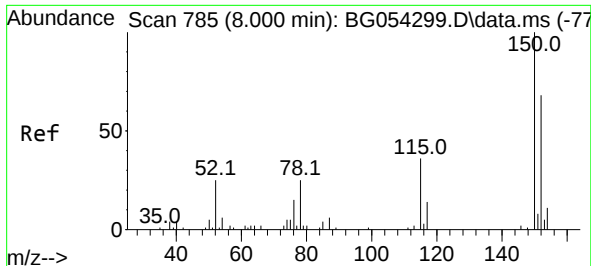

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.973 min Scan# 84
 Delta R.T. 0.001 min
 Lab File: BG054548.D
 Acq: 8 Aug 2022 11:10




Instrument :
 BNA_G
 ClientSampleId :
 PB146797BL


Tgt Ion:152 Resp: 17882
 Ion Ratio Lower Upper
 152 100
 150 141.4 131.6 197.4
 115 54.4 50.9 76.3

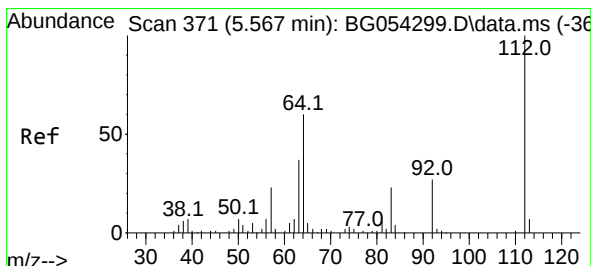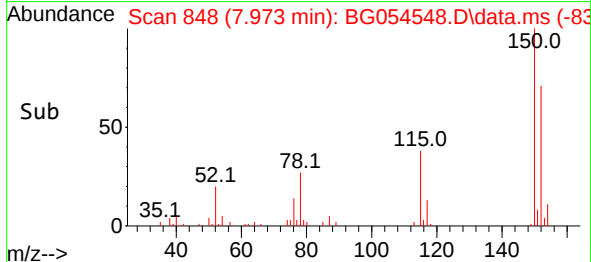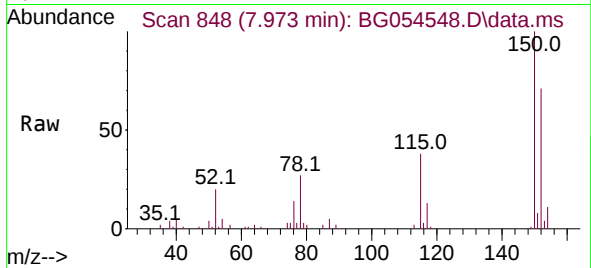

#5
 2-Fluorophenol
 Concen: 155.390 ng
 RT: 5.558 min Scan# 437
 Delta R.T. -0.006 min
 Lab File: BG054548.D
 Acq: 8 Aug 2022 11:10

Tgt Ion:112 Resp: 133086
 Ion Ratio Lower Upper
 112 100
 64 59.7 55.1 82.7
 63 35.0 30.4 45.6


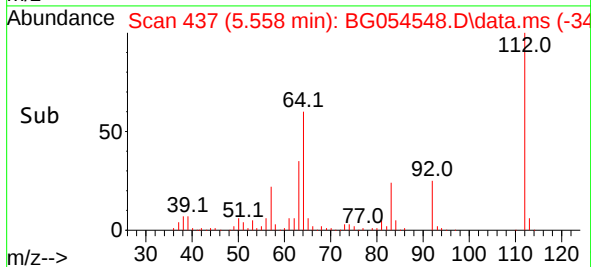

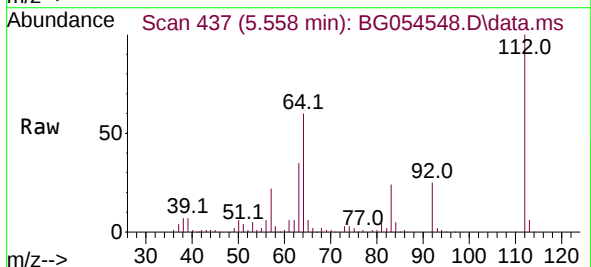


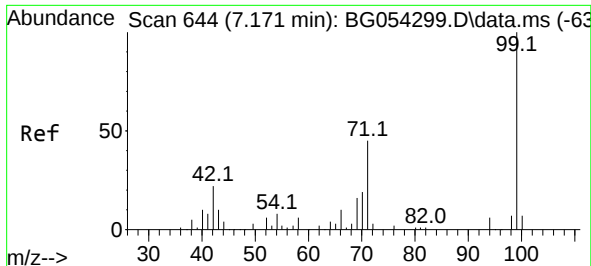

#7
Phenol-d6
Concen: 148.032 ng
RT: 7.174 min Scan# 71
Delta R.T. -0.006 min
Lab File: BG054548.D
Acq: 8 Aug 2022 11:10




Instrument :
BNA_G
ClientSampleId :
PB146797BL

Tgt Ion: 99 Resp: 173726
Ion Ratio Lower Upper
99 100
42 20.6 17.0 25.6
71 44.6 33.8 50.8

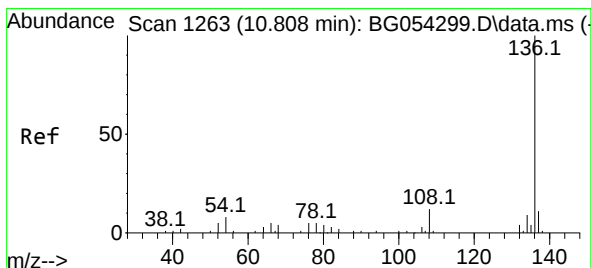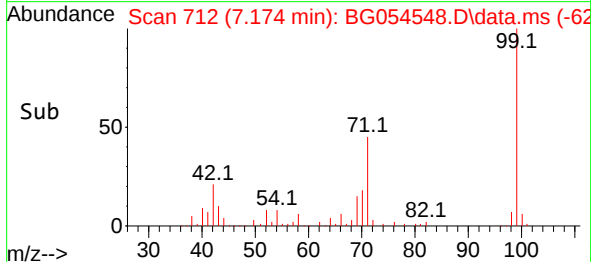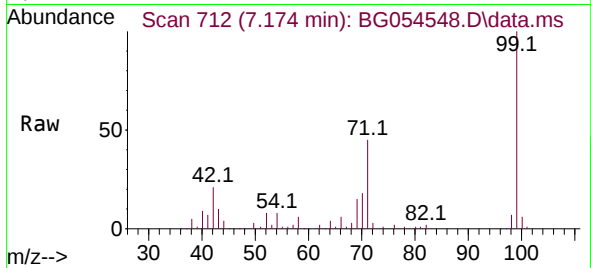

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.787 min Scan# 1327
Delta R.T. 0.000 min
Lab File: BG054548.D
Acq: 8 Aug 2022 11:10

Tgt Ion: 136 Resp: 67981
Ion Ratio Lower Upper
136 100
137 11.5 8.5 12.7
54 6.2 7.4 11.2#
68 3.7 4.9 7.3#


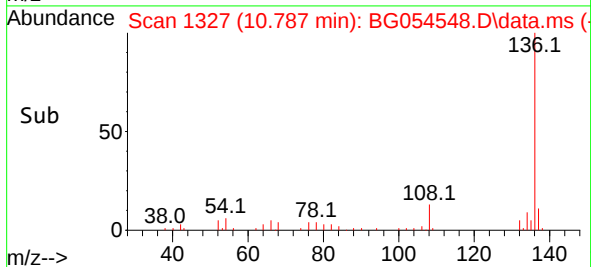

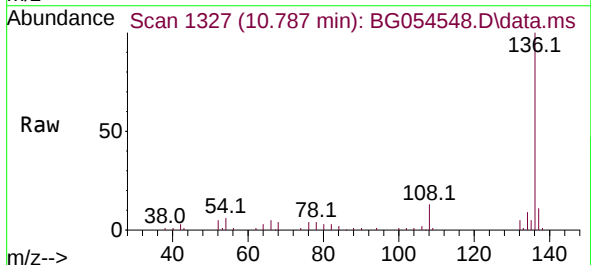




#23
Nitrobenzene-d5
Concen: 94.822 ng
RT: 9.142 min Scan# 10
Delta R.T. 0.000 min
Lab File: BG054548.D
Acq: 8 Aug 2022 11:10




Instrument :
BNA_G
ClientSampleId :
PB146797BL


Tgt Ion: 82 Resp: 118370
Ion Ratio Lower Upper
82 100
128 41.1 27.9 41.9
54 55.1 41.2 61.8

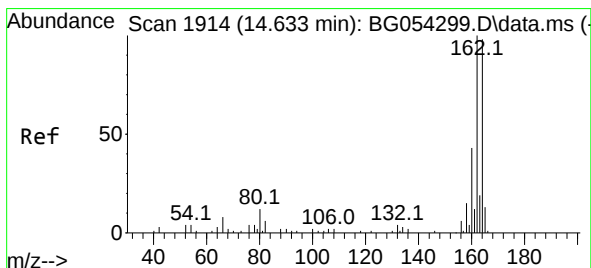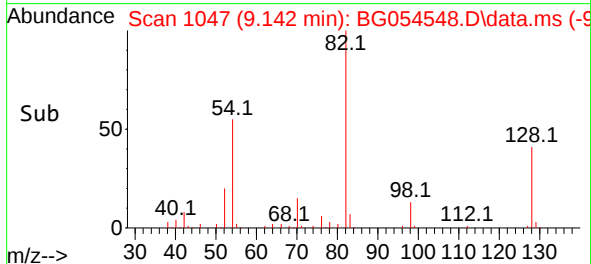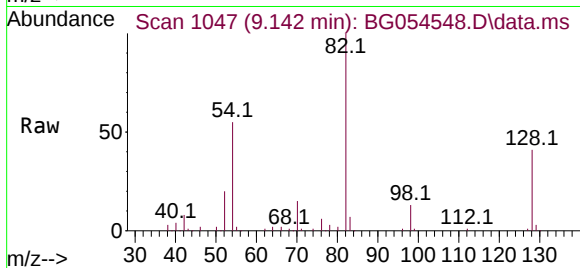

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.618 min Scan# 1979
Delta R.T. 0.000 min
Lab File: BG054548.D
Acq: 8 Aug 2022 11:10

Tgt Ion:164 Resp: 54324
Ion Ratio Lower Upper
164 100
162 103.2 82.3 123.5
160 44.3 34.2 51.2


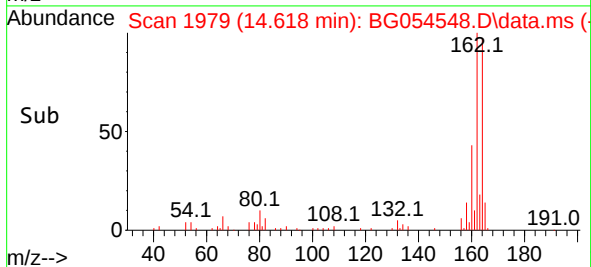

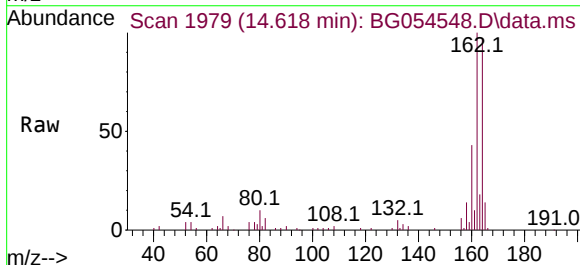


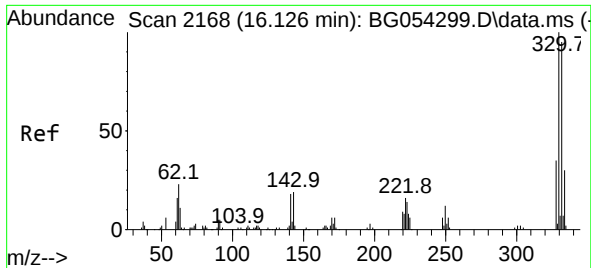

#42
 2,4,6-Tribromophenol
 Concen: 130.445 ng
 RT: 16.116 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BG054548.D
 Acq: 8 Aug 2022 11:10




Instrument :
 BNA_G
 ClientSampleId :
 PB146797BL


Tgt Ion:330 Resp: 148786
 Ion Ratio Lower Upper
 330 100
 332 96.4 76.0 114.0
 141 21.1 27.1 40.7#

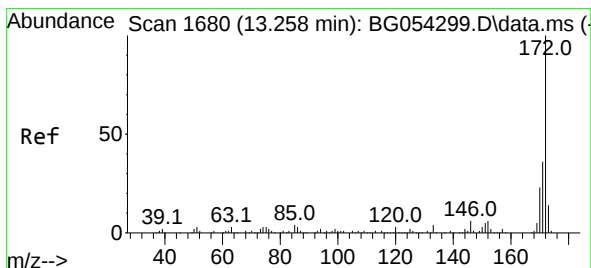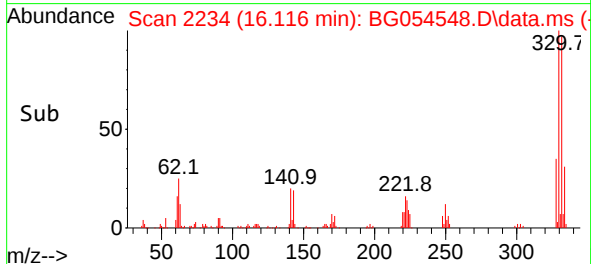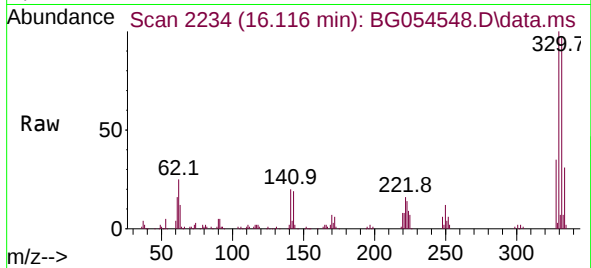

#45
 2-Fluorobiphenyl
 Concen: 91.326 ng
 RT: 13.237 min Scan# 1744
 Delta R.T. 0.000 min
 Lab File: BG054548.D
 Acq: 8 Aug 2022 11:10

Tgt Ion:172 Resp: 351686
 Ion Ratio Lower Upper
 172 100
 171 36.2 28.5 42.7
 170 24.3 18.9 28.3


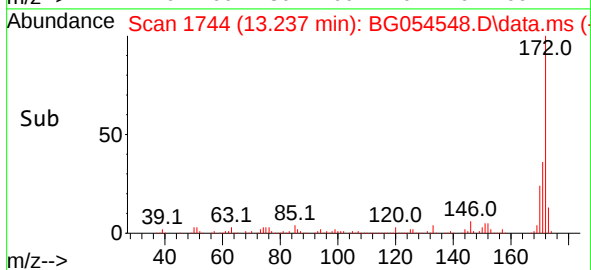

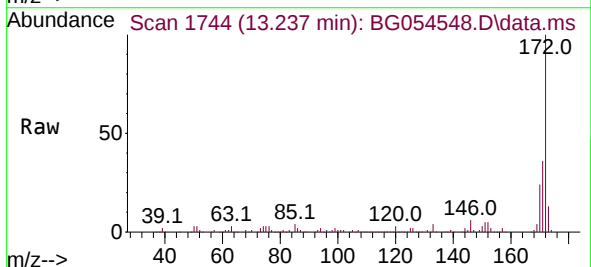


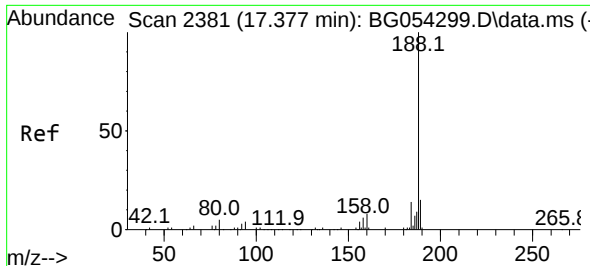

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.362 min Scan# 24
Delta R.T. 0.000 min
Lab File: BG054548.D
Acq: 8 Aug 2022 11:10




Instrument :
BNA_G
ClientSampleId :
PB146797BL


Tgt Ion:188 Resp: 156290
Ion Ratio Lower Upper
188 100
94 4.2 5.4 8.0#
80 4.8 6.8 10.2#

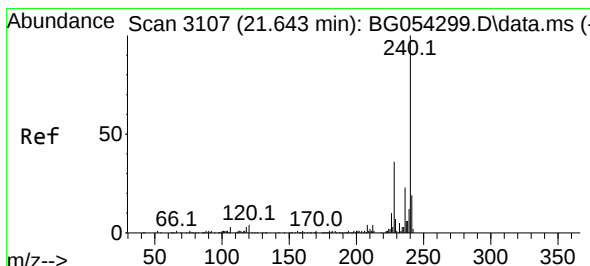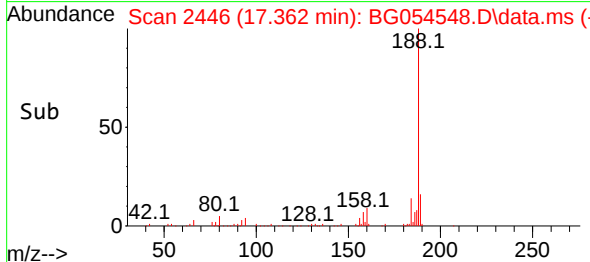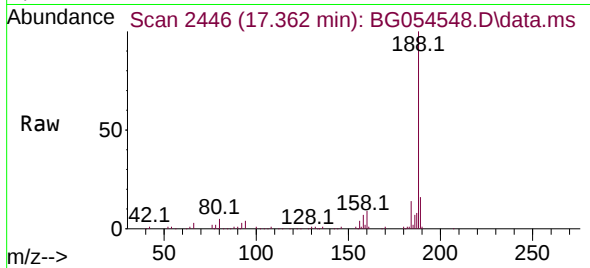

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.633 min Scan# 3173
Delta R.T. 0.000 min
Lab File: BG054548.D
Acq: 8 Aug 2022 11:10

Tgt Ion:240 Resp: 194928
Ion Ratio Lower Upper
240 100
120 4.3 4.6 7.0#
236 24.9 20.2 30.4


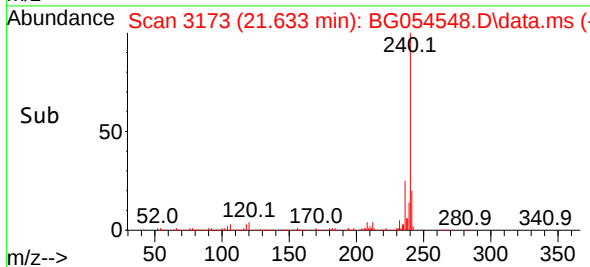

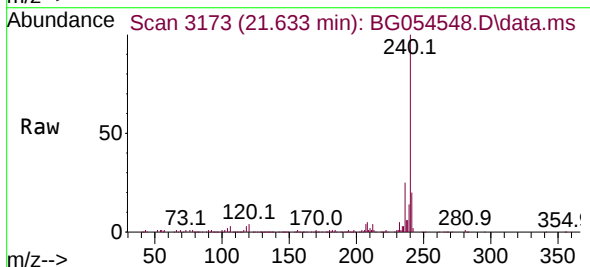


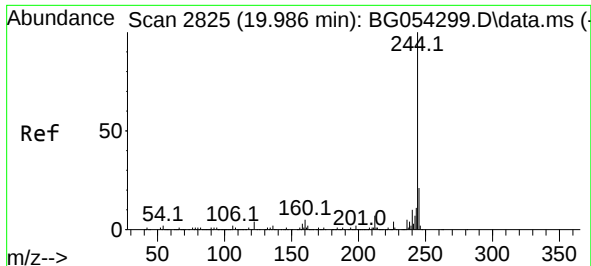

#79
 Terphenyl-d14
 Concen: 99.076 ng
 RT: 19.976 min Scan# 2825
 Delta R.T. 0.006 min
 Lab File: BG054548.D
 Acq: 8 Aug 2022 11:10

Instrument :
 BNA_G
 ClientSampleId :
 PB146797BL

Tgt Ion:244 Resp: 973520
 Ion Ratio Lower Upper
 244 100
 212 7.3 6.5 9.7
 122 4.8 5.0 7.4#

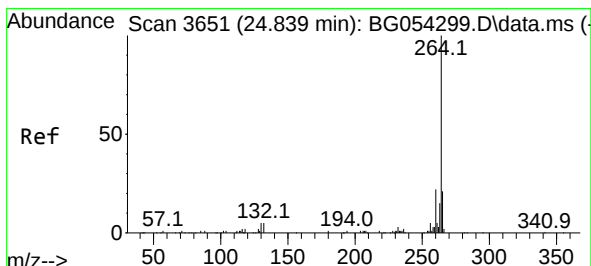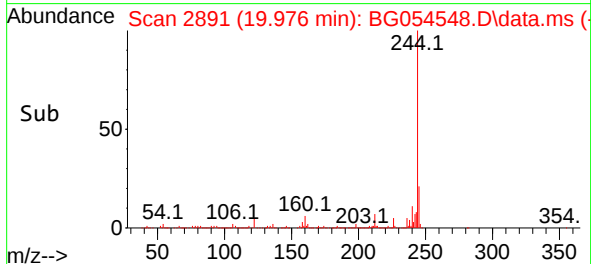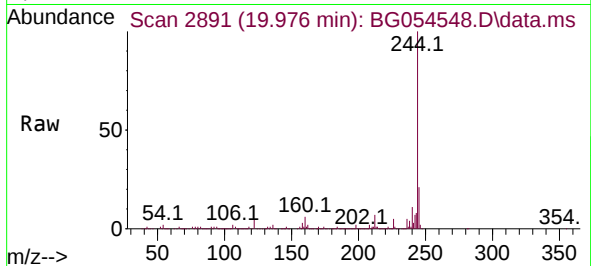

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.835 min Scan# 3718
 Delta R.T. 0.000 min
 Lab File: BG054548.D
 Acq: 8 Aug 2022 11:10

Tgt Ion:264 Resp: 199820
 Ion Ratio Lower Upper
 264 100
 260 23.4 19.0 28.6
 265 22.6 17.4 26.2

