


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080822\
Data File : BG054546.D
Acq On : 8 Aug 2022 9:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 08 14:48:51 2022

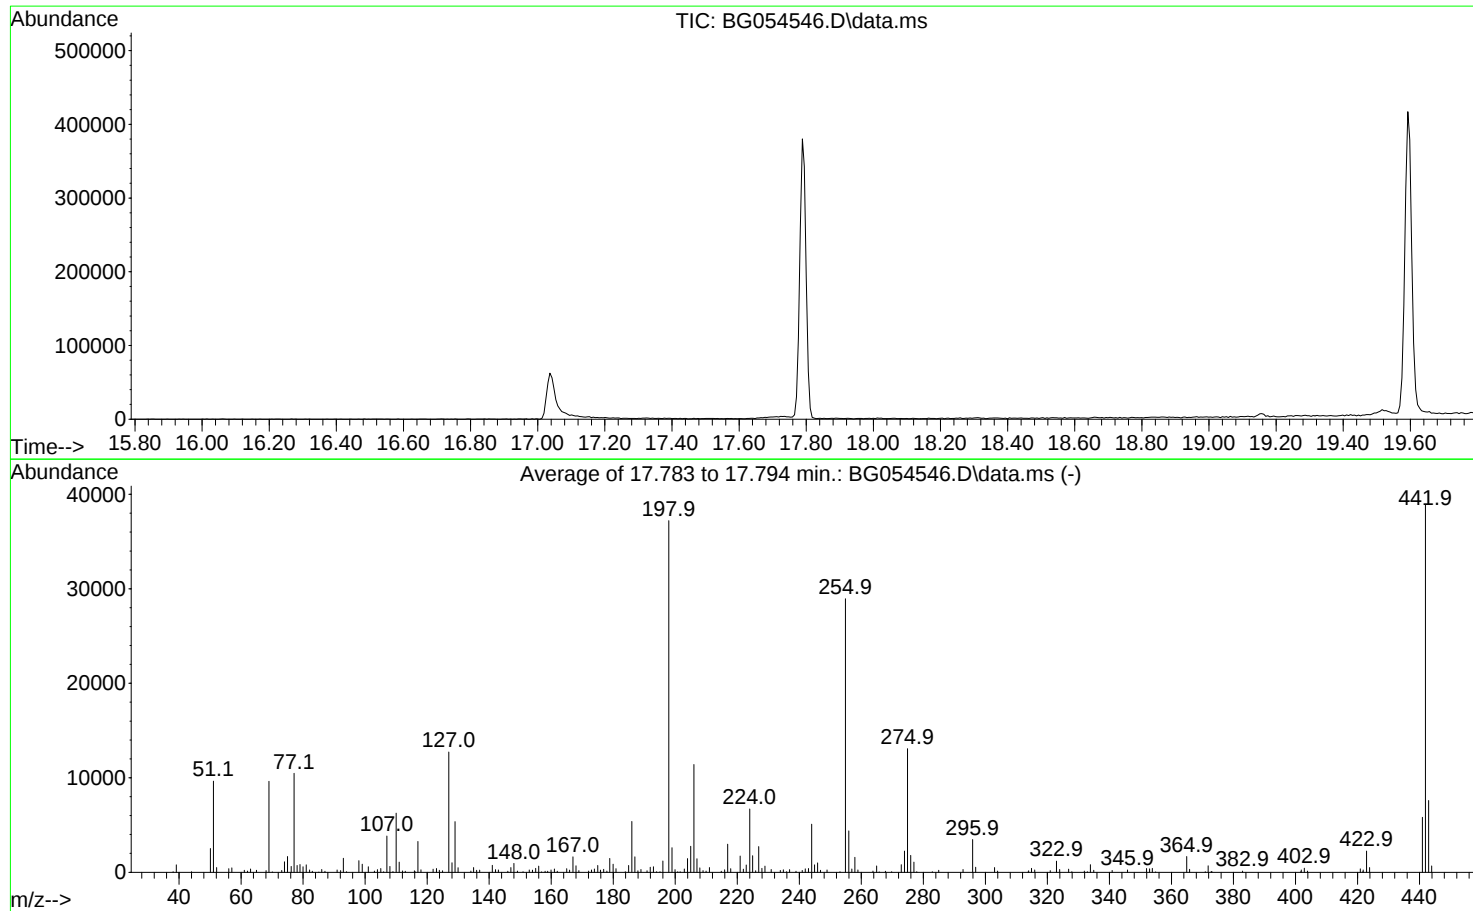




AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.9	9642	PASS
68	69	0.00	2	1.8	174	PASS
69	198	0.00	100	25.9	9631	PASS
70	69	0.00	2	0.5	51	PASS
127	198	10	80	34.2	12724	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	37213	PASS
199	198	5	9	7.0	2607	PASS
275	198	10	60	35.1	13080	PASS
365	198	1	100	4.5	1670	PASS
441	198	0.01	100	15.7	5825	PASS
442	442	50	100	100.0	38928	PASS
443	442	15	24	19.5	7603	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080822\
Data File : BG054546.D
Acq On : 8 Aug 2022 9:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 09 07:15:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 08 14:48:51 2022
Response via : Initial Calibration

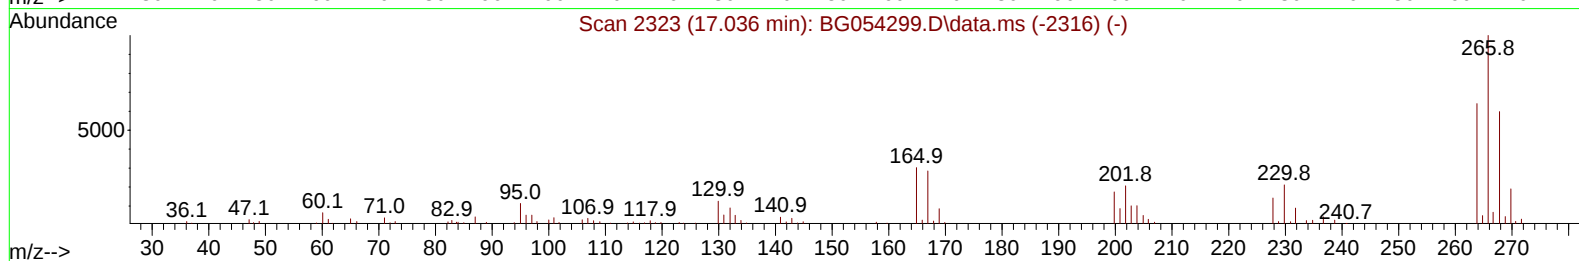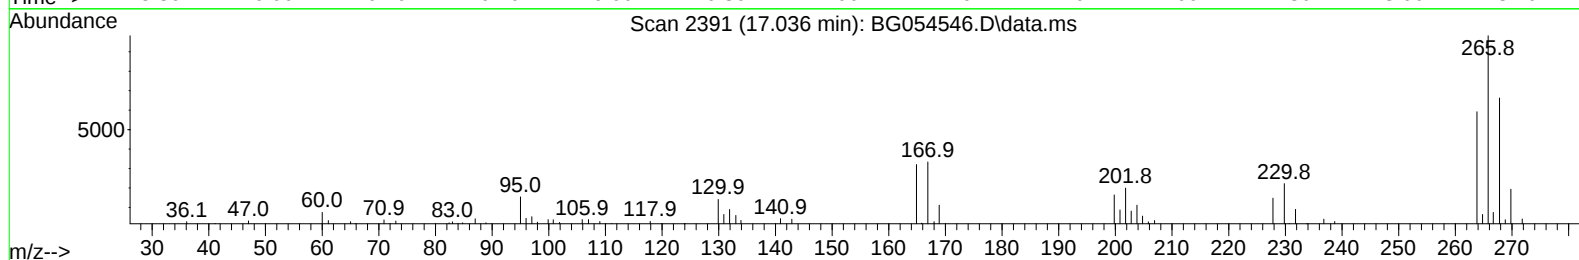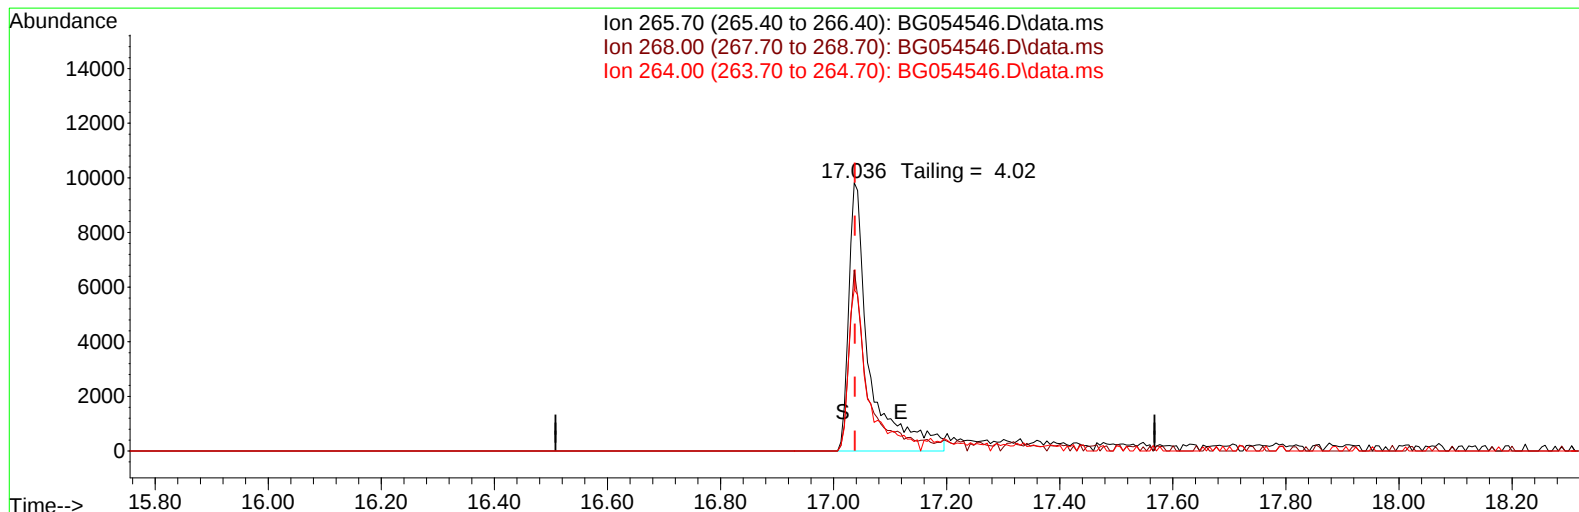

TIC: BG054546.D\data.ms

(70) Pentachlorophenol (C)

17.036min (-0.002) 18919.76 ng




response 23928

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	67.39
264.00	66.20	60.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080822\
Data File : BG054546.D
Acq On : 8 Aug 2022 9:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 09 07:15:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 08 14:48:51 2022
Response via : Initial Calibration

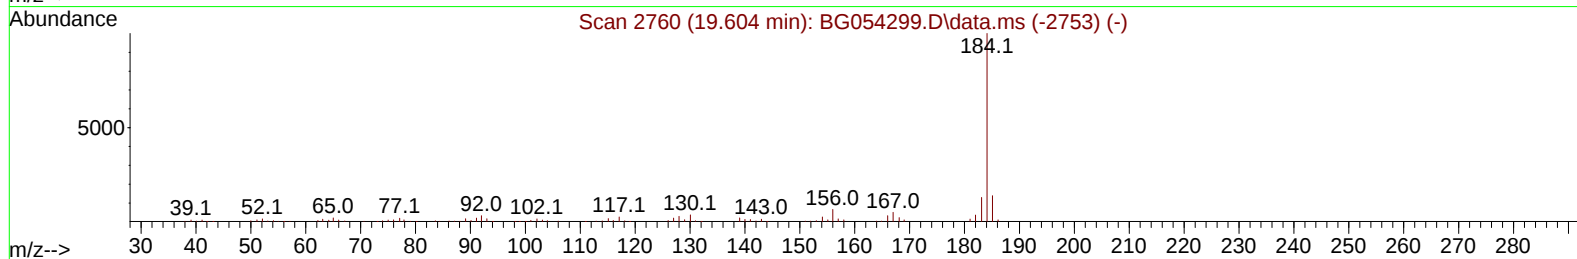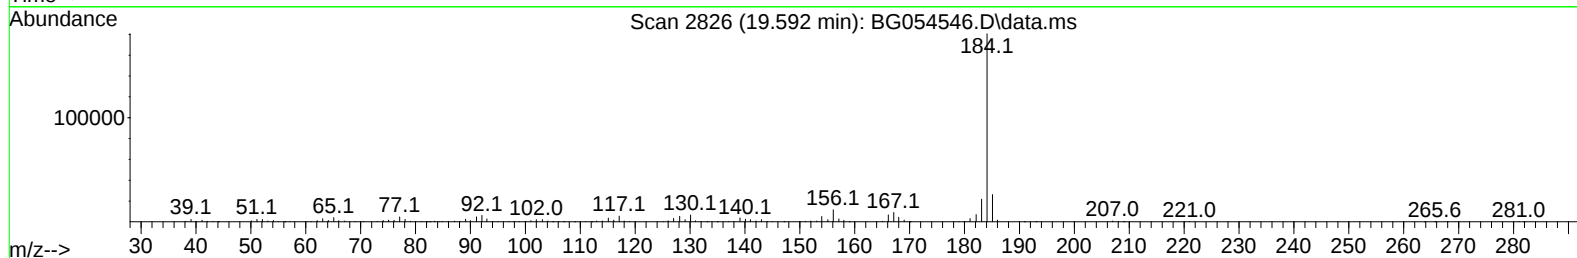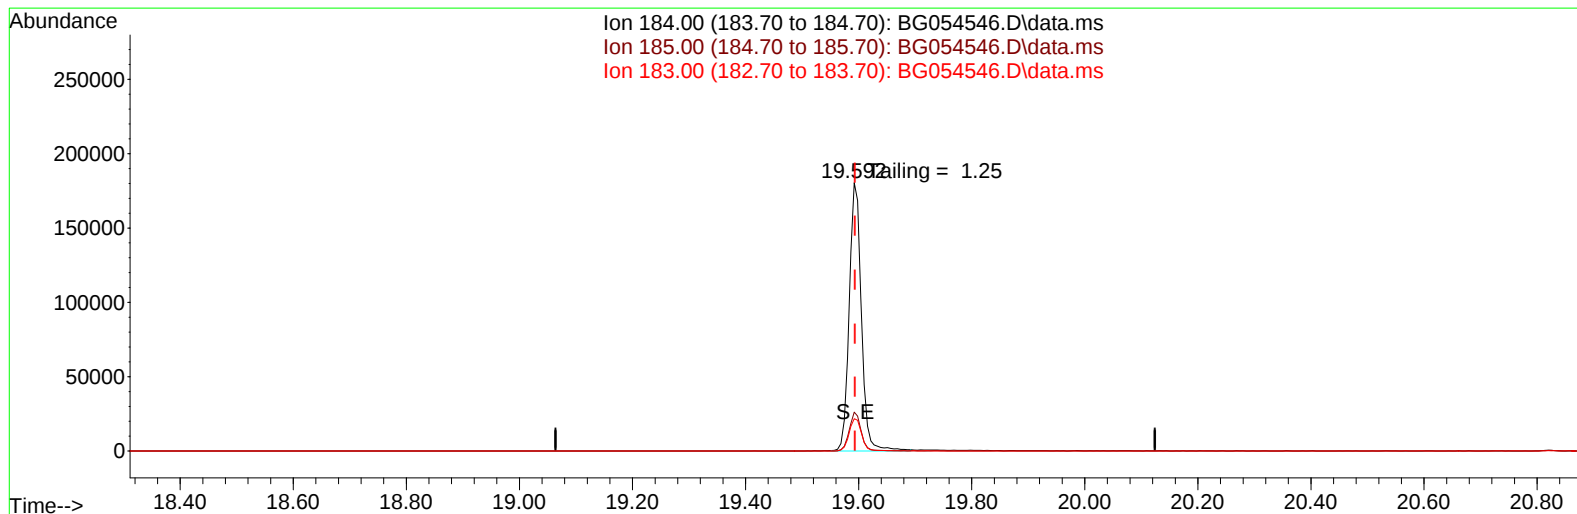

TIC: BG054546.D\data.ms

(77) Benzidine

19.592min (-0.002) 0.00 ng

response 269508

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.53
183.00	11.10	12.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/8/2022	BNA_G	BG054546.D
Compound Name	Response	Retention Time
DDT	143417	20.82
DDD	8743	20.385
DDE	387	19.874
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9130	152547	5.99

Instrument :
BNA_G
ClientSampleId :
DFTPP