


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080823\
Data File : BG058633.D
Acq On : 8 Aug 2023 8:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 28 22:29:07 2023

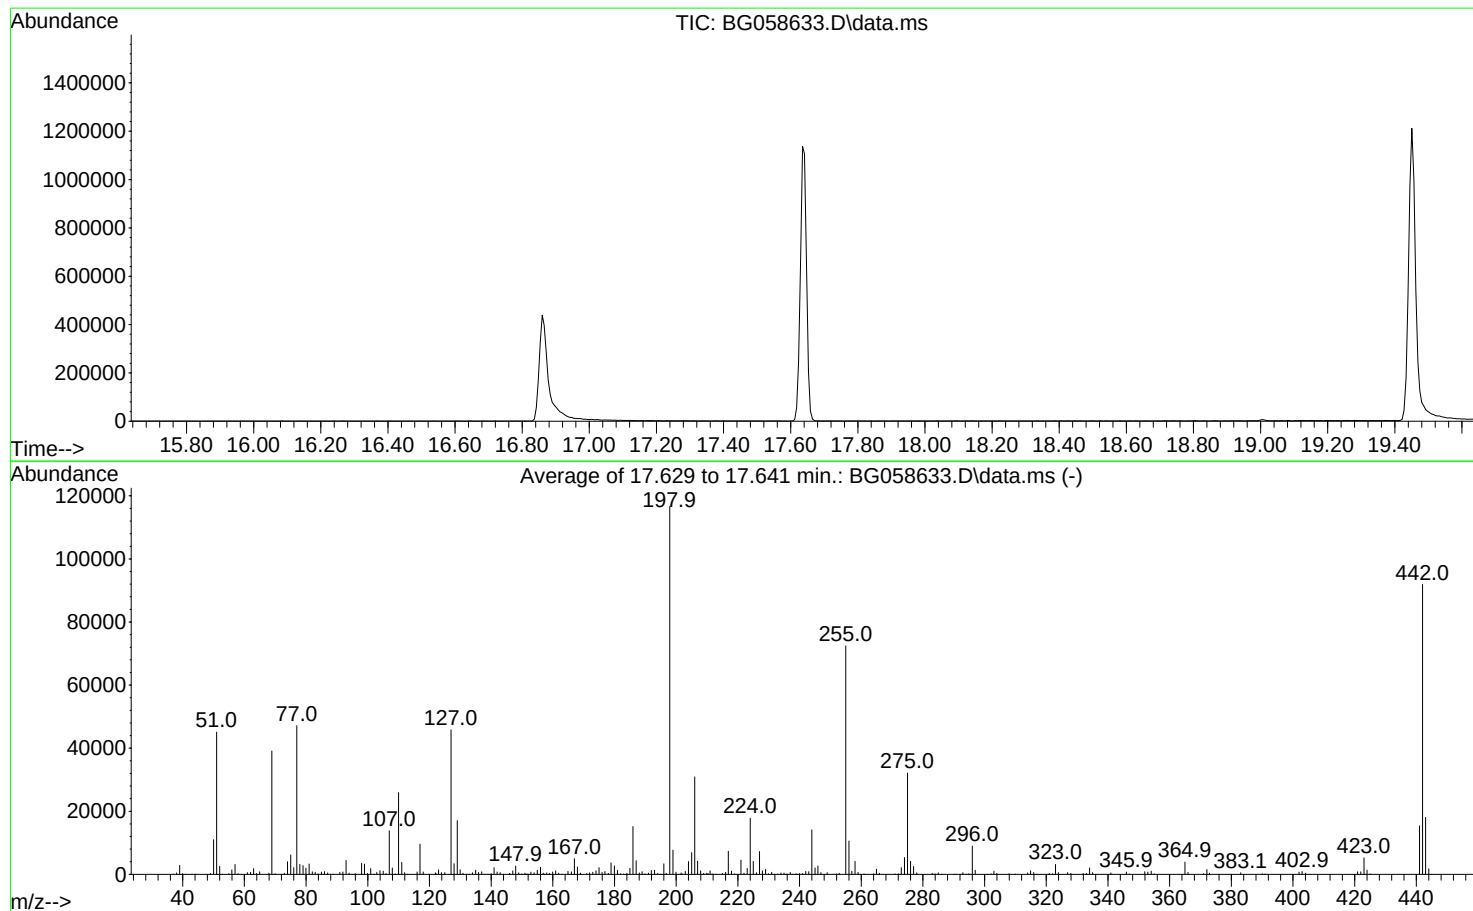




Spectrum Information: Average of 17.629 to 17.641 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	45101	PASS
68	69	0.00	2	1.0	391	PASS
69	198	0.00	100	33.5	39104	PASS
70	69	0.00	2	0.6	229	PASS
127	198	10	80	39.3	45787	PASS
197	198	0.00	2	0.3	343	PASS
198	198	100	100	100.0	116616	PASS
199	198	5	9	6.6	7708	PASS
275	198	10	60	27.5	32117	PASS
365	198	1	100	3.4	3933	PASS
441	198	0.01	100	13.2	15362	PASS
442	442	50	100	100.0	91893	PASS
443	442	15	24	19.7	18086	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080823\
Data File : BG058633.D
Acq On : 8 Aug 2023 8:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 08 10:47:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

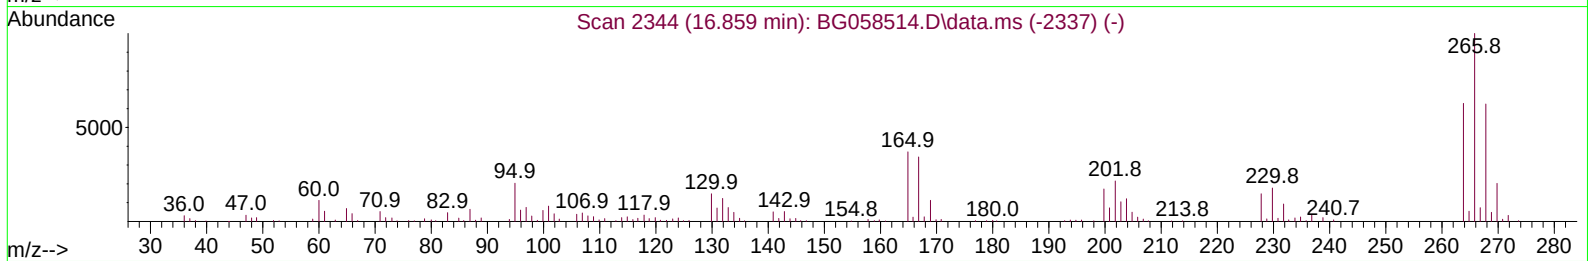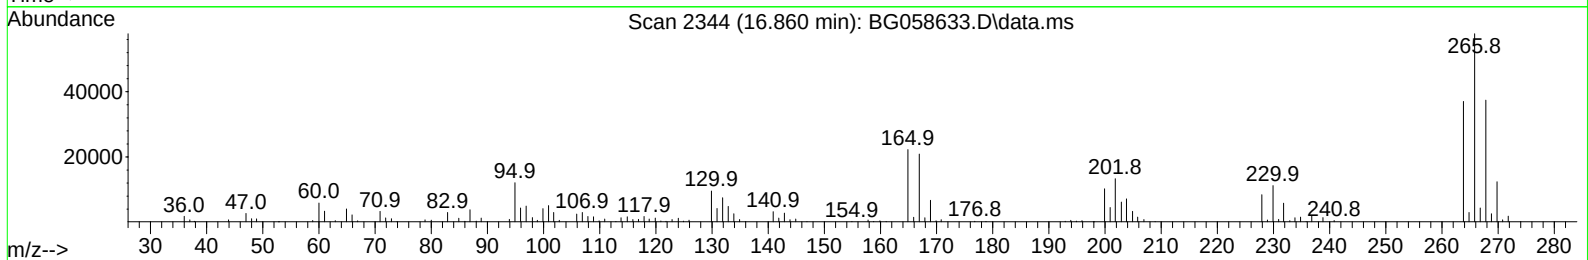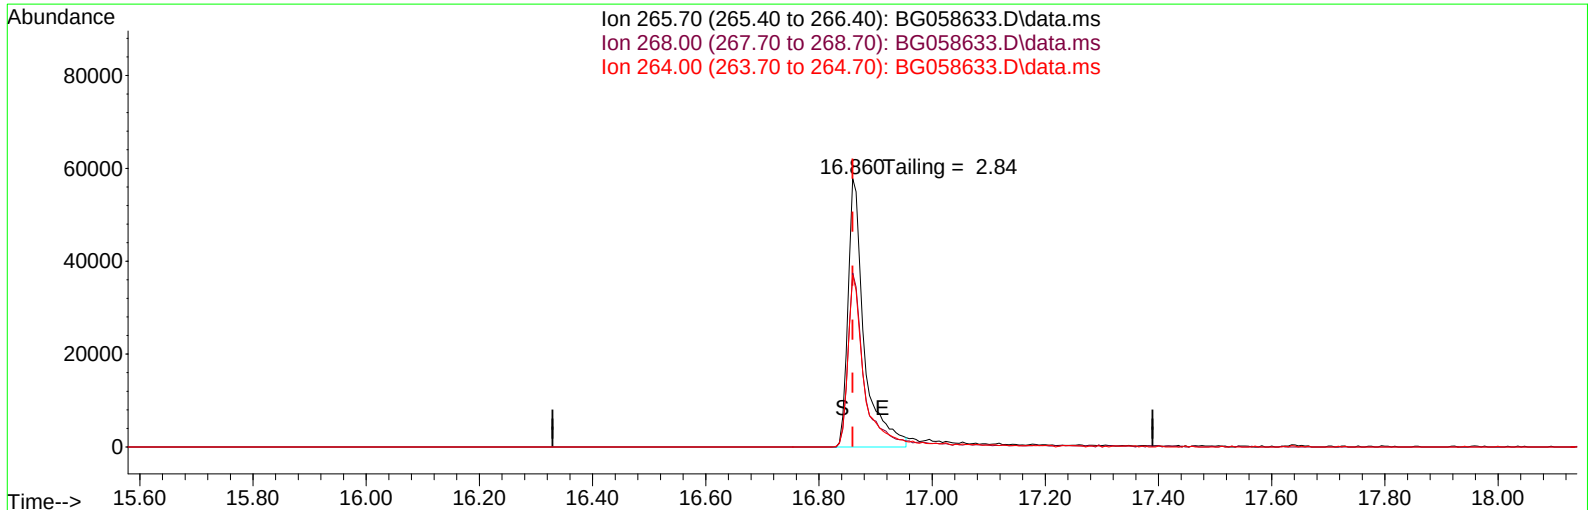

TIC: BG058633.D\data.ms

(70) Pentachlorophenol (C)

16.860min (+ 0.001) 27830.06 ng




response 117019

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	64.77
264.00	62.80	64.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080823\
Data File : BG058633.D
Acq On : 8 Aug 2023 8:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 08 10:47:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

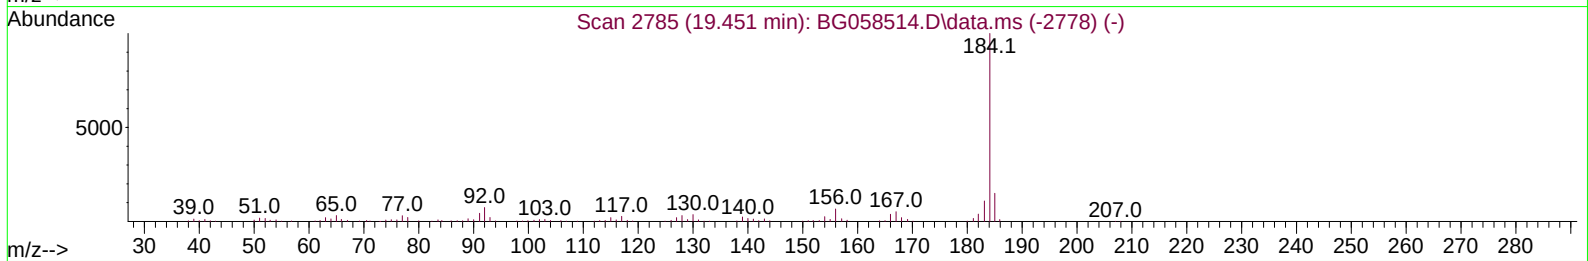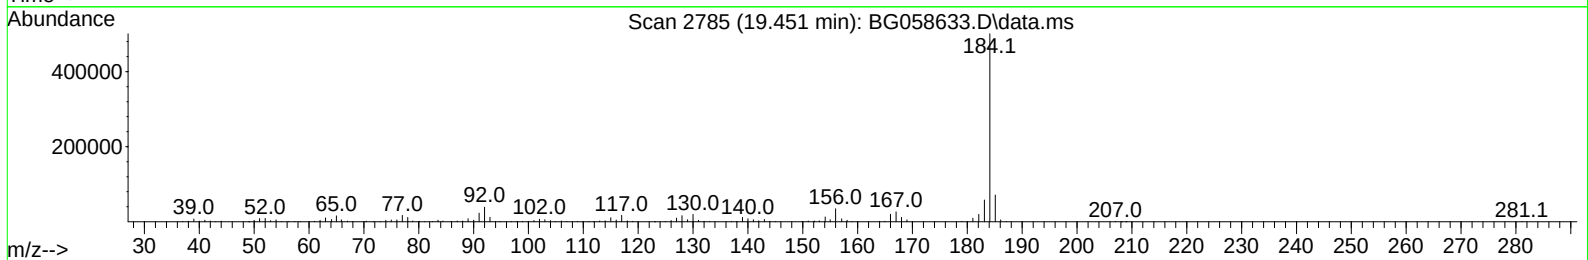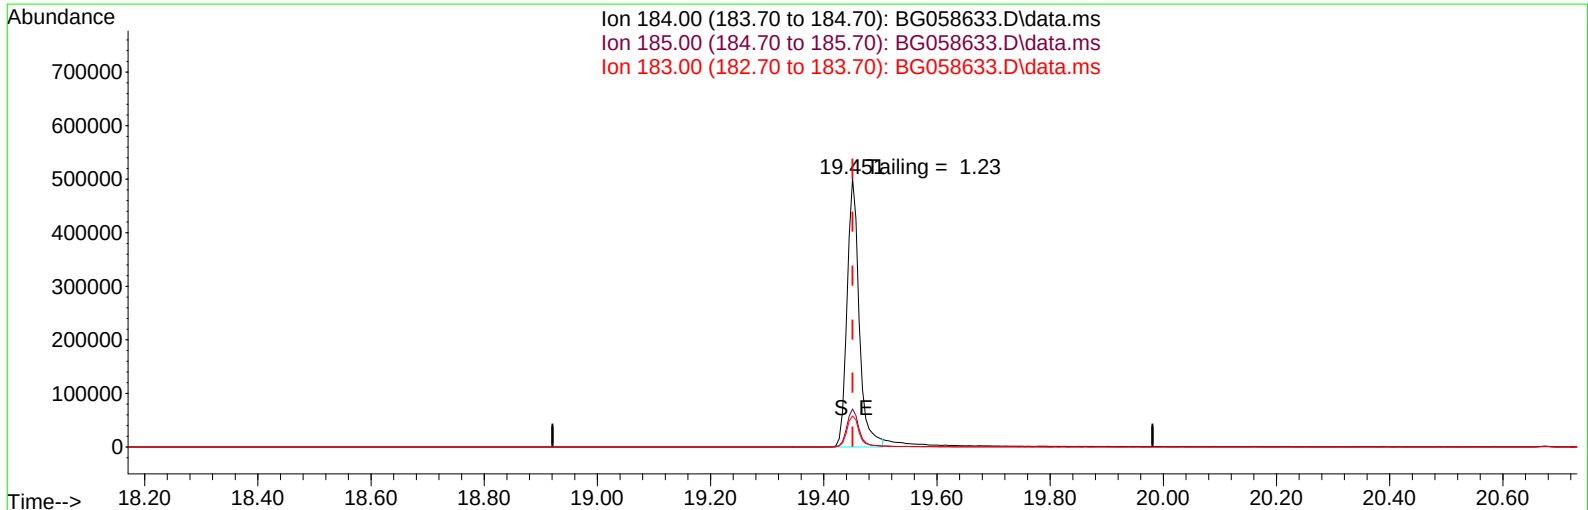

TIC: BG058633.D\data.ms

(77) Benzidine

19.451min (+ 0.000) 0.00 ng

response 786662

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.18
183.00	10.90	11.53
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/8/2023	BNA_G	<u>BG058633.D</u>
Compound Name	Response	Retention Time
DDT	397979	20.673
DDD	12210	20.238
DDE	2837	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15047	413026	3.64

Instrument :
BNA_G
ClientSampleId :
DFTPP