




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
 Data File : BG062321.D
 Acq On : 8 Aug 2024 5:53
 Operator : MA/JU
 Sample : P3437-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E05W7

Manual IntegrationsAPPROVED

Quant Time: Aug 08 06:31:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 07 01:46:39 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/09/2024
 Supervised By :mohammad ahmed 08/12/2024

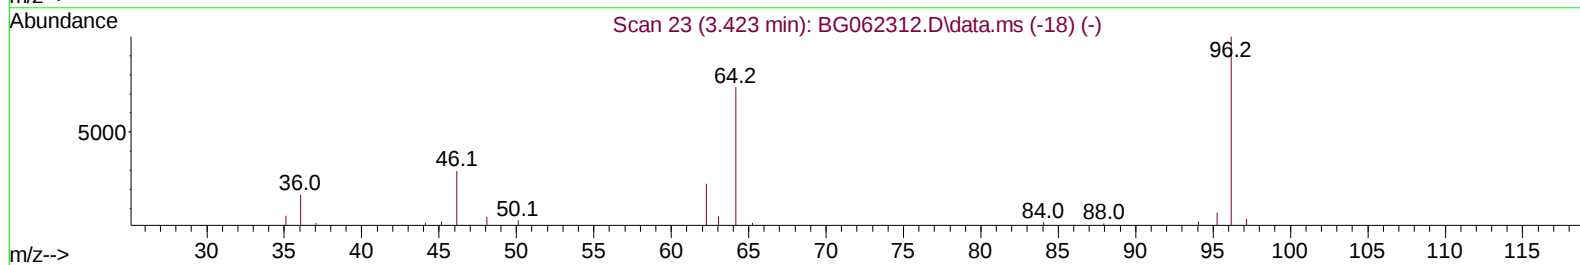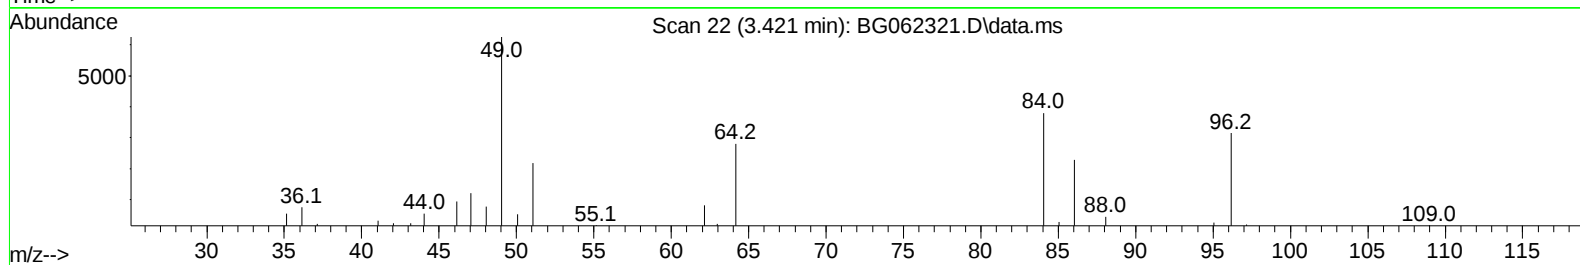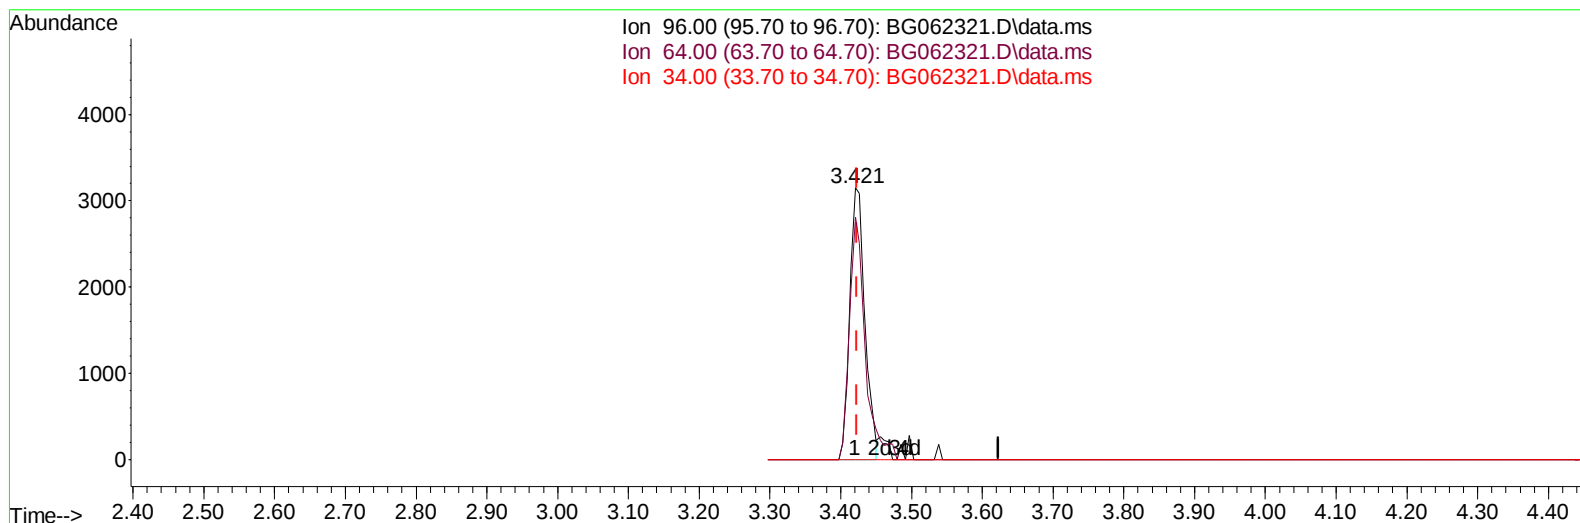

TIC: BG062321.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.421min (-0.002) 3.02 ng/uL

response 4676

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	84.50	89.20
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062321.D
Acq On : 8 Aug 2024 5:53
Operator : MA/JU
Sample : P3437-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E05W7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/09/2024
Supervised By :mohammad ahmed 08/12/2024

Quant Time: Aug 08 06:31:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 07 01:46:39 2024
Response via : Initial Calibration

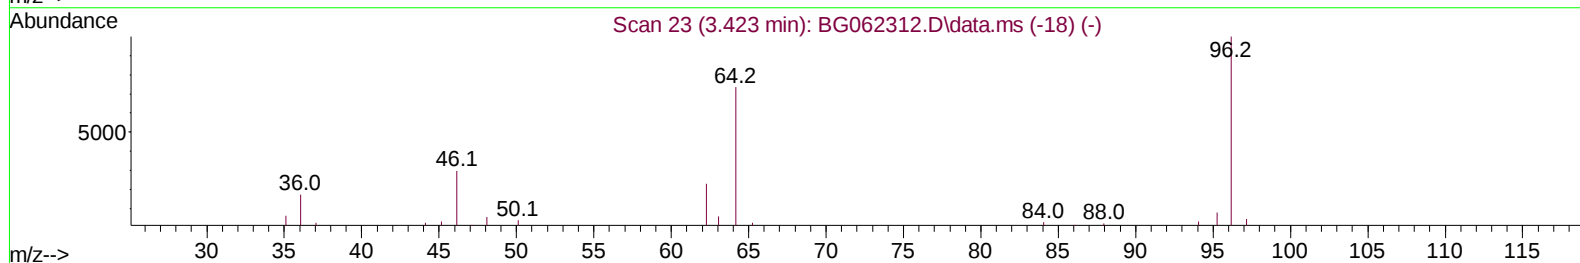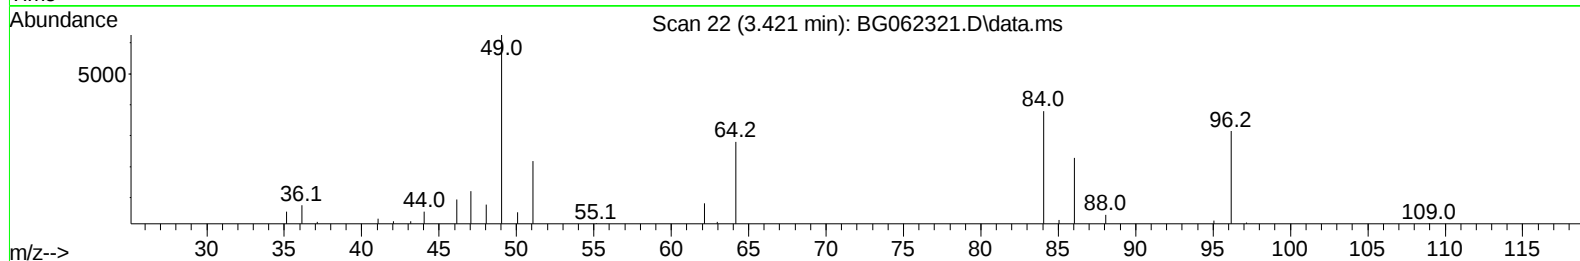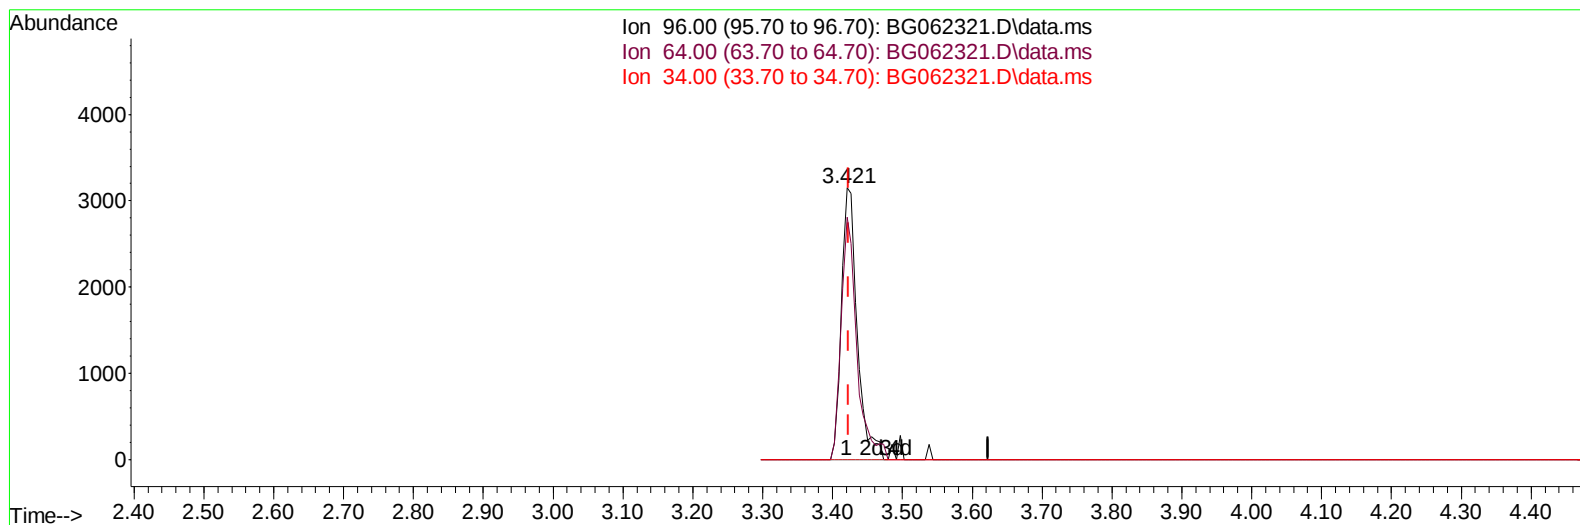

TIC: BG062321.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.421min (-0.002) 3.18 ng/uL m

response 4918

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	84.50	89.20
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
 Data File : BG062321.D
 Acq On : 8 Aug 2024 5:53
 Operator : MA/JU
 Sample : P3437-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E05W7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/09/2024
 Supervised By :mohammad ahmed 08/12/2024

Quant Time: Aug 08 06:33:46 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 07 01:46:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.956	152	66749	20.000	ng/ul	0.00
20) Naphthalene-d8	10.752	136	308939	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.576	164	242338	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.314	188	512665	20.000	ng/ul	0.00
79) Chrysene-d12	21.555	240	496541	20.000	ng/ul	0.00
88) Perylene-d12	24.639	264	572188	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.421	96	4918m	3.177	ng/uL	0.00
4) Pyridine-d5	3.826	84	36719	7.540	ng/ul	0.00
7) Phenol-d5	7.110	99	39598	6.215	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.286	67	50265	12.817	ng/ul	0.00
11) 2-Chlorophenol-d4	7.486	132	63892	13.997	ng/ul	0.00
15) 4-Methylphenol-d8	8.649	113	61878	11.660	ng/ul	0.00
21) Nitrobenzene-d5	9.107	128	28575	15.000	ng/ul	0.00
24) 2-Nitrophenol-d4	9.830	143	31321	17.478	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.364	165	74117	14.240	ng/ul	0.00
31) 4-Chloroaniline-d4	10.875	131	137510	18.216	ng/ul	0.00
46) Dimethylphthalate-d6	13.983	166	238765	12.770	ng/ul	0.00
49) Acenaphthylene-d8	14.265	160	252320	11.902	ng/ul	0.00
54) 4-Nitrophenol-d4	14.752	143	15505	5.923	ng/ul	0.00
60) Fluorene-d10	15.563	176	209715	12.496	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.669	200	23499	15.477	ng/ul	0.00
73) Anthracene-d10	17.413	188	345512	13.973	ng/ul	0.00
81) Pyrene-d10	19.693	212	427283	14.478	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.427	264	444113	14.519	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062321.D
Acq On : 8 Aug 2024 5:53
Operator : MA/JU
Sample : P3437-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E05W7

Manual IntegrationsAPPROVED

Quant Time: Aug 08 06:33:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 07 01:46:39 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/09/2024
Supervised By :mohammad ahmed 08/12/2024

