

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
 Data File : BG062313.D
 Acq On : 8 Aug 2024 00:22
 Operator : MA/JU
 Sample : PB162446BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK446

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062313.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.420	19	22	29	rVB2	14282	21948	1.11%	0.109%
2	3.826	86	91	112	rBV	201903	357603	18.04%	1.771%
3	4.172	146	150	155	rVB4	4232	8127	0.41%	0.040%
4	7.109	643	650	663	rBV	266576	462234	23.32%	2.289%
5	7.286	673	680	689	rBV	186926	322371	16.26%	1.597%
6	7.491	707	715	729	rVB	230719	411518	20.76%	2.038%
7	7.961	788	795	807	rVB	218242	381858	19.27%	1.891%
8	8.648	903	912	925	rBV	315114	561565	28.33%	2.781%
9	9.107	983	990	1003	rVB	248474	436545	22.02%	2.162%
10	9.829	1105	1113	1121	rBV	194710	342542	17.28%	1.697%
11	10.364	1196	1204	1218	rVB	345594	603043	30.42%	2.987%
12	10.751	1262	1270	1279	rVB	347638	600893	30.32%	2.976%
13	10.875	1283	1291	1301	rBV	337494	600373	30.29%	2.974%
14	12.332	1535	1539	1545	rBV2	5557	8048	0.41%	0.040%
15	13.982	1813	1820	1828	rBV	649726	936756	47.26%	4.640%
16	14.270	1862	1869	1879	rBV	729602	1177265	59.39%	5.831%
17	14.576	1914	1921	1928	rBV	660473	993740	50.14%	4.922%
18	14.746	1944	1950	1962	rBV	271874	434740	21.93%	2.153%
19	15.568	2082	2090	2098	rBV	978632	1488855	75.11%	7.374%
20	15.668	2101	2107	2117	rBV	199772	299009	15.09%	1.481%
21	15.803	2126	2130	2133	rVB2	3596	4379	0.22%	0.022%
22	16.356	2219	2224	2227	rBV3	2259	3029	0.15%	0.015%
23	17.313	2380	2387	2396	rBV	781214	1149801	58.01%	5.695%
24	17.413	2397	2404	2413	rVV	1065833	1572366	79.33%	7.788%
25	19.263	2714	2719	2725	rBV2	13366	18576	0.94%	0.092%
26	19.328	2725	2730	2736	rVV	12263	17743	0.90%	0.088%
27	19.416	2740	2745	2748	rVB4	2118	3327	0.17%	0.016%
28	19.504	2754	2760	2764	rBV5	1104	2382	0.12%	0.012%
29	19.645	2779	2784	2786	rBV3	4982	6216	0.31%	0.031%
30	19.692	2786	2792	2807	rVV	1303571	1865297	94.11%	9.239%
31	20.679	2957	2960	2965	rBV4	5262	6393	0.32%	0.032%
32	21.249	3054	3057	3059	rBV4	2853	2796	0.14%	0.014%
33	21.554	3102	3109	3117	rBV2	803438	1282696	64.71%	6.353%
34	21.713	3134	3136	3139	rVB3	2882	2505	0.13%	0.012%
35	21.784	3146	3148	3151	rVB3	4077	3735	0.19%	0.018%
36	22.383	3244	3250	3251	rBV3	10845	16106	0.81%	0.080%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
 Data File : BG062313.D
 Acq On : 8 Aug 2024 00:22
 Operator : MA/JU
 Sample : PB162446BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK446

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

37	23.047	3357	3363	3369	rBV2	14326	26904	1.36%	0.133%
38	23.828	3491	3496	3503	rVB4	20074	37584	1.90%	0.186%
39	24.433	3588	3599	3617	rBV	723721	1982122	100.00%	9.817%
40	24.644	3623	3635	3646	rBV	518053	1402746	70.77%	6.948%
41	24.750	3646	3653	3661	rVB3	27815	69065	3.48%	0.342%
42	25.849	3831	3840	3848	rBV5	27762	85251	4.30%	0.422%
43	26.260	3908	3910	3913	rVB4	2517	2196	0.11%	0.011%
44	26.401	3932	3934	3936	rBV3	2073	2216	0.11%	0.011%
45	26.624	3970	3972	3975	rVV4	2511	2505	0.13%	0.012%
46	26.982	4031	4033	4036	rBV4	2428	2891	0.15%	0.014%
47	27.153	4055	4062	4074	rVB4	25802	77620	3.92%	0.384%
48	27.482	4117	4118	4120	rBV2	2411	2182	0.11%	0.011%
49	27.787	4168	4170	4175	rBV5	2844	2386	0.12%	0.012%
50	28.668	4317	4320	4322	rBV4	3497	5451	0.28%	0.027%
51	28.733	4322	4331	4342	rVB10	15582	65483	3.30%	0.324%
52	30.478	4627	4628	4632	rBV3	2533	2490	0.13%	0.012%
53	30.625	4650	4653	4654	rBV3	4196	4474	0.23%	0.022%
54	31.523	4804	4806	4812	rVB5	2454	2465	0.12%	0.012%
55	31.629	4822	4824	4826	rBV3	1897	2082	0.11%	0.010%
56	32.228	4924	4926	4928	rVB3	2857	2471	0.12%	0.012%
57	32.393	4952	4954	4957	rVB3	4004	3166	0.16%	0.016%




Sum of corrected areas: 20190130

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062313.D
Acq On : 8 Aug 2024 00:22
Operator : MA/JU
Sample : PB162446BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK446

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

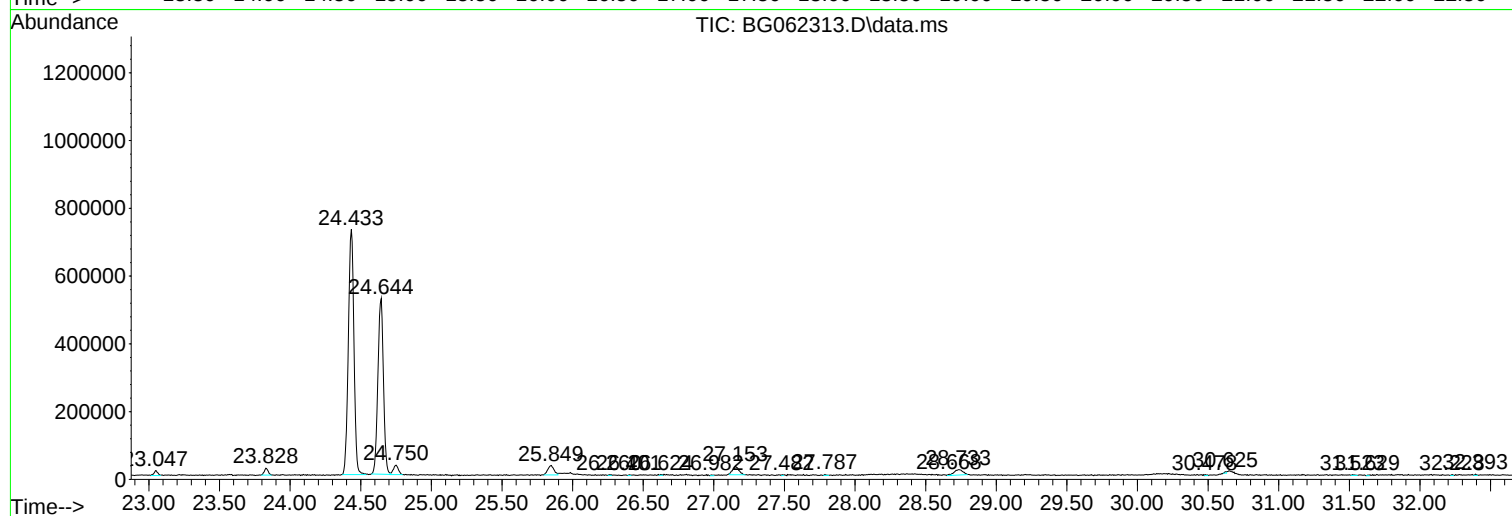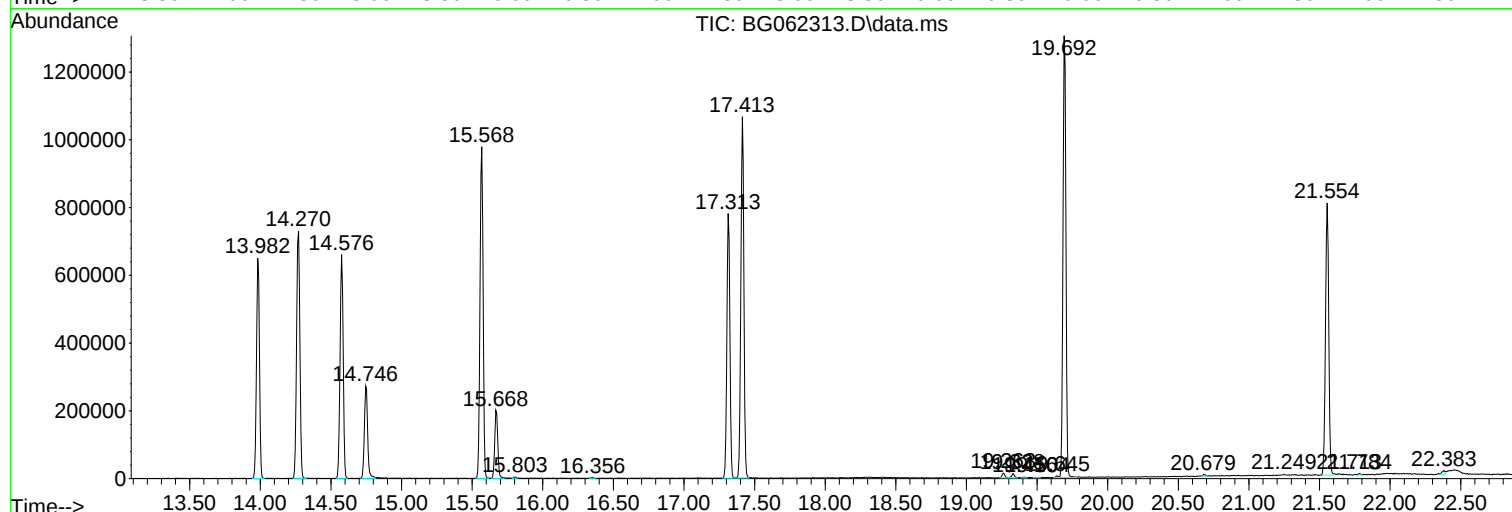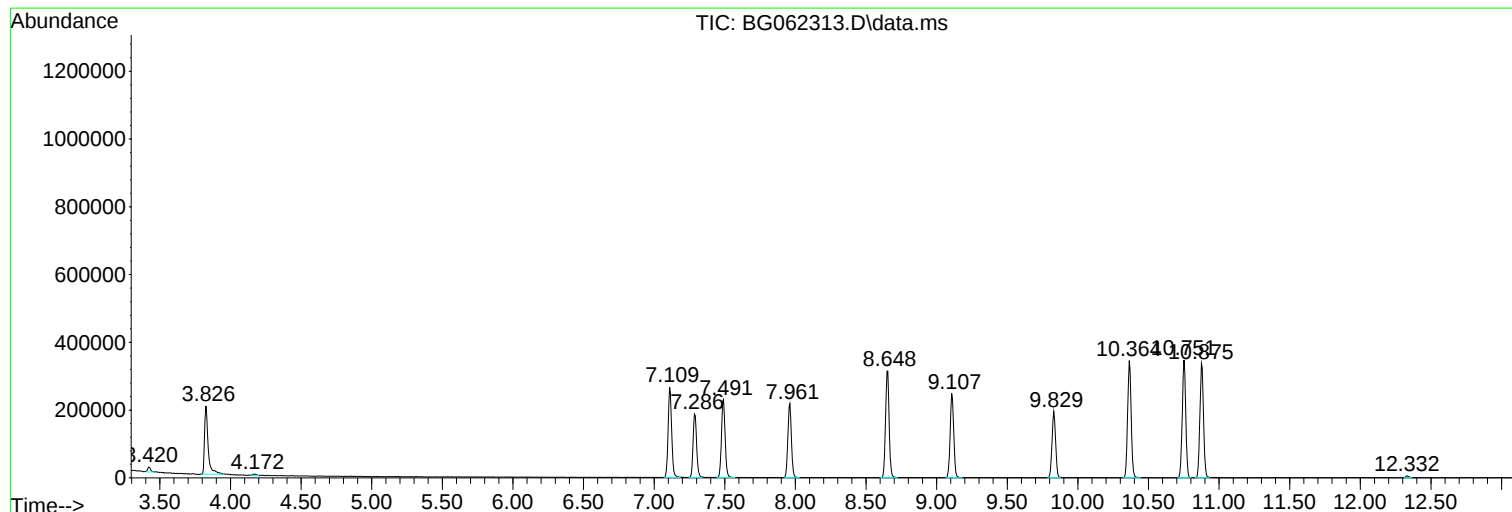

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062313.D
Acq On : 8 Aug 2024 00:22
Operator : MA/JU
Sample : PB162446BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK446

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062313.D
Acq On : 8 Aug 2024 00:22
Operator : MA/JU
Sample : PB162446BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK446

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc