

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
 Data File : BG062314.D
 Acq On : 8 Aug 2024 1:03
 Operator : MA/JU
 Sample : PB162447BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK447

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs : 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062314.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.833	89	93	98	rBV	19798	39907	14.12%	1.359%
2	4.239	160	162	163	rVB	1383	732	0.26%	0.025%
3	4.544	212	214	216	rBV	864	676	0.24%	0.023%
4	4.568	216	218	220	rBV2	798	782	0.28%	0.027%
5	4.709	240	242	244	rVB2	816	592	0.21%	0.020%
6	4.732	244	246	247	rBV	791	596	0.21%	0.020%
7	5.008	291	293	294	rBV2	569	546	0.19%	0.019%
8	5.020	294	295	296	rVB	1321	465	0.16%	0.016%
9	5.032	296	297	300	rBV3	1044	1065	0.38%	0.036%
10	5.149	315	317	321	rVB2	925	791	0.28%	0.027%
11	5.184	321	323	324	rBV2	717	412	0.15%	0.014%
12	5.208	325	327	331	rBV3	420	553	0.20%	0.019%
13	5.361	351	353	354	rBV	603	511	0.18%	0.017%
14	5.396	357	359	362	rVB3	641	785	0.28%	0.027%
15	5.537	380	383	384	rBV	760	582	0.21%	0.020%
16	5.596	391	393	395	rBV2	596	435	0.15%	0.015%
17	5.807	428	429	431	rBV	751	472	0.17%	0.016%
18	5.954	452	454	456	rVB2	534	490	0.17%	0.017%
19	6.019	462	465	468	rBV2	714	745	0.26%	0.025%
20	6.124	479	483	484	rBV	484	568	0.20%	0.019%
21	6.242	499	503	505	rVB2	672	921	0.33%	0.031%
22	6.383	526	527	531	rVB2	451	525	0.19%	0.018%
23	6.483	541	544	546	rBV2	673	535	0.19%	0.018%
24	6.718	581	584	585	rBV2	621	488	0.17%	0.017%
25	6.770	590	593	594	rBV2	655	645	0.23%	0.022%
26	6.929	617	620	621	rBV2	562	470	0.17%	0.016%
27	7.117	641	652	661	rBV	42109	87228	30.86%	2.970%
28	7.217	667	669	673	rVB	600	489	0.17%	0.017%
29	7.293	675	682	688	rBV	32351	64430	22.80%	2.194%
30	7.493	710	716	725	rBV2	40844	80283	28.41%	2.734%
31	7.675	745	747	750	rBV	720	621	0.22%	0.021%
32	7.728	752	756	757	rBV2	434	484	0.17%	0.016%
33	7.781	763	765	767	rBB	730	641	0.23%	0.022%
34	7.810	767	770	771	rBV	539	615	0.22%	0.021%
35	7.963	790	796	805	rBV2	44077	82702	29.26%	2.816%
36	8.404	868	871	873	rBV	311	460	0.16%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062314.D
Acq On : 8 Aug 2024 1:03
Operator : MA/JU
Sample : PB162447BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK447

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Title : SVOA CALIBRATION

37	8.492	882	886	889	rBV2	706	1250	0.44%	0.043%
38	8.545	891	895	898	rVV	280	432	0.15%	0.015%
39	8.650	906	913	925	rVB	51377	96592	34.18%	3.289%
40	8.762	928	932	933	rBV	381	455	0.16%	0.015%

41	9.108	984	991	999	rBV	40945	74542	26.38%	2.538%
42	9.320	1024	1027	1031	rBV	403	597	0.21%	0.020%
43	9.749	1096	1100	1101	rVB	481	550	0.19%	0.019%
44	9.766	1101	1103	1105	rBV	351	423	0.15%	0.014%
45	9.831	1108	1114	1124	rVB2	27951	50136	17.74%	1.707%

46	10.366	1199	1205	1217	rVV	53904	91581	32.40%	3.119%
47	10.753	1263	1271	1280	rBV	60990	108382	38.35%	3.691%
48	10.877	1285	1292	1302	rBV	49332	92482	32.72%	3.149%
49	11.570	1408	1410	1414	rVB	453	576	0.20%	0.020%
50	12.005	1481	1484	1491	rVB	577	705	0.25%	0.024%

51	12.328	1537	1539	1543	rVB3	822	1067	0.38%	0.036%
52	12.856	1626	1629	1631	rBV	414	445	0.16%	0.015%
53	13.426	1723	1726	1729	rBV	1103	969	0.34%	0.033%
54	13.790	1786	1788	1792	rVB	393	447	0.16%	0.015%
55	13.831	1792	1795	1798	rBV	276	432	0.15%	0.015%

56	13.978	1815	1820	1828	rBV	93863	139841	49.48%	4.762%
57	14.266	1863	1869	1876	rBV	112163	175642	62.15%	5.981%
58	14.572	1915	1921	1928	rBB	97792	149430	52.87%	5.089%
59	14.748	1945	1951	1959	rBV2	21539	38673	13.68%	1.317%
60	14.871	1971	1972	1975	rBV2	540	423	0.15%	0.014%

61	15.288	2041	2043	2045	rBV	498	426	0.15%	0.015%
62	15.447	2068	2070	2071	rBV	554	489	0.17%	0.017%
63	15.500	2076	2079	2080	rVB2	505	410	0.15%	0.014%
64	15.564	2084	2090	2098	rVV	153191	220225	77.92%	7.499%
65	15.670	2103	2108	2113	rVB2	13077	18188	6.44%	0.619%

66	15.705	2113	2114	2117	rBV2	1115	585	0.21%	0.020%
67	15.758	2121	2123	2126	rBV	511	537	0.19%	0.018%
68	15.911	2148	2149	2152	rVB	582	489	0.17%	0.017%
69	16.052	2170	2173	2174	rBV	587	669	0.24%	0.023%
70	16.123	2181	2185	2186	rBV2	590	898	0.32%	0.031%

71	16.193	2196	2197	2202	rBV2	478	531	0.19%	0.018%
72	16.264	2207	2209	2213	rVB	566	528	0.19%	0.018%
73	16.410	2232	2234	2235	rBV	518	475	0.17%	0.016%
74	16.457	2239	2242	2246	rBV2	676	1006	0.36%	0.034%
75	16.563	2258	2260	2261	rBV	512	436	0.15%	0.015%

76	16.681	2278	2280	2283	rVB	779	824	0.29%	0.028%
----	--------	------	------	------	-----	-----	-----	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
 Data File : BG062314.D
 Acq On : 8 Aug 2024 1:03
 Operator : MA/JU
 Sample : PB162447BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK447

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

77	16.704	2283	2284	2285	rBV	702	419	0.15%	0.014%
78	17.039	2339	2341	2346	rBV2	440	453	0.16%	0.015%
79	17.098	2349	2351	2352	rBV	832	525	0.19%	0.018%
80	17.186	2364	2366	2371	rBV2	442	903	0.32%	0.031%
81	17.250	2375	2377	2380	rBV	507	701	0.25%	0.024%
82	17.315	2382	2388	2394	rVV	110539	166767	59.01%	5.679%
83	17.409	2398	2404	2413	rVV	153613	228596	80.88%	7.784%
84	17.615	2437	2439	2441	rBV	570	500	0.18%	0.017%
85	17.673	2447	2449	2452	rVB2	798	721	0.26%	0.025%
86	17.738	2458	2460	2463	rBB	503	448	0.16%	0.015%
87	17.991	2501	2503	2504	rBV2	721	455	0.16%	0.015%
88	18.179	2534	2535	2537	rBV	861	529	0.19%	0.018%
89	18.290	2552	2554	2555	rBV	1133	503	0.18%	0.017%
90	18.372	2567	2568	2569	rBV	1098	453	0.16%	0.015%
91	18.519	2591	2593	2596	rBV2	1188	1308	0.46%	0.045%
92	18.613	2607	2609	2612	rBV2	733	946	0.33%	0.032%
93	19.265	2716	2720	2724	rBV4	1946	2566	0.91%	0.087%
94	19.318	2728	2729	2730	rBV	1183	653	0.23%	0.022%
95	19.518	2761	2763	2766	rBV3	982	828	0.29%	0.028%
96	19.612	2777	2779	2781	rBV3	1115	1023	0.36%	0.035%
97	19.694	2787	2793	2802	rVB	197332	282622	100.00%	9.624%
98	21.550	3104	3109	3115	rBV2	110653	178953	63.32%	6.094%
99	24.429	3591	3599	3608	rVB3	92632	242055	85.65%	8.243%
100	24.640	3627	3635	3644	rVB2	67664	177607	62.84%	6.048%

Sum of corrected areas: 2936564




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062314.D
Acq On : 8 Aug 2024 1:03
Operator : MA/JU
Sample : PB162447BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK447

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L

TIC Integration Parameters: LSCINT.P

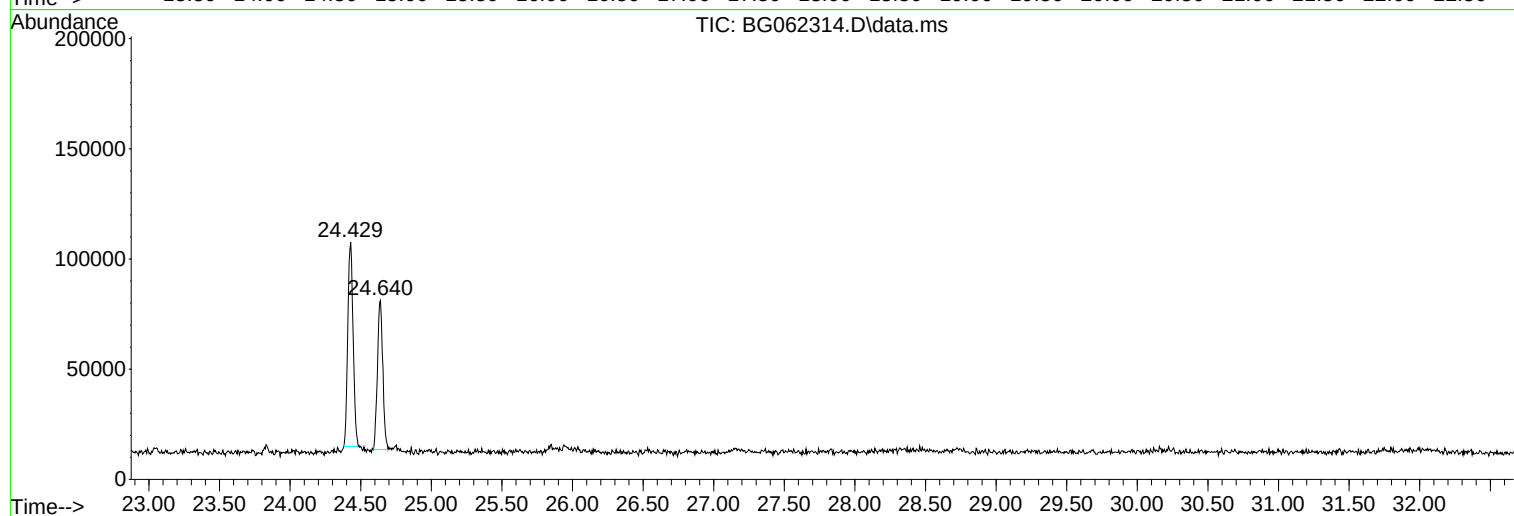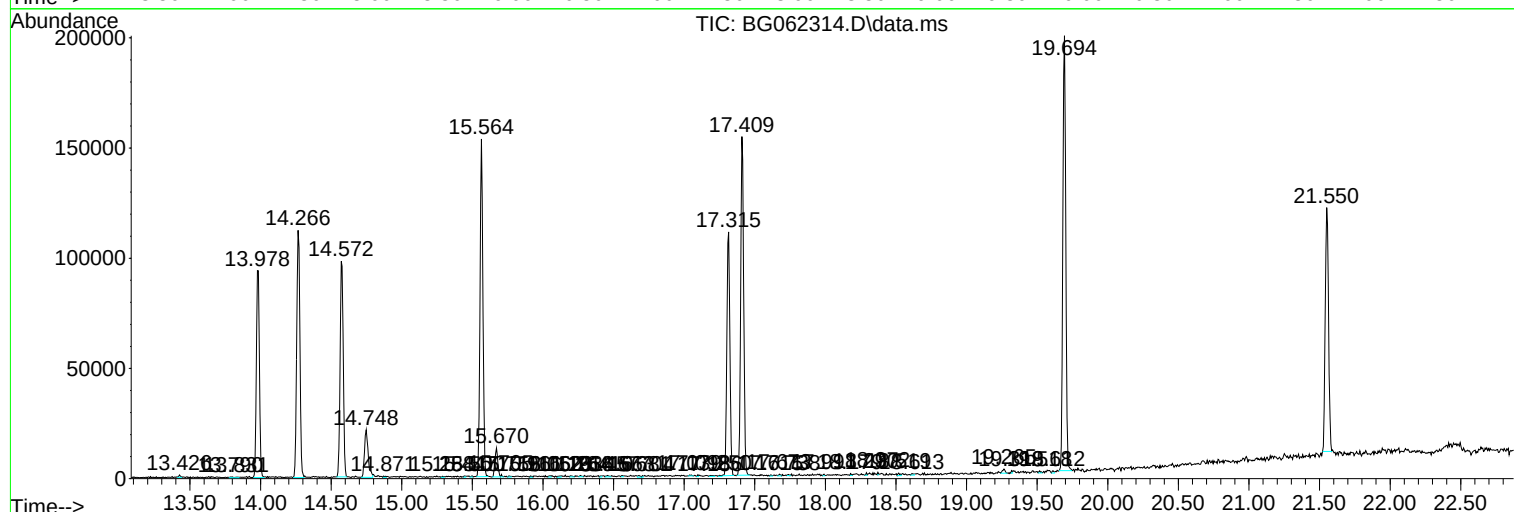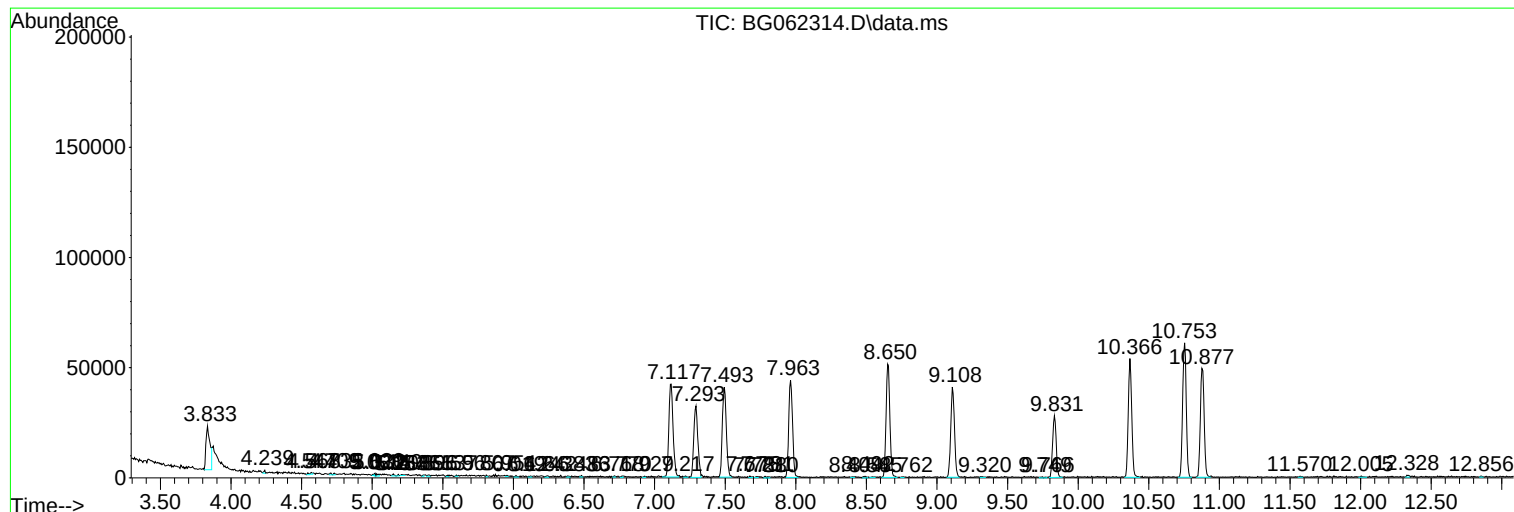

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062314.D
Acq On : 8 Aug 2024 1:03
Operator : MA/JU
Sample : PB162447BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK447

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062314.D
Acq On : 8 Aug 2024 1:03
Operator : MA/JU
Sample : PB162447BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK447

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc