

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
 Data File : BG062315.D
 Acq On : 8 Aug 2024 1:45
 Operator : MA/JU
 Sample : P3437-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062315.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.423	19	23	30	rVB	16600	26338	1.57%	0.139%
2	3.828	87	92	103	rVB	119863	199413	11.91%	1.055%
3	4.169	146	150	152	rBV3	1996	2536	0.15%	0.013%
4	6.048	464	470	474	rBV3	2028	3400	0.20%	0.018%
5	7.112	644	651	659	rBV	146900	249325	14.90%	1.318%
6	7.288	674	681	690	rBV	143538	239217	14.29%	1.265%
7	7.488	708	715	722	rBV	181023	297537	17.78%	1.573%
8	7.552	722	726	734	rVB	9603	16456	0.98%	0.087%
9	7.958	788	795	803	rBV	216582	354020	21.15%	1.872%
10	8.028	803	807	810	rVB3	1455	2301	0.14%	0.012%
11	8.651	906	913	922	rBV	224885	378323	22.60%	2.001%
12	9.109	983	991	999	rVB	188355	325510	19.45%	1.721%
13	9.673	1082	1087	1092	rVB3	7002	10998	0.66%	0.058%
14	9.832	1106	1114	1123	rVB	140172	248932	14.87%	1.316%
15	10.366	1197	1205	1216	rBV	269191	467455	27.93%	2.472%
16	10.748	1263	1270	1280	rVB	323996	580857	34.70%	3.072%
17	10.877	1284	1292	1302	rBV	256334	462020	27.60%	2.443%
18	11.282	1354	1361	1367	rBV3	3126	4334	0.26%	0.023%
19	11.482	1389	1395	1403	rBV	44521	80175	4.79%	0.424%
20	12.328	1535	1539	1546	rVB	5446	8502	0.51%	0.045%
21	12.939	1640	1643	1650	rVB2	1725	2886	0.17%	0.015%
22	13.198	1683	1687	1692	rBV3	3143	4436	0.27%	0.023%
23	13.485	1731	1736	1740	rVB2	1329	2397	0.14%	0.013%
24	13.985	1814	1821	1828	rVB	514188	758712	45.33%	4.012%
25	14.267	1858	1869	1879	rBV2	606112	950774	56.80%	5.028%
26	14.578	1912	1922	1930	rVV	604214	958003	57.24%	5.066%
27	14.678	1936	1939	1943	rVB2	5757	6645	0.40%	0.035%
28	14.748	1943	1951	1953	rBV	120473	178516	10.67%	0.944%
29	14.784	1953	1957	1958	rVV	534140	617864	36.91%	3.267%
30	14.801	1958	1960	1972	rVB	643135	858745	51.31%	4.541%
31	15.089	2004	2009	2014	rBV4	1825	2881	0.17%	0.015%
32	15.383	2055	2059	2066	rBV5	2930	5555	0.33%	0.029%
33	15.565	2082	2090	2098	rBV	810111	1205992	72.05%	6.377%
34	15.671	2101	2108	2114	rBV	91049	138315	8.26%	0.731%
35	15.735	2117	2119	2123	rVB3	2541	2652	0.16%	0.014%
36	15.806	2126	2131	2134	rBV3	2202	3371	0.20%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
 Data File : BG062315.D
 Acq On : 8 Aug 2024 1:45
 Operator : MA/JU
 Sample : P3437-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

37	16.117	2177	2184	2191	rBV5	5405	9747	0.58%	0.052%
38	16.235	2197	2204	2209	rBV2	5925	7553	0.45%	0.040%
39	16.305	2212	2216	2219	rBV3	3213	3540	0.21%	0.019%
40	16.470	2239	2244	2247	rVB2	1441	2495	0.15%	0.013%
41	16.722	2282	2287	2291	rBV3	2083	3640	0.22%	0.019%
42	16.881	2310	2314	2319	rBV4	2166	3462	0.21%	0.018%
43	16.998	2329	2334	2337	rVB3	1537	3021	0.18%	0.016%
44	17.092	2346	2350	2356	rBV6	3126	4891	0.29%	0.026%
45	17.251	2373	2377	2381	rVV2	15405	18185	1.09%	0.096%
46	17.315	2381	2388	2394	rVV	766660	1129879	67.51%	5.975%
47	17.362	2394	2396	2398	rVV3	4650	4965	0.30%	0.026%
48	17.409	2398	2404	2412	rVB	864532	1305521	78.00%	6.904%
49	17.709	2448	2455	2460	rBV4	6024	12705	0.76%	0.067%
50	17.827	2473	2475	2480	rBV3	2660	3593	0.21%	0.019%
51	18.003	2500	2505	2509	rBV	11810	15365	0.92%	0.081%
52	18.085	2516	2519	2524	rBV4	3661	4887	0.29%	0.026%
53	18.214	2537	2541	2549	rBV2	47041	72139	4.31%	0.381%
54	18.291	2553	2554	2558	rVB3	3750	2702	0.16%	0.014%
55	18.396	2571	2572	2578	rBV3	1743	2249	0.13%	0.012%
56	18.526	2589	2594	2596	rBV2	2561	4579	0.27%	0.024%
57	18.649	2612	2615	2619	rVB3	4051	4700	0.28%	0.025%
58	18.772	2632	2636	2641	rBV3	3624	4932	0.29%	0.026%
59	19.019	2675	2678	2683	rBV5	3426	5455	0.33%	0.029%
60	19.078	2683	2688	2694	rBV5	5901	10875	0.65%	0.058%
61	19.137	2694	2698	2699	rBV2	4288	5573	0.33%	0.029%
62	19.166	2699	2703	2707	rVB2	34262	39790	2.38%	0.210%
63	19.260	2715	2719	2723	rBV2	11349	15928	0.95%	0.084%
64	19.301	2723	2726	2728	rVV2	6731	6015	0.36%	0.032%
65	19.330	2728	2731	2735	rVV	13299	18179	1.09%	0.096%
66	19.360	2735	2736	2739	rVV2	4517	4650	0.28%	0.025%
67	19.395	2740	2742	2746	rVB3	6157	6497	0.39%	0.034%
68	19.489	2754	2758	2762	rBV4	12666	18894	1.13%	0.100%
69	19.642	2778	2784	2787	rBV7	6226	11168	0.67%	0.059%
70	19.695	2787	2793	2801	rVV	1158317	1582191	94.53%	8.367%
71	19.836	2814	2817	2821	rVB6	2106	2716	0.16%	0.014%
72	19.930	2829	2833	2836	rBV6	3154	4870	0.29%	0.026%
73	20.118	2860	2865	2868	rVB5	4460	7580	0.45%	0.040%
74	20.229	2879	2884	2885	rBV4	3514	5979	0.36%	0.032%
75	20.482	2925	2927	2930	rVB4	2933	2712	0.16%	0.014%
76	20.752	2970	2973	2976	rVB4	4726	5924	0.35%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
 Data File : BG062315.D
 Acq On : 8 Aug 2024 1:45
 Operator : MA/JU
 Sample : P3437-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

77	21.234	3050	3055	3062	rBV2	38200	66210	3.96%	0.350%
78	21.551	3103	3109	3116	rBV2	787971	1274673	76.16%	6.741%
79	21.780	3144	3148	3152	rBV3	9177	13078	0.78%	0.069%
80	22.373	3247	3249	3255	rVB3	11502	15099	0.90%	0.080%
81	22.526	3271	3275	3277	rBV4	7681	9492	0.57%	0.050%
82	22.655	3295	3297	3302	rVB5	6392	7646	0.46%	0.040%
83	22.714	3304	3307	3312	rVB5	7618	11892	0.71%	0.063%
84	22.843	3327	3329	3333	rBV5	2889	4866	0.29%	0.026%
85	23.049	3360	3364	3372	rVB3	15469	25950	1.55%	0.137%
86	23.231	3388	3395	3402	rVB2	60493	117948	7.05%	0.624%
87	23.572	3450	3453	3454	rBV3	3236	3972	0.24%	0.021%
88	23.830	3490	3497	3504	rBV5	18136	42107	2.52%	0.223%
89	24.429	3588	3599	3616	rBV	632100	1673768	100.00%	8.851%
90	24.641	3624	3635	3647	rBV2	508274	1394983	83.34%	7.377%
91	24.747	3647	3653	3663	rVB4	23250	61584	3.68%	0.326%
92	24.870	3673	3674	3677	rBV3	3161	2704	0.16%	0.014%
93	25.845	3832	3840	3850	rVB2	21727	61218	3.66%	0.324%
94	26.356	3926	3927	3930	rBV2	3397	3149	0.19%	0.017%
95	26.433	3938	3940	3941	rBV2	3034	2536	0.15%	0.013%
96	27.149	4053	4062	4072	rBV7	19896	61376	3.67%	0.325%
97	30.639	4649	4656	4657	rBV6	7348	13099	0.78%	0.069%
98	30.979	4712	4714	4718	rVB5	2225	2458	0.15%	0.013%
99	31.614	4818	4822	4824	rBV5	2771	3434	0.21%	0.018%
100	32.372	4949	4951	4953	rBV3	2049	2239	0.13%	0.012%




Sum of corrected areas: 18910620

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062315.D
Acq On : 8 Aug 2024 1:45
Operator : MA/JU
Sample : P3437-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

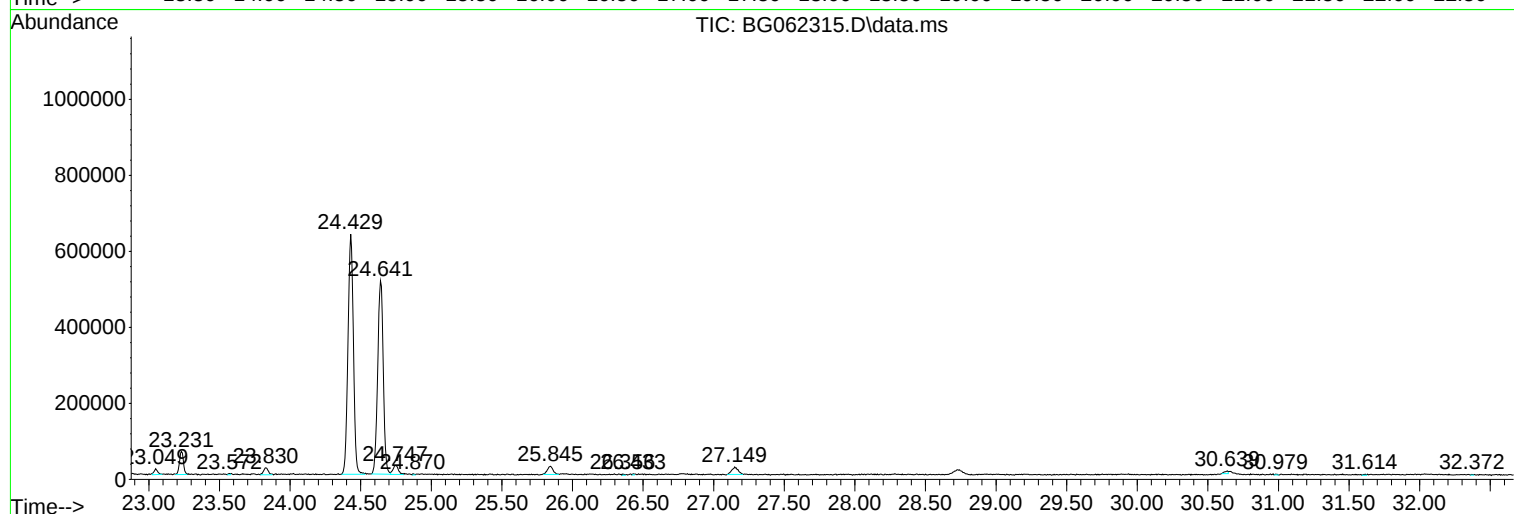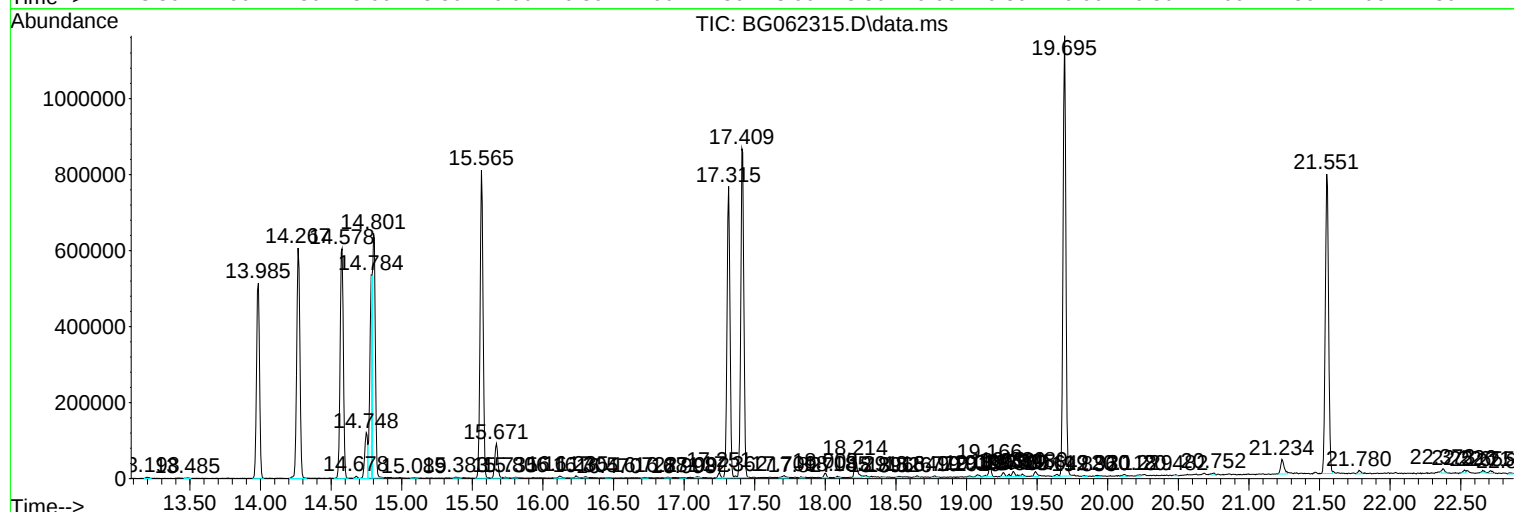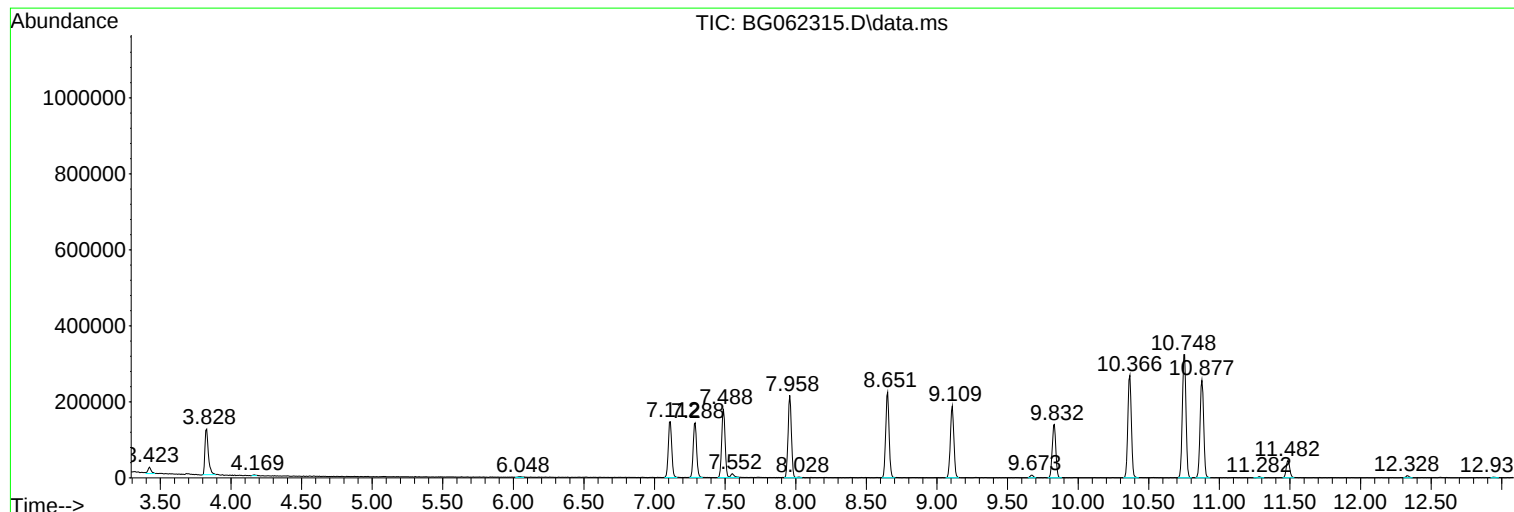

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062315.D
Acq On : 8 Aug 2024 1:45
Operator : MA/JU
Sample : P3437-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Phenoxypropan-2-ol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.482	2.76 ng/ul	80175	Naphthalene-d8	10.748

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1-Phenoxypropan-2-ol	152	C9H12O2	000770-35-4	97
2			1-Phenoxypropan-2-ol	152	C9H12O2	000770-35-4	97
3			1-Phenoxypropan-2-ol	152	C9H12O2	000770-35-4	94
4			1-Propanol, 3-phenoxy-	152	C9H12O2	006180-61-6	87
5			1-Phenoxypropan-2-ol	152	C9H12O2	000770-35-4	64

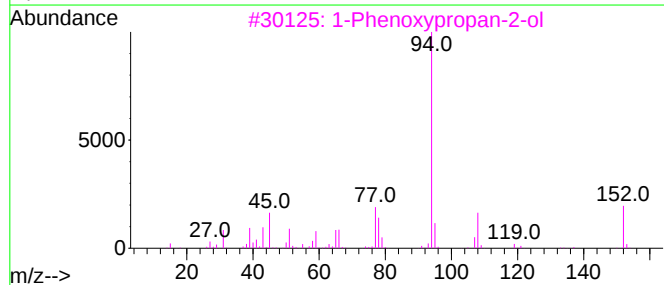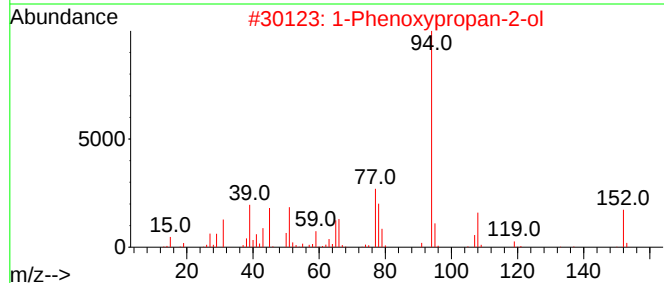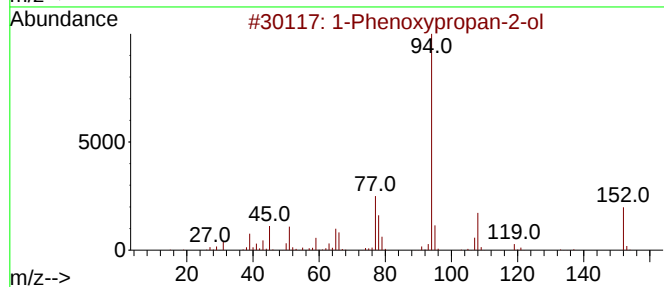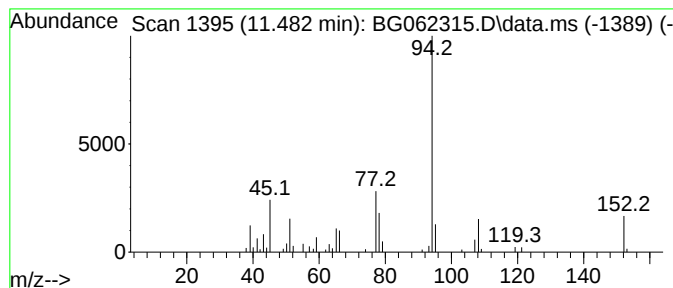

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062315.D
Acq On : 8 Aug 2024 1:45
Operator : MA/JU
Sample : P3437-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.801	17.93 ng/ul	858745	Acenaphthene-d10	14.578

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propanoic acid, 2-octyl ester, (...	186	C11H22O2	1000164-41-5	27
2			3-Octanol, acetate	172	C10H20O2	004864-61-3	16
3			Tridecane, 4-methyl-	198	C14H30	026730-12-1	15
4			3-Octanol, acetate	172	C10H20O2	004864-61-3	14
5			Carbonic acid, eicosyl prop-1-en...	382	C24H46O3	1000383-10-8	12

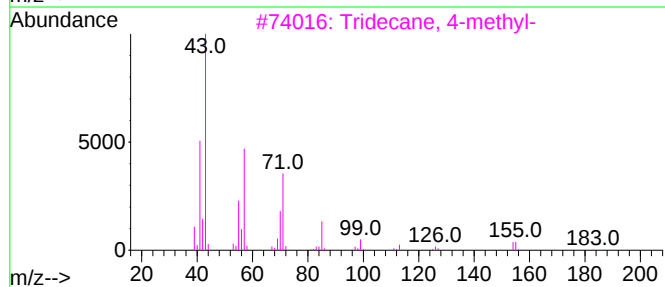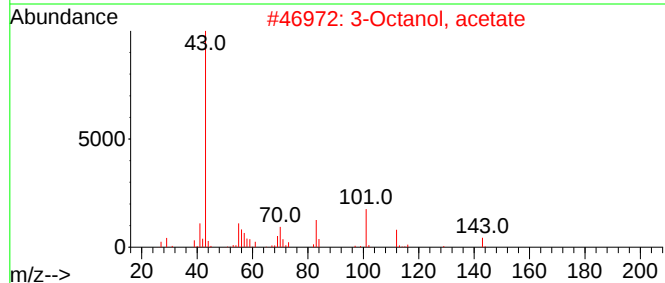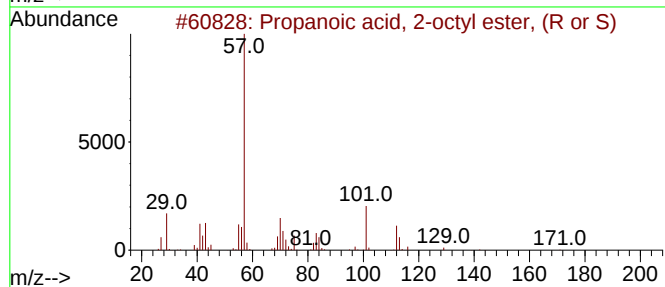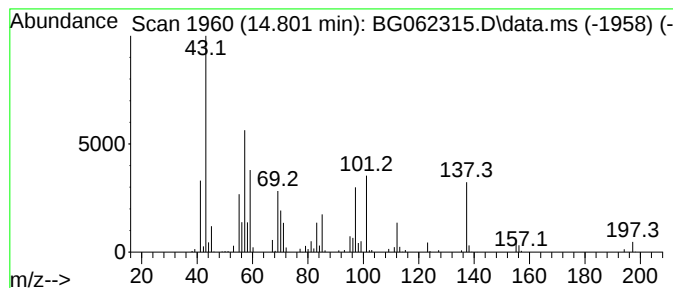

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062315.D
Acq On : 8 Aug 2024 1:45
Operator : MA/JU
Sample : P3437-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Phenoxypropan...	11.482	2.8	ng/u1	80175	2	10.748	580857	20.0
unknown-01	14.801	17.9	ng/u1	858745	3	14.578	958003	20.0