

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
 Data File : BG062316.D
 Acq On : 8 Aug 2024 2:26
 Operator : MA/JU
 Sample : P3437-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062316.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.423	19	23	27	rBV2	12755	18705	1.15%	0.126%
2	3.829	87	92	102	rBV	107143	181272	11.11%	1.218%
3	4.169	147	150	152	rVB3	3255	3008	0.18%	0.020%
4	5.344	347	350	357	rBV5	1186	2666	0.16%	0.018%
5	7.107	644	650	661	rBV	138841	240513	14.74%	1.617%
6	7.289	674	681	693	rVV	105806	180139	11.04%	1.211%
7	7.488	709	715	725	rBV	135915	229993	14.09%	1.546%
8	7.958	788	795	804	rBV	255844	423612	25.96%	2.847%
9	8.652	906	913	924	rBV	180944	307514	18.84%	2.067%
10	9.110	983	991	998	rBV	135873	238731	14.63%	1.605%
11	9.674	1082	1087	1092	rVB3	2248	3199	0.20%	0.022%
12	9.826	1107	1113	1123	rBV	103453	181400	11.11%	1.219%
13	10.367	1198	1205	1218	rVB	185509	332259	20.36%	2.233%
14	10.749	1261	1270	1278	rBV	384896	682863	41.84%	4.590%
15	10.878	1284	1292	1304	rBV	188274	342338	20.98%	2.301%
16	11.489	1386	1396	1402	rBV2	7186	13191	0.81%	0.089%
17	12.329	1535	1539	1545	rBV4	2919	5405	0.33%	0.036%
18	13.986	1814	1821	1828	rBV	368850	535188	32.79%	3.597%
19	14.268	1862	1869	1881	rVB	439026	678695	41.59%	4.562%
20	14.573	1915	1921	1929	rVB	737753	1145875	70.21%	7.702%
21	14.743	1944	1950	1955	rBV	119245	193501	11.86%	1.301%
22	14.784	1955	1957	1958	rVV	6352	5770	0.35%	0.039%
23	15.566	2083	2090	2102	rVB	583710	858354	52.59%	5.769%
24	15.671	2102	2108	2115	rBV	79751	121279	7.43%	0.815%
25	15.807	2124	2131	2133	rBV3	1578	2809	0.17%	0.019%
26	16.235	2200	2204	2208	rBV2	1470	1982	0.12%	0.013%
27	17.093	2347	2350	2355	rVB2	2088	2727	0.17%	0.018%
28	17.252	2374	2377	2381	rBV5	2070	2860	0.18%	0.019%
29	17.316	2381	2388	2396	rBV	894691	1338068	81.99%	8.993%
30	17.410	2397	2404	2412	rVB	606566	903709	55.37%	6.074%
31	17.851	2475	2479	2481	rBV	1431	1650	0.10%	0.011%
32	17.998	2499	2504	2506	rBV3	1597	2405	0.15%	0.016%
33	18.215	2536	2541	2547	rBV3	6362	10107	0.62%	0.068%
34	18.397	2571	2572	2577	rBV3	1327	1659	0.10%	0.011%
35	19.167	2700	2703	2707	rVB4	2906	3325	0.20%	0.022%
36	19.202	2707	2709	2713	rBV2	1054	1654	0.10%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
 Data File : BG062316.D
 Acq On : 8 Aug 2024 2:26
 Operator : MA/JU
 Sample : P3437-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

37	19.261	2713	2719	2724	rBV3	9263	12359	0.76%	0.083%
38	19.331	2727	2731	2736	rVB2	7677	10652	0.65%	0.072%
39	19.496	2755	2759	2761	rBV4	1568	1989	0.12%	0.013%
40	19.643	2780	2784	2787	rBV3	4217	4768	0.29%	0.032%

41	19.695	2787	2793	2801	rBV	736169	1078689	66.09%	7.250%
42	19.925	2828	2832	2834	rBV4	2117	2781	0.17%	0.019%
43	20.306	2893	2897	2900	rBV4	1784	2326	0.14%	0.016%
44	20.353	2902	2905	2906	rBV2	1829	1715	0.11%	0.012%
45	20.682	2958	2961	2966	rVB6	4676	5063	0.31%	0.034%

46	20.923	3000	3002	3007	rBV5	1845	2991	0.18%	0.020%
47	21.235	3050	3055	3061	rBV5	9308	20899	1.28%	0.140%
48	21.552	3102	3109	3122	rBV2	943537	1514683	92.81%	10.180%
49	21.787	3146	3149	3155	rVB7	4216	7118	0.44%	0.048%
50	22.280	3231	3233	3235	rBV3	2567	2839	0.17%	0.019%

51	22.380	3245	3250	3252	rBV4	5368	8952	0.55%	0.060%
52	22.492	3267	3269	3273	rVB4	3210	2231	0.14%	0.015%
53	22.533	3273	3276	3279	rVB5	3090	3671	0.22%	0.025%
54	22.838	3326	3328	3331	rVB4	2975	2637	0.16%	0.018%
55	22.868	3331	3333	3337	rBV5	2003	2746	0.17%	0.018%

56	23.050	3359	3364	3369	rVB7	8239	13363	0.82%	0.090%
57	23.232	3389	3395	3402	rBV3	13347	24186	1.48%	0.163%
58	23.831	3491	3497	3502	rBV6	11601	22864	1.40%	0.154%
59	24.072	3536	3538	3543	rVB6	2051	2831	0.17%	0.019%
60	24.430	3588	3599	3616	rVB	420136	1111521	68.11%	7.471%

61	24.642	3624	3635	3647	rBV	593908	1632034	100.00%	10.969%
62	24.747	3649	3653	3662	rVB4	15998	37738	2.31%	0.254%
63	25.170	3723	3725	3728	rBV4	2206	2287	0.14%	0.015%
64	25.347	3753	3755	3759	rVV4	1872	2011	0.12%	0.014%
65	25.846	3831	3840	3848	rBV5	15843	48013	2.94%	0.323%

66	26.140	3888	3890	3892	rVB2	3298	2200	0.13%	0.015%
67	27.150	4052	4062	4072	rBV7	15923	55793	3.42%	0.375%
68	28.096	4221	4223	4224	rBV2	2165	2027	0.12%	0.014%
69	28.249	4247	4249	4251	rBV2	1679	1681	0.10%	0.011%
70	28.448	4281	4283	4284	rBV2	2184	1927	0.12%	0.013%

71	28.719	4324	4329	4330	rBV5	7693	11097	0.68%	0.075%
72	29.177	4406	4407	4409	rVB2	2949	1815	0.11%	0.012%
73	29.253	4416	4420	4423	rBV6	1846	3111	0.19%	0.021%
74	29.288	4423	4426	4427	rBV2	2984	2480	0.15%	0.017%
75	29.641	4485	4486	4490	rVB4	2054	1799	0.11%	0.012%

76	29.794	4508	4512	4513	rBV3	2183	2743	0.17%	0.018%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062316.D
Acq On : 8 Aug 2024 2:26
Operator : MA/JU
Sample : P3437-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Title : SVOA CALIBRATION

77	29.893	4528	4529	4531	rBV	2467	1710	0.10%	0.011%
78	30.099	4562	4564	4566	rBV3	2123	2152	0.13%	0.014%
79	30.175	4575	4577	4579	rBV3	2552	1773	0.11%	0.012%
80	32.531	4976	4978	4979	rBV	2418	1726	0.11%	0.012%




Sum of corrected areas: 14878416

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062316.D
Acq On : 8 Aug 2024 2:26
Operator : MA/JU
Sample : P3437-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

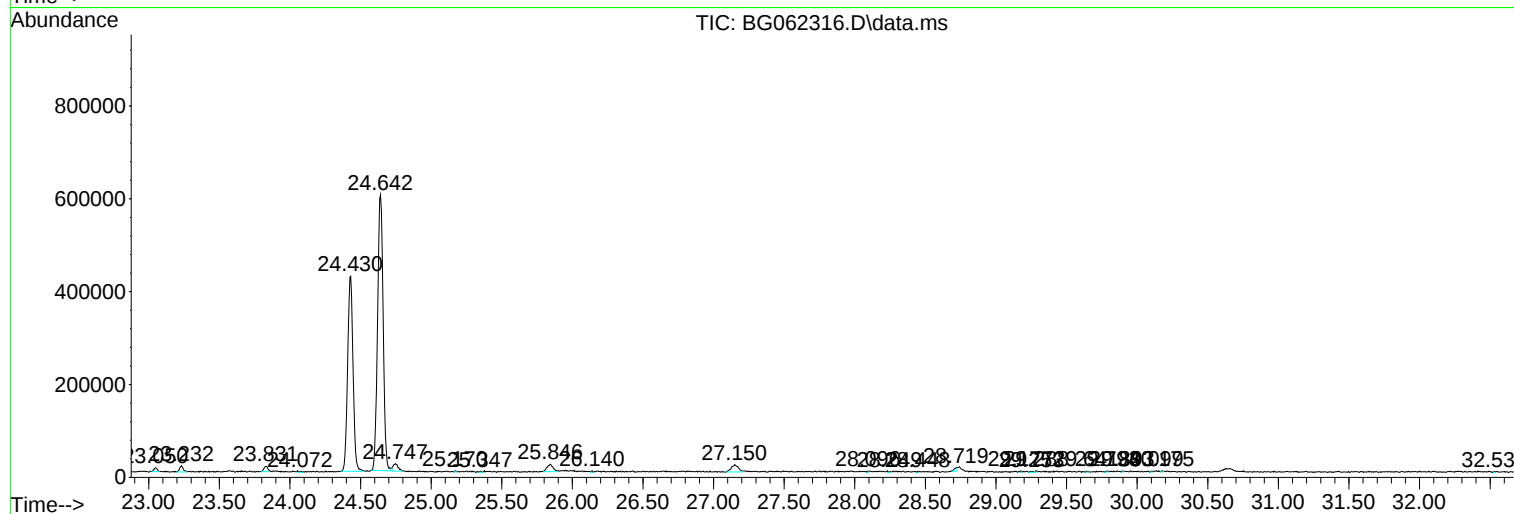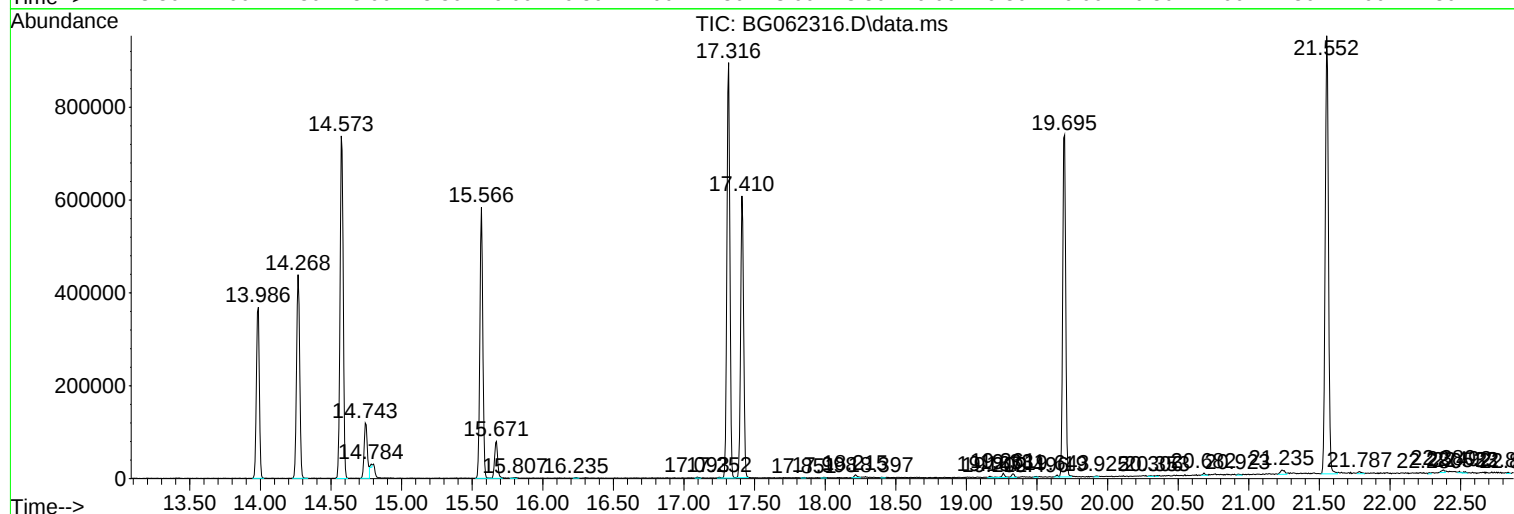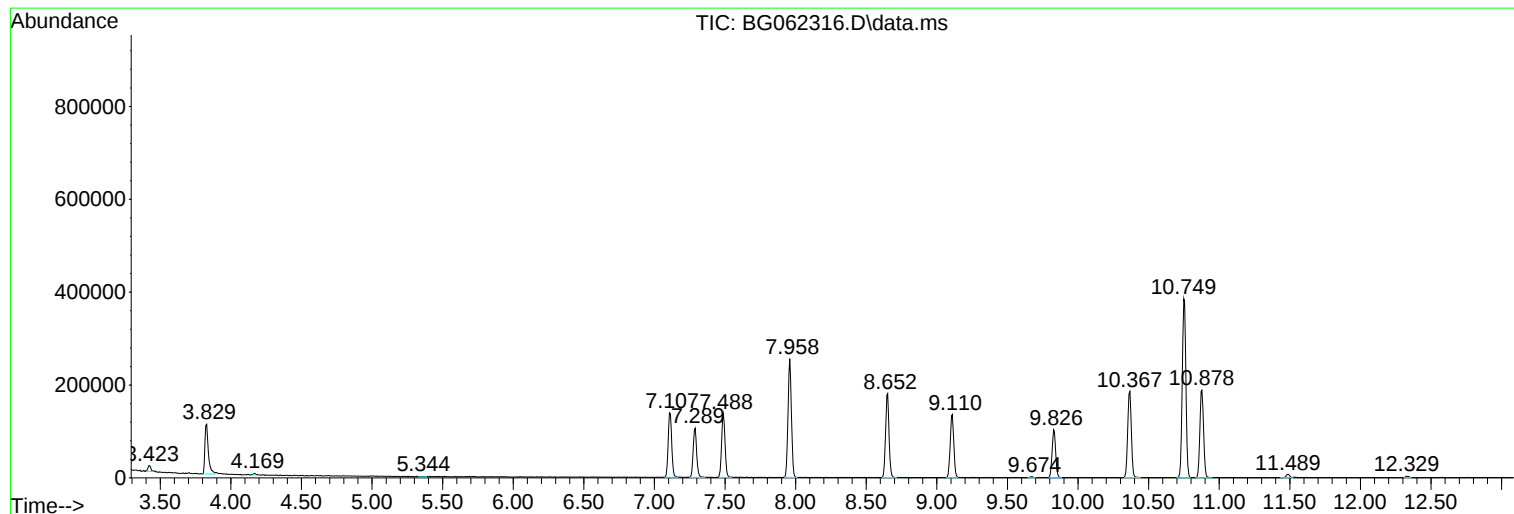

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062316.D
Acq On : 8 Aug 2024 2:26
Operator : MA/JU
Sample : P3437-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062316.D
Acq On : 8 Aug 2024 2:26
Operator : MA/JU
Sample : P3437-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc