

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
 Data File : BG062330.D
 Acq On : 8 Aug 2024 15:25
 Operator : MA/JU
 Sample : PB162447BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK447

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062330.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.423	19	23	27	rVB	13233	18207	0.90%	0.093%
2	3.823	87	91	105	rBV	189436	315514	15.67%	1.610%
3	4.163	146	149	153	rVB2	3488	4557	0.23%	0.023%
4	7.112	644	651	659	rVV	247520	415996	20.67%	2.123%
5	7.283	674	680	692	rBV	165973	282388	14.03%	1.441%
6	7.488	708	715	725	rVB	218091	357956	17.78%	1.827%
7	7.958	789	795	804	rVB	198994	327783	16.28%	1.673%
8	8.651	906	913	927	rBV	303951	508846	25.28%	2.597%
9	9.110	983	991	1000	rVB	216459	379257	18.84%	1.935%
10	9.832	1106	1114	1123	rVB	172957	309466	15.37%	1.579%
11	10.367	1197	1205	1217	rBV	317834	557085	27.68%	2.843%
12	10.754	1263	1271	1280	rVB	295913	534283	26.54%	2.727%
13	10.878	1283	1292	1303	rBV	308288	554986	27.57%	2.832%
14	12.329	1534	1539	1546	rBV2	4296	7512	0.37%	0.038%
15	13.985	1814	1821	1829	rBV	606409	886073	44.02%	4.522%
16	14.267	1862	1869	1879	rVB	722537	1110897	55.19%	5.669%
17	14.573	1914	1921	1929	rVB	606160	935822	46.49%	4.776%
18	14.749	1944	1951	1963	rBV	271847	429034	21.31%	2.189%
19	15.565	2083	2090	2102	rVB	979146	1423099	70.70%	7.262%
20	15.671	2102	2108	2121	rBV	186309	283852	14.10%	1.449%
21	15.806	2127	2131	2136	rVB4	3397	4940	0.25%	0.025%
22	16.353	2219	2224	2228	rVB3	2593	4061	0.20%	0.021%
23	17.310	2381	2387	2394	rBV	749742	1110854	55.19%	5.669%
24	17.410	2397	2404	2417	rVB	1020284	1533465	76.18%	7.826%
25	18.285	2549	2553	2556	rBV4	2157	2272	0.11%	0.012%
26	19.260	2712	2719	2723	rBV2	13248	19991	0.99%	0.102%
27	19.325	2727	2730	2737	rVV	10805	15768	0.78%	0.080%
28	19.636	2780	2783	2786	rBV3	3391	4052	0.20%	0.021%
29	19.695	2786	2793	2800	rVV	1267532	1842690	91.55%	9.404%
30	20.682	2957	2961	2964	rVB6	4560	5640	0.28%	0.029%
31	21.240	3052	3056	3058	rBV5	2825	3728	0.19%	0.019%
32	21.475	3091	3096	3101	rVB7	2990	6637	0.33%	0.034%
33	21.552	3101	3109	3117	rBV	798340	1291032	64.14%	6.588%
34	22.339	3239	3243	3244	rBV3	3216	3627	0.18%	0.019%
35	22.374	3244	3249	3252	rBV6	11150	22387	1.11%	0.114%
36	23.044	3357	3363	3371	rVB4	20047	42835	2.13%	0.219%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
 Data File : BG062330.D
 Acq On : 8 Aug 2024 15:25
 Operator : MA/JU
 Sample : PB162447BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK447

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

37	23.555	3446	3450	3452	rBV4	3011	4346	0.22%	0.022%
38	23.608	3456	3459	3462	rBV4	3019	3697	0.18%	0.019%
39	23.825	3489	3496	3504	rVB2	28606	66846	3.32%	0.341%
40	24.430	3587	3599	3618	rBV2	730861	2012865	100.00%	10.272%
41	24.636	3623	3634	3645	rVV	515330	1413565	70.23%	7.214%
42	24.735	3645	3651	3662	rVB3	43893	109503	5.44%	0.559%
43	25.828	3828	3837	3845	rBV4	43827	126554	6.29%	0.646%
44	26.116	3883	3886	3887	rBV3	2488	2431	0.12%	0.012%
45	27.138	4049	4060	4074	rBV2	39941	135841	6.75%	0.693%
46	27.485	4117	4119	4122	rBV4	2566	3009	0.15%	0.015%
47	28.049	4213	4215	4217	rBV3	2604	2852	0.14%	0.015%
48	28.701	4314	4326	4327	rBV5	27786	58085	2.89%	0.296%
49	29.505	4461	4463	4466	rBV4	2853	3050	0.15%	0.016%
50	29.658	4487	4489	4492	rBV4	2192	2536	0.13%	0.013%
51	30.551	4638	4641	4642	rBV2	2991	3264	0.16%	0.017%
52	30.616	4642	4652	4665	rVB7	19984	88114	4.38%	0.450%
53	32.225	4925	4926	4927	rBV	3830	2347	0.12%	0.012%


Sum of corrected areas: 19595497

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062330.D
Acq On : 8 Aug 2024 15:25
Operator : MA/JU
Sample : PB162447BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK447

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

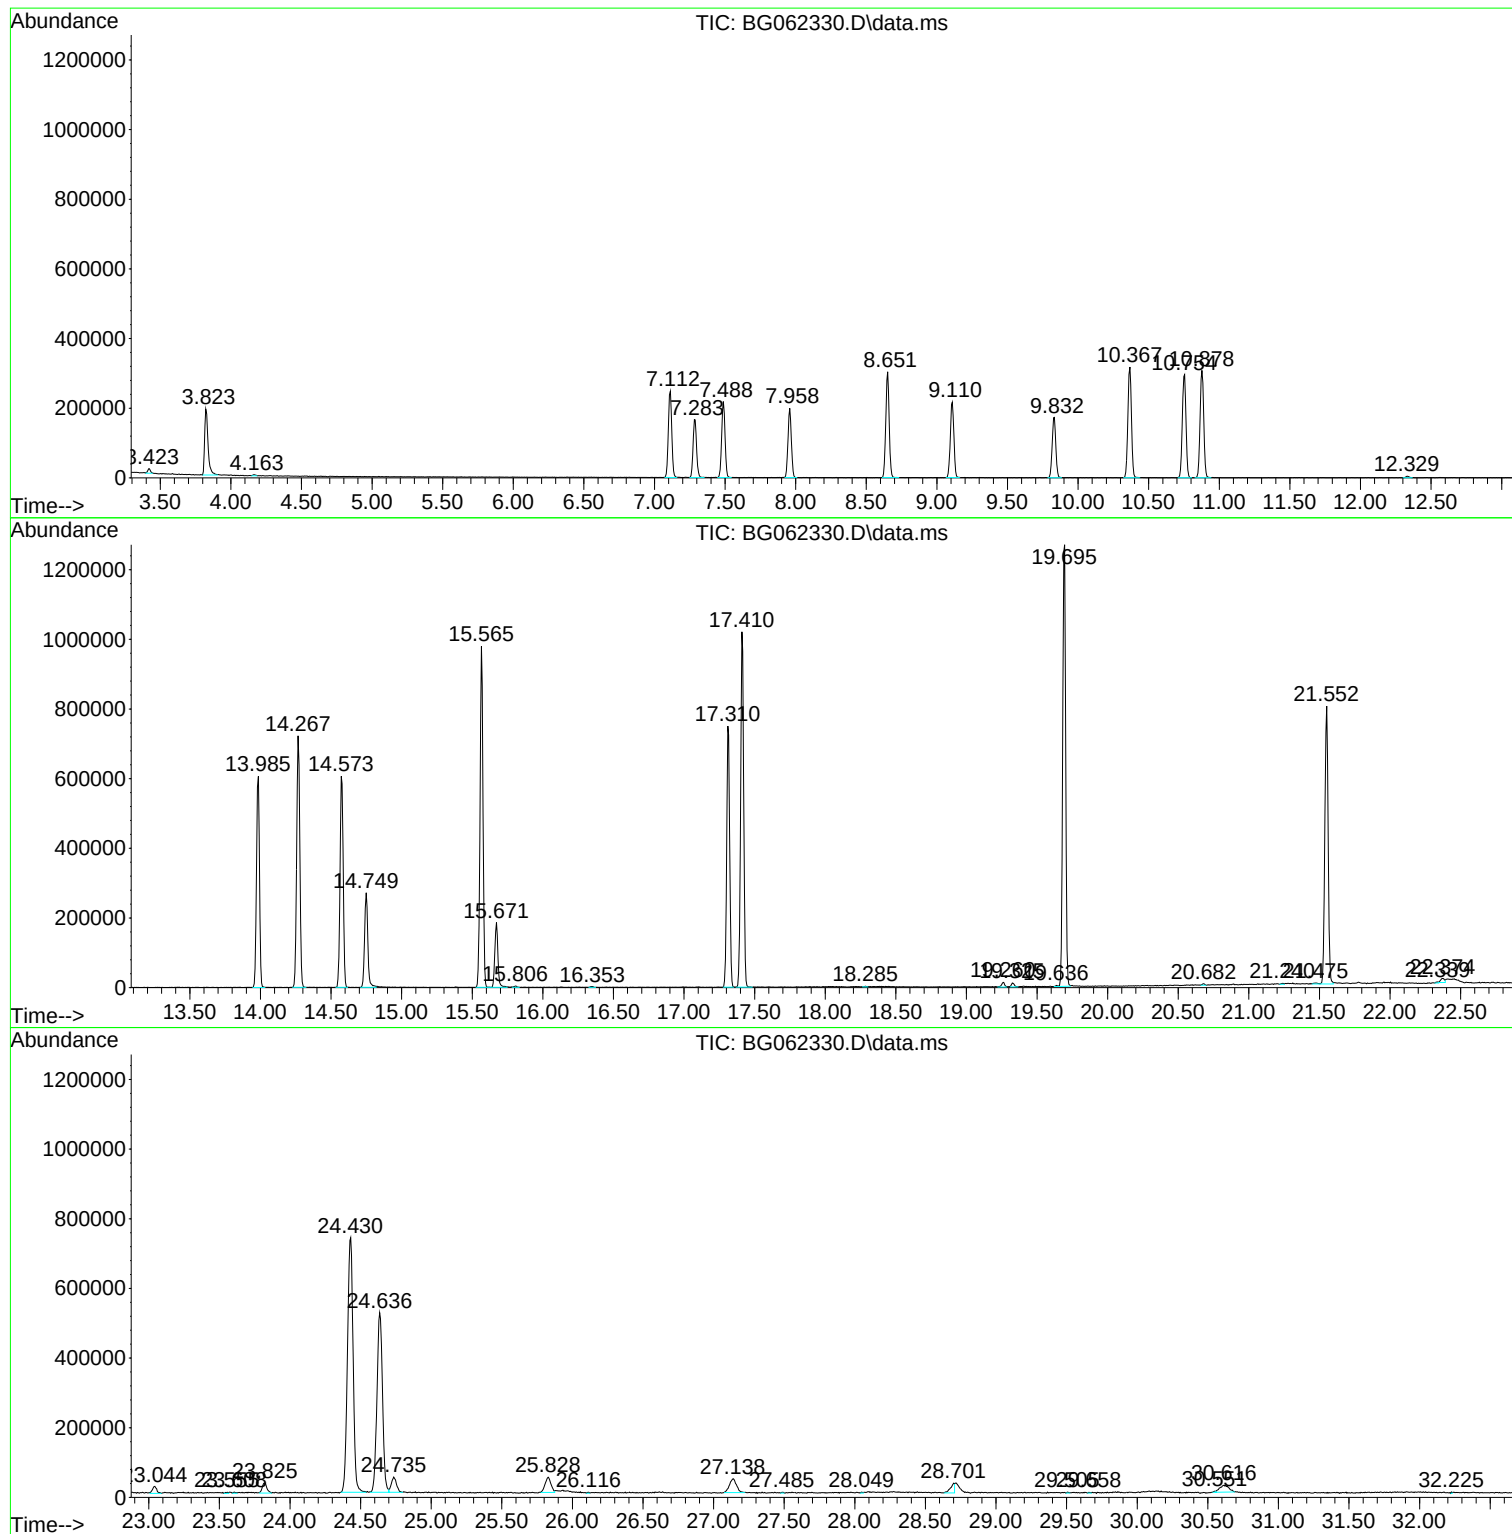

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062330.D
Acq On : 8 Aug 2024 15:25
Operator : MA/JU
Sample : PB162447BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK447

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062330.D
Acq On : 8 Aug 2024 15:25
Operator : MA/JU
Sample : PB162447BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK447

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc