

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
 Data File : BG062342.D
 Acq On : 9 Aug 2024 1:05
 Operator : MA/JU
 Sample : PB162448BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK448

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062342.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.417	19	22	30	rVB	18540	29037	1.15%	0.115%
2	3.822	86	91	104	rBV	252850	409460	16.24%	1.619%
3	4.168	146	150	154	rVB2	4545	5844	0.23%	0.023%
4	7.112	644	651	661	rBV	335520	549634	21.80%	2.173%
5	7.282	672	680	690	rBV	221519	372472	14.77%	1.472%
6	7.487	708	715	724	rBV	291561	491758	19.50%	1.944%
7	7.957	784	795	805	rBV	279454	471370	18.69%	1.863%
8	8.651	905	913	922	rBV	390017	679075	26.93%	2.685%
9	9.109	983	991	1001	rVB	293360	520968	20.66%	2.060%
10	9.825	1105	1113	1125	rVB	251341	441586	17.51%	1.746%
11	10.360	1197	1204	1220	rVB	415665	741049	29.39%	2.930%
12	10.748	1261	1270	1278	rBV	456595	796372	31.58%	3.148%
13	10.877	1284	1292	1303	rBV	427515	755696	29.97%	2.987%
14	12.334	1534	1540	1548	rVB4	6864	11054	0.44%	0.044%
15	13.979	1811	1820	1832	rBV	770750	1126317	44.67%	4.453%
16	14.267	1862	1869	1876	rBV	914883	1408796	55.87%	5.569%
17	14.572	1914	1921	1931	rVB	827571	1280832	50.80%	5.063%
18	14.748	1944	1951	1965	rBV	353591	574753	22.80%	2.272%
19	15.565	2083	2090	2097	rBV	1198980	1794884	71.19%	7.096%
20	15.671	2101	2108	2120	rBV	286024	428217	16.98%	1.693%
21	15.806	2126	2131	2136	rVB4	3944	6154	0.24%	0.024%
22	16.346	2220	2223	2227	rVB2	3344	3579	0.14%	0.014%
23	17.315	2380	2388	2395	rBV	1003834	1524529	60.46%	6.027%
24	17.409	2397	2404	2415	rBV2	1265121	1925185	76.35%	7.611%
25	19.260	2714	2719	2724	rBV2	17250	24686	0.98%	0.098%
26	19.324	2726	2730	2734	rBV	13488	19604	0.78%	0.077%
27	19.636	2780	2783	2786	rBV3	4092	4710	0.19%	0.019%
28	19.694	2786	2793	2802	rBV	1660540	2313875	91.77%	9.147%
29	20.675	2957	2960	2964	rVB4	6928	7851	0.31%	0.031%
30	21.028	3017	3020	3023	rBV5	2894	4068	0.16%	0.016%
31	21.140	3035	3039	3041	rBV4	2516	3923	0.16%	0.016%
32	21.551	3102	3109	3119	rBV2	1077436	1749636	69.39%	6.917%
33	21.768	3142	3146	3149	rBV4	5021	6865	0.27%	0.027%
34	21.839	3157	3158	3160	rBV2	3037	2585	0.10%	0.010%
35	21.956	3176	3178	3183	rVB6	3087	3448	0.14%	0.014%
36	22.361	3243	3247	3254	rBV8	9572	18469	0.73%	0.073%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
 Data File : BG062342.D
 Acq On : 9 Aug 2024 1:05
 Operator : MA/JU
 Sample : PB162448BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK448

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

37	23.037	3357	3362	3366	rBV5	10242	17414	0.69%	0.069%
38	23.184	3385	3387	3391	rBV4	2551	3769	0.15%	0.015%
39	23.818	3489	3495	3502	rVB4	16031	34051	1.35%	0.135%
40	24.429	3587	3599	3615	rBV2	929279	2521387	100.00%	9.968%
41	24.641	3623	3635	3644	rBV	700150	1930914	76.58%	7.633%
42	24.735	3647	3651	3658	rVB4	26120	53755	2.13%	0.213%
43	25.722	3817	3819	3822	rBV3	2788	2884	0.11%	0.011%
44	25.821	3828	3836	3847	rBV3	24925	77814	3.09%	0.308%
45	26.333	3921	3923	3925	rBV2	2746	2818	0.11%	0.011%
46	26.391	3931	3933	3936	rBV3	3384	4415	0.18%	0.017%
47	27.131	4052	4059	4070	rVB5	21889	70069	2.78%	0.277%
48	28.065	4217	4218	4220	rBV2	3517	2571	0.10%	0.010%
49	28.365	4268	4269	4272	rBV3	3013	2790	0.11%	0.011%
50	28.694	4316	4325	4336	rVB9	13927	53700	2.13%	0.212%
51	30.562	4641	4643	4644	rBV2	4429	3107	0.12%	0.012%
52	30.586	4645	4647	4648	rVB	4445	2750	0.11%	0.011%
53	31.343	4774	4776	4777	rBV2	3707	3120	0.12%	0.012%




Sum of corrected areas: 25295669

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062342.D
Acq On : 9 Aug 2024 1:05
Operator : MA/JU
Sample : PB162448BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK448

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

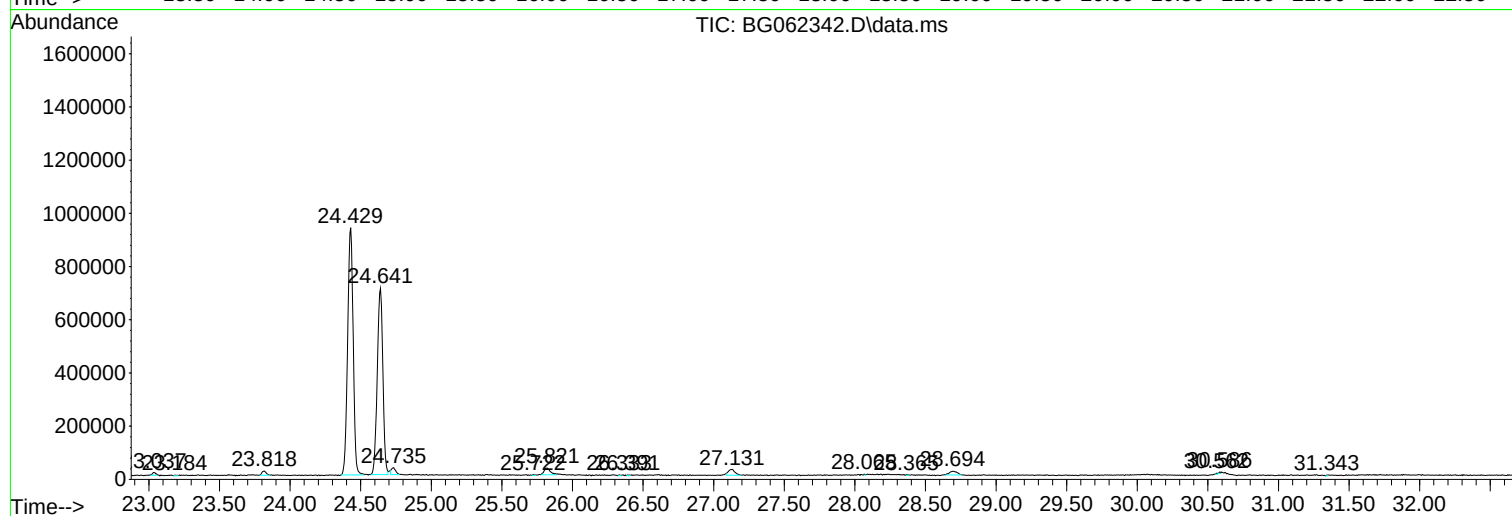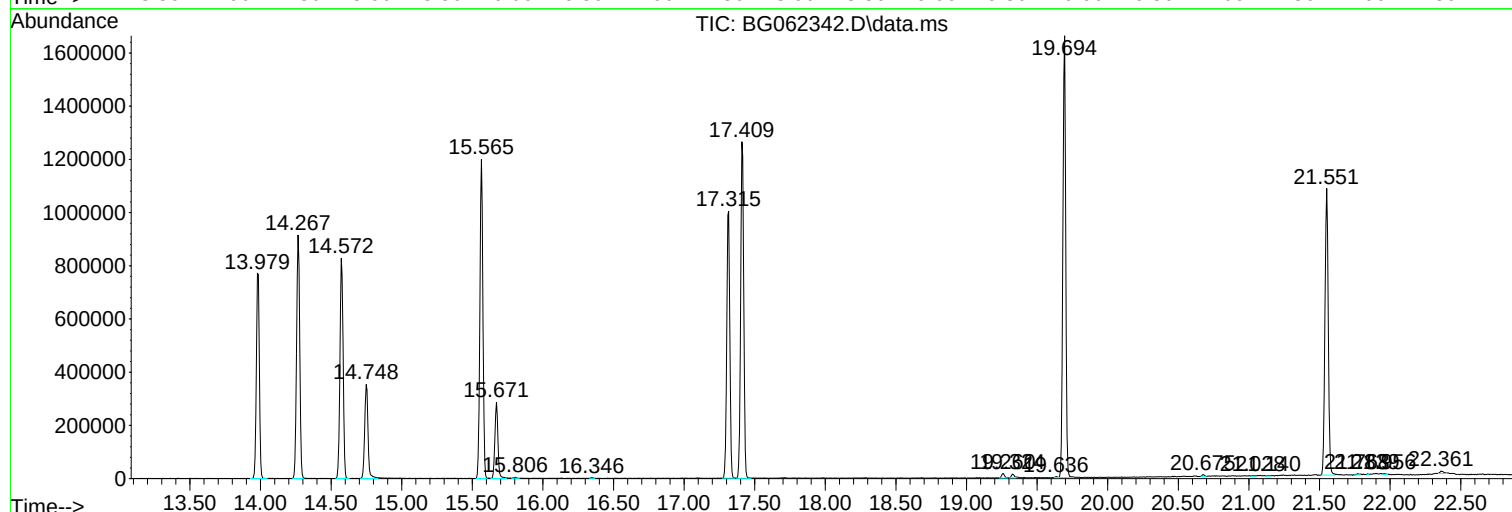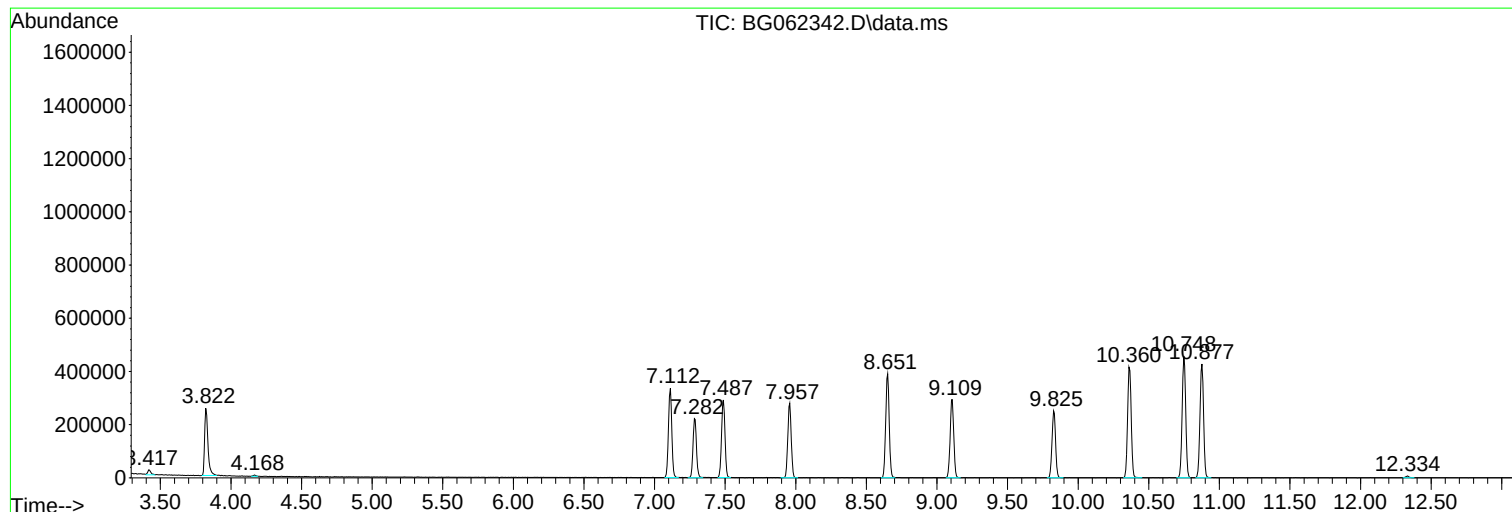

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062342.D
Acq On : 9 Aug 2024 1:05
Operator : MA/JU
Sample : PB162448BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK448

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062342.D
Acq On : 9 Aug 2024 1:05
Operator : MA/JU
Sample : PB162448BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK448

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------