

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
 Data File : BG062352.D
 Acq On : 9 Aug 2024 9:08
 Operator : MA/JU
 Sample : PB162597BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK597

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062352.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.417	19	22	30	rVB2	11565	18926	1.09%	0.118%
2	3.822	87	91	109	rBV	170936	293825	16.85%	1.830%
3	7.106	643	650	660	rBV	233329	396837	22.75%	2.471%
4	7.282	674	680	691	rBV	159695	266055	15.25%	1.657%
5	7.488	706	715	723	rBV	197419	347052	19.90%	2.161%
6	7.952	788	794	804	rVB	147102	253236	14.52%	1.577%
7	8.651	906	913	921	rBV	286362	484059	27.75%	3.014%
8	9.109	982	991	998	rBV	195698	354179	20.31%	2.205%
9	9.826	1104	1113	1120	rBV	176197	304866	17.48%	1.898%
10	10.366	1197	1205	1214	rBV	290924	517511	29.67%	3.222%
11	10.748	1263	1270	1278	rVB	230272	407633	23.37%	2.538%
12	10.877	1285	1292	1300	rBV	295237	534023	30.62%	3.325%
13	12.328	1535	1539	1547	rVB2	3486	6334	0.36%	0.039%
14	13.985	1814	1821	1827	rBV	525085	765953	43.92%	4.769%
15	14.267	1862	1869	1877	rBV2	608301	965957	55.38%	6.015%
16	14.578	1913	1922	1930	rBV	406733	639626	36.67%	3.983%
17	14.748	1945	1951	1967	rBV	228020	389371	22.32%	2.425%
18	15.565	2083	2090	2098	rBV	803380	1222331	70.08%	7.611%
19	15.671	2102	2108	2118	rBV	182092	270796	15.53%	1.686%
20	16.352	2219	2224	2228	rBV4	2482	3201	0.18%	0.020%
21	17.315	2381	2388	2396	rBV	498593	737308	42.27%	4.591%
22	17.415	2398	2405	2412	rBV2	870395	1318099	75.57%	8.208%
23	17.709	2449	2455	2460	rVB3	3064	5796	0.33%	0.036%
24	18.214	2538	2541	2548	rBV4	2239	4364	0.25%	0.027%
25	18.285	2548	2553	2557	rBV2	1922	3222	0.18%	0.020%
26	19.266	2714	2720	2726	rVB2	11690	16820	0.96%	0.105%
27	19.330	2726	2731	2735	rBV2	10937	17334	0.99%	0.108%
28	19.360	2735	2736	2740	rVB2	5445	4779	0.27%	0.030%
29	19.636	2781	2783	2787	rVB4	2199	2751	0.16%	0.017%
30	19.695	2787	2793	2802	rBV	1160895	1601189	91.80%	9.970%
31	20.041	2848	2852	2853	rBV3	2035	2144	0.12%	0.013%
32	20.329	2898	2901	2904	rVB2	2100	2475	0.14%	0.015%
33	20.352	2904	2905	2909	rBV3	2005	2261	0.13%	0.014%
34	20.546	2936	2938	2939	rBV2	2101	1911	0.11%	0.012%
35	20.617	2948	2950	2954	rBV3	2610	3251	0.19%	0.020%
36	20.681	2958	2961	2966	rVV7	3404	4228	0.24%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
 Data File : BG062352.D
 Acq On : 9 Aug 2024 9:08
 Operator : MA/JU
 Sample : PB162597BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK597

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

37	21.034	3020	3021	3024	rBV3	2099	2336	0.13%	0.015%
38	21.140	3037	3039	3042	rBV3	2634	2254	0.13%	0.014%
39	21.245	3055	3057	3059	rBV3	2547	2115	0.12%	0.013%
40	21.469	3093	3095	3099	rVB5	4983	4924	0.28%	0.031%
41	21.557	3103	3110	3116	rBV2	534282	873799	50.10%	5.441%
42	21.756	3142	3144	3145	rBV2	2809	1855	0.11%	0.012%
43	21.780	3145	3148	3151	rVV5	4196	5679	0.33%	0.035%
44	21.897	3166	3168	3173	rBV6	2557	4233	0.24%	0.026%
45	21.939	3173	3175	3178	rBV4	2590	3255	0.19%	0.020%
46	22.373	3244	3249	3251	rBV6	9331	15103	0.87%	0.094%
47	23.043	3358	3363	3372	rVB5	12137	25554	1.47%	0.159%
48	23.818	3490	3495	3503	rVB3	17366	36435	2.09%	0.227%
49	24.429	3588	3599	3613	rBV2	642644	1744166	100.00%	10.861%
50	24.641	3624	3635	3645	rBV	335104	937986	53.78%	5.841%
51	24.735	3645	3651	3661	rVB2	25051	60457	3.47%	0.376%
52	24.940	3684	3686	3688	rBV3	3641	3859	0.22%	0.024%
53	25.040	3702	3703	3707	rBV4	2977	3147	0.18%	0.020%
54	25.822	3829	3836	3845	rBV5	24011	67511	3.87%	0.420%
55	26.321	3919	3921	3922	rBV2	2823	1929	0.11%	0.012%
56	27.132	4051	4059	4066	rVB5	18760	51792	2.97%	0.322%
57	27.455	4112	4114	4117	rBV3	3000	2863	0.16%	0.018%
58	28.624	4311	4313	4314	rBV2	3469	2567	0.15%	0.016%
59	28.700	4319	4326	4327	rBV7	8396	17472	1.00%	0.109%
60	29.669	4489	4491	4492	rBV	2773	1941	0.11%	0.012%
61	30.169	4574	4576	4581	rVB6	4278	4811	0.28%	0.030%
62	30.445	4622	4623	4626	rVB3	3516	2066	0.12%	0.013%
63	30.874	4695	4696	4698	rBV2	2511	2172	0.12%	0.014%
64	31.103	4733	4735	4739	rBV4	2841	3311	0.19%	0.021%
65	32.037	4892	4894	4895	rBV2	2446	1758	0.10%	0.011%
66	32.477	4967	4969	4970	rBV2	2799	2581	0.15%	0.016%




Sum of corrected areas: 16059634

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062352.D
Acq On : 9 Aug 2024 9:08
Operator : MA/JU
Sample : PB162597BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK597

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

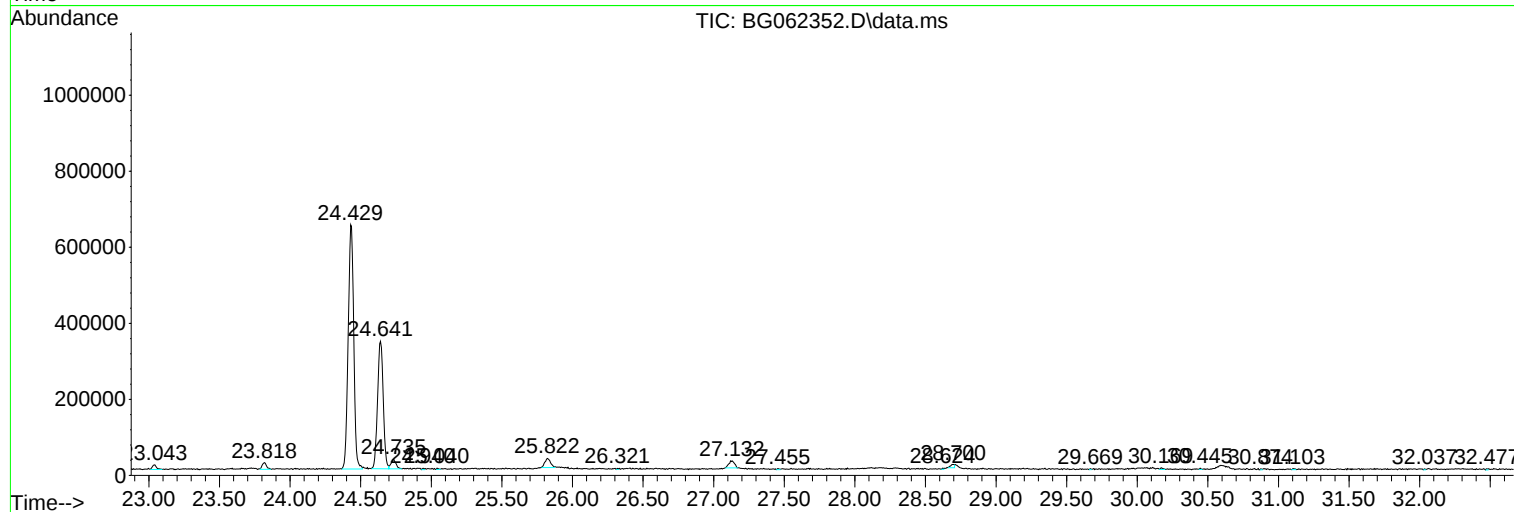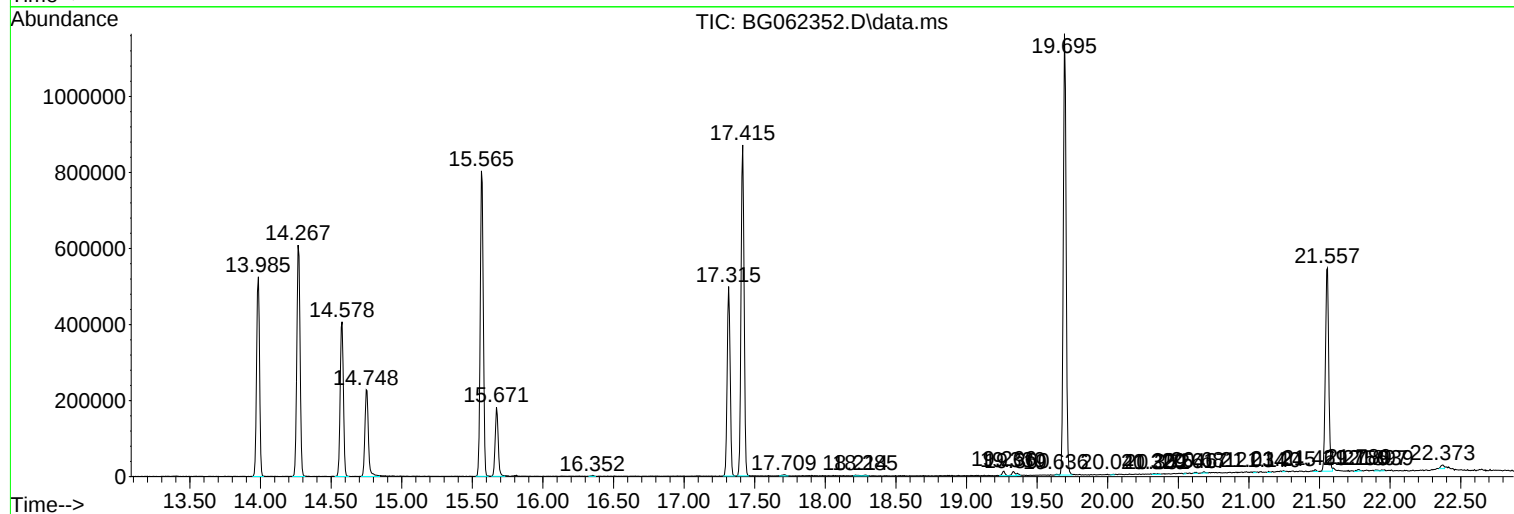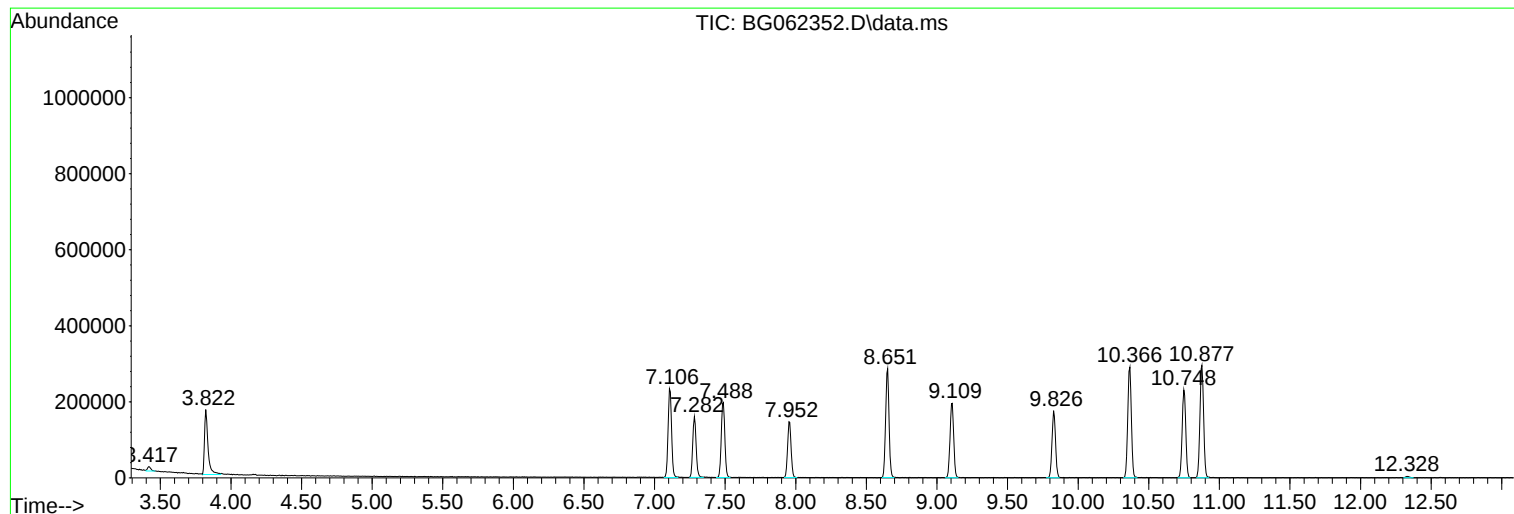

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062352.D
Acq On : 9 Aug 2024 9:08
Operator : MA/JU
Sample : PB162597BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK597

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080824\
Data File : BG062352.D
Acq On : 9 Aug 2024 9:08
Operator : MA/JU
Sample : PB162597BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK597

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc