
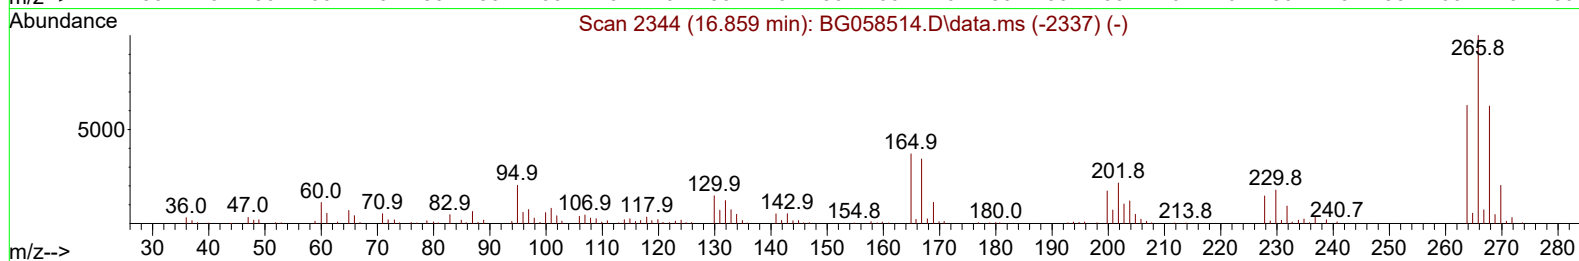
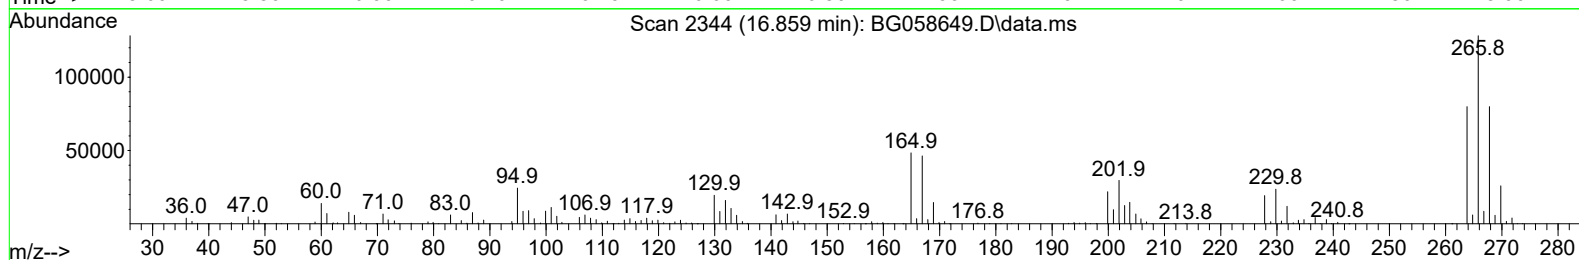


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080923\
Data File : BG058649.D
Acq On : 9 Aug 2023 7:39
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 08:14:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

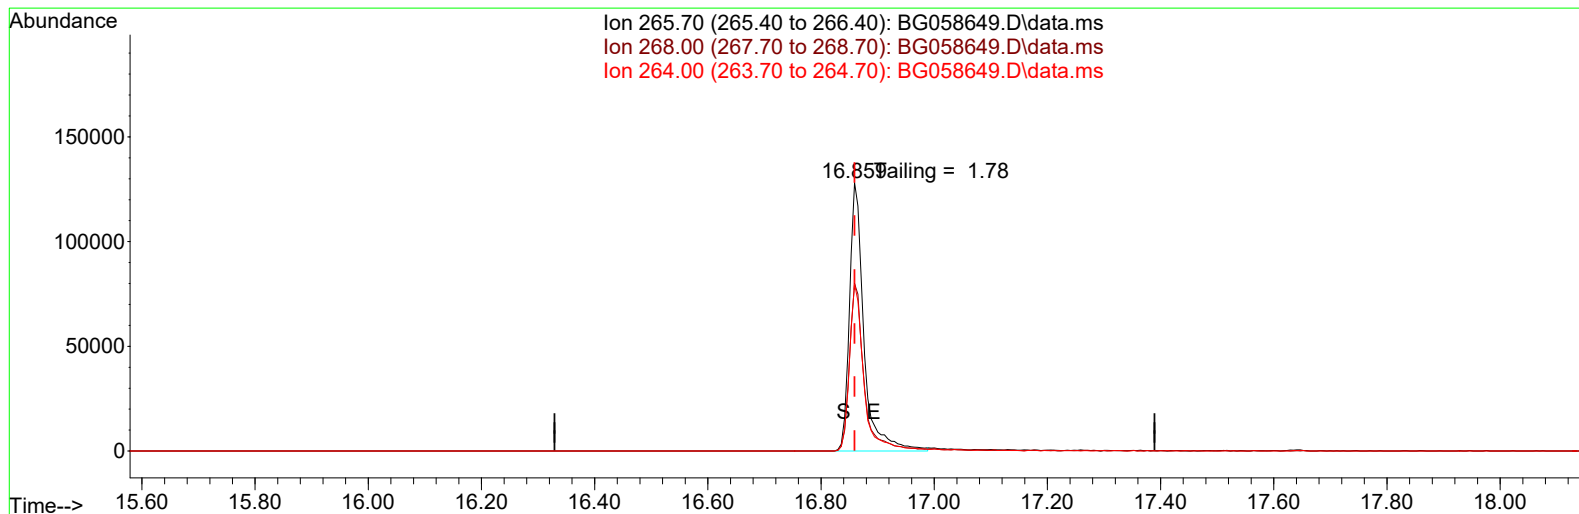

TIC: BG058649.D\data.ms

(70) Pentachlorophenol (C)




16.859min (+ 0.000) 26112.22 ng

response 227570

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	62.35
264.00	62.80	62.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080923\
 Data File : BG058649.D
 Acq On : 9 Aug 2023 7:39
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 08:14:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 28 22:29:07 2023
 Response via : Initial Calibration

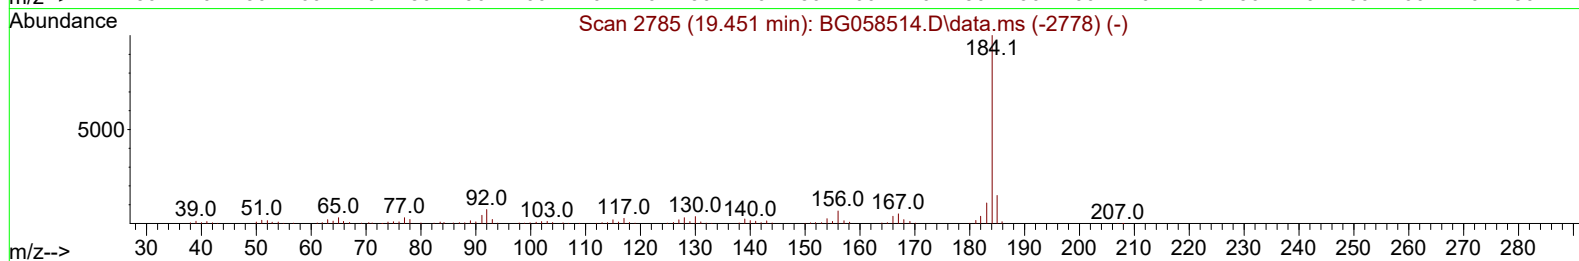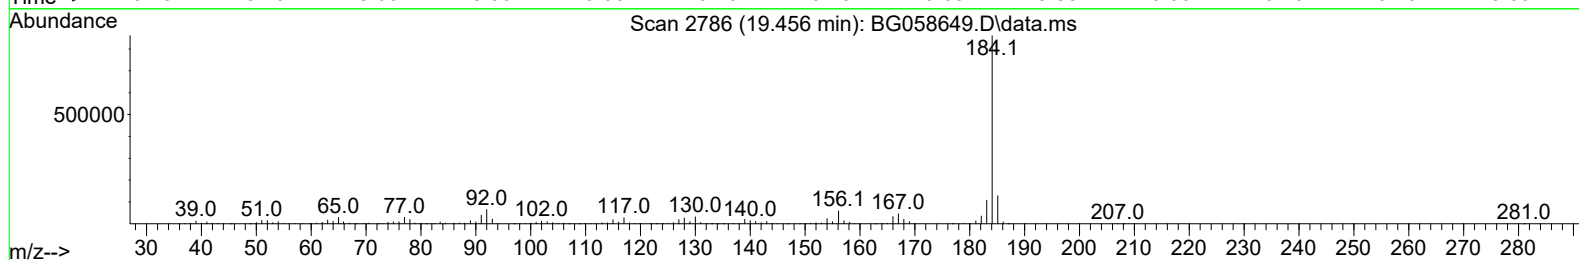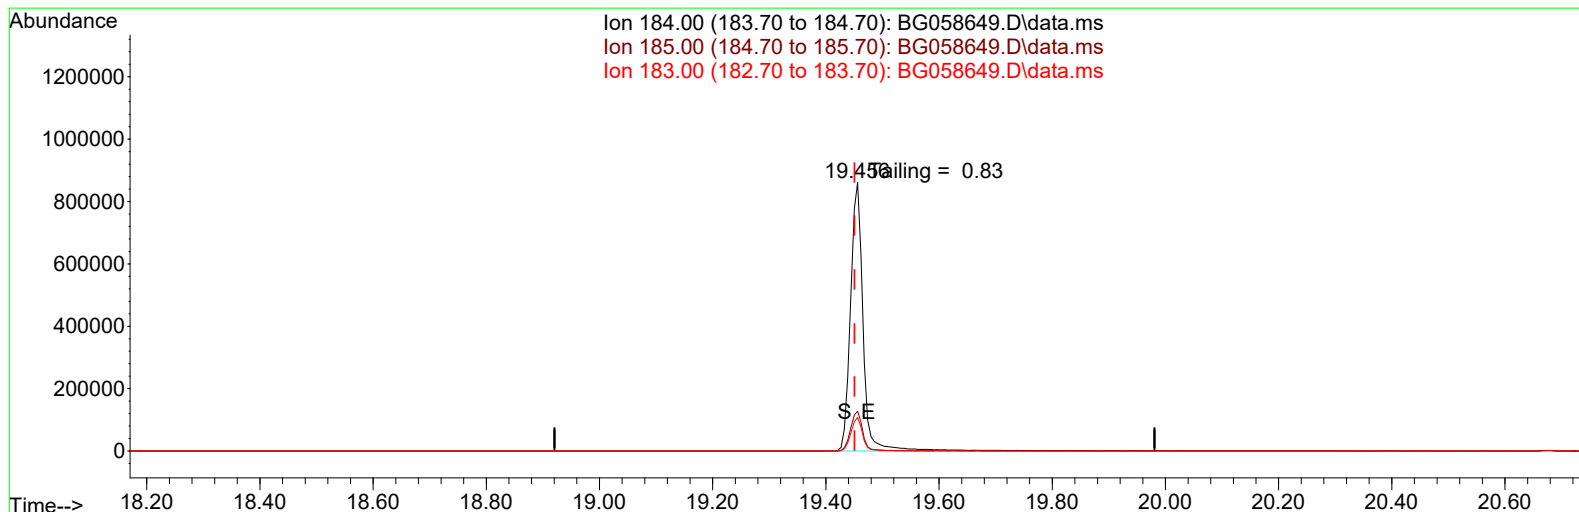

TIC: BG058649.D\data.ms

(77) Benzidine

19.456min (+ 0.006) 0.00 ng

response 1332377

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.88
183.00	10.90	12.49
0.00	0.00	0.00