
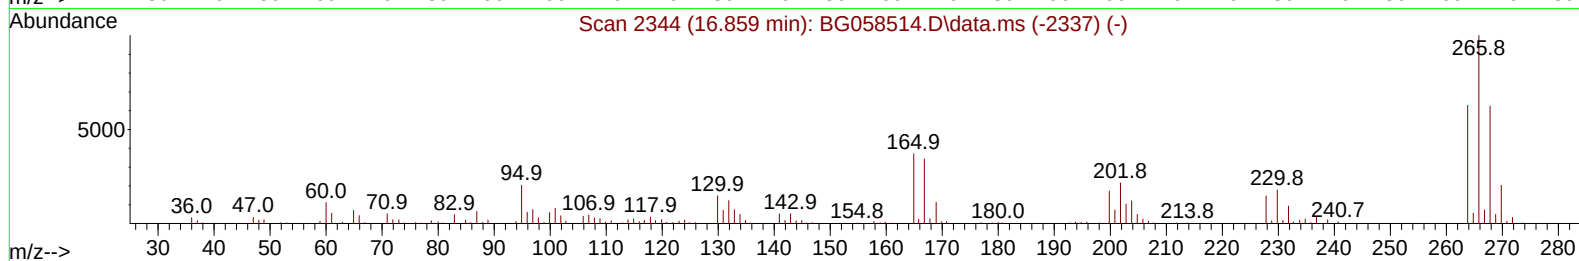
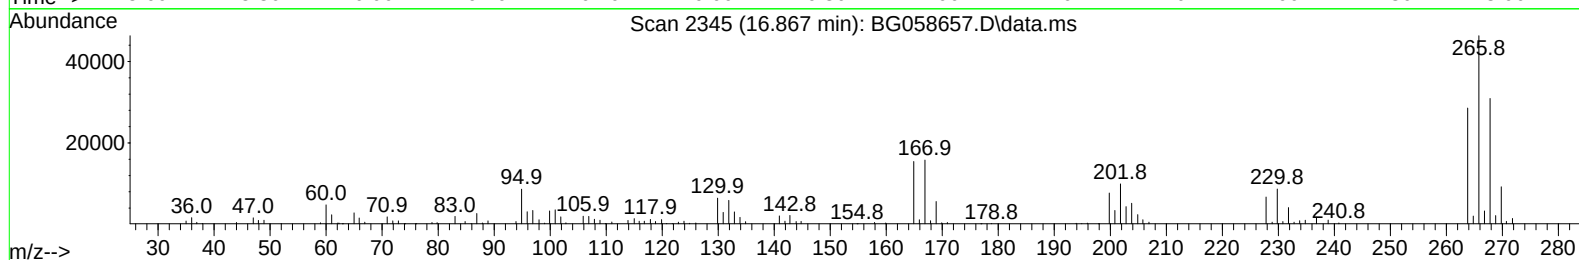


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080923\
Data File : BG058657.D
Acq On : 9 Aug 2023 13:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 14:22:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

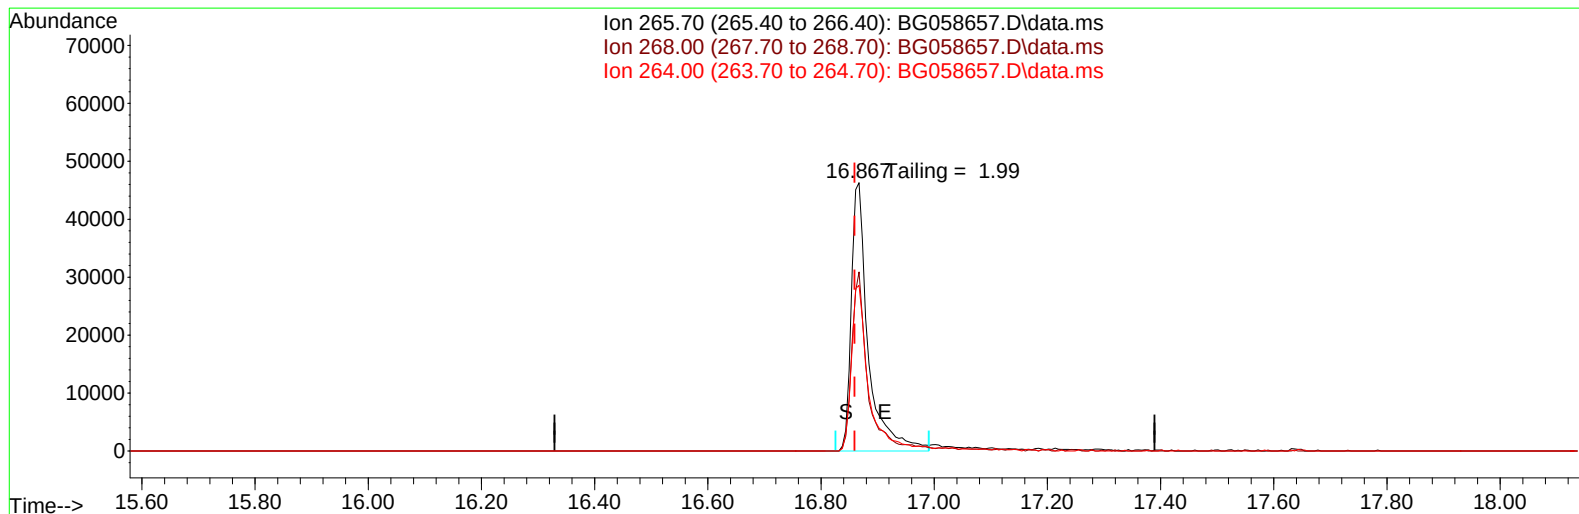

TIC: BG058657.D\data.ms

(70) Pentachlorophenol (C)




16.867min (+ 0.008) 26318.42 ng

response 96495

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	66.74
264.00	62.80	61.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080923\
Data File : BG058657.D
Acq On : 9 Aug 2023 13:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 14:22:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

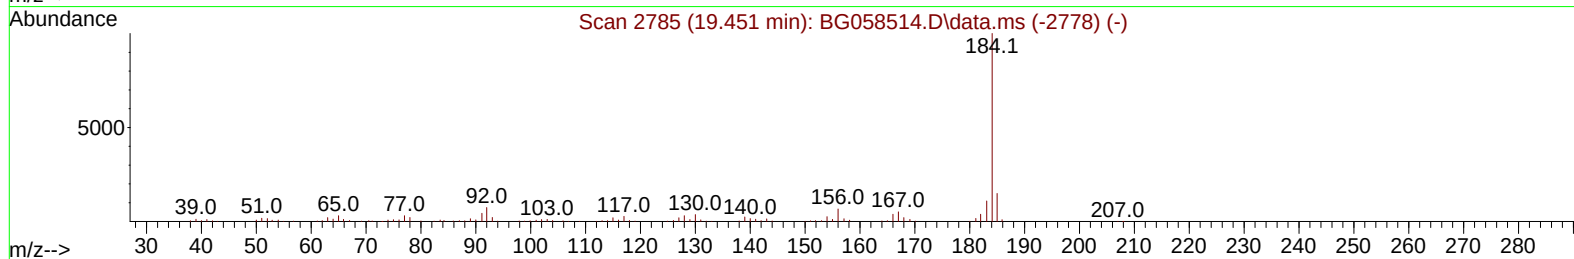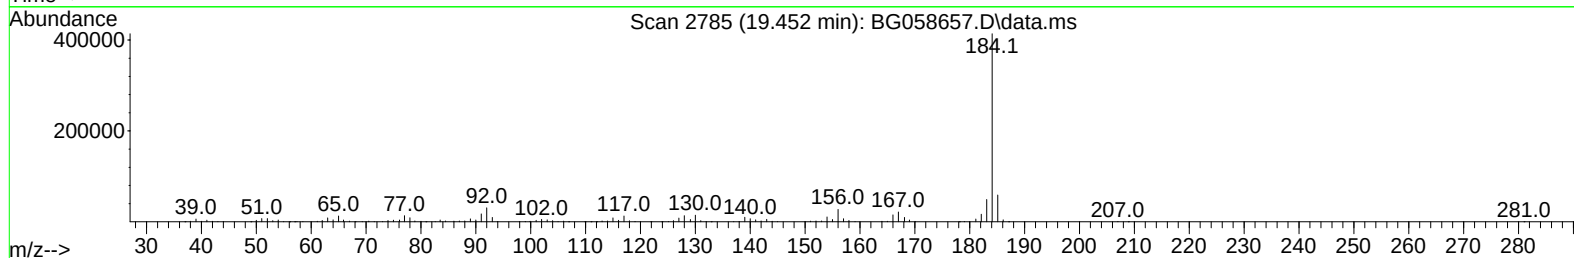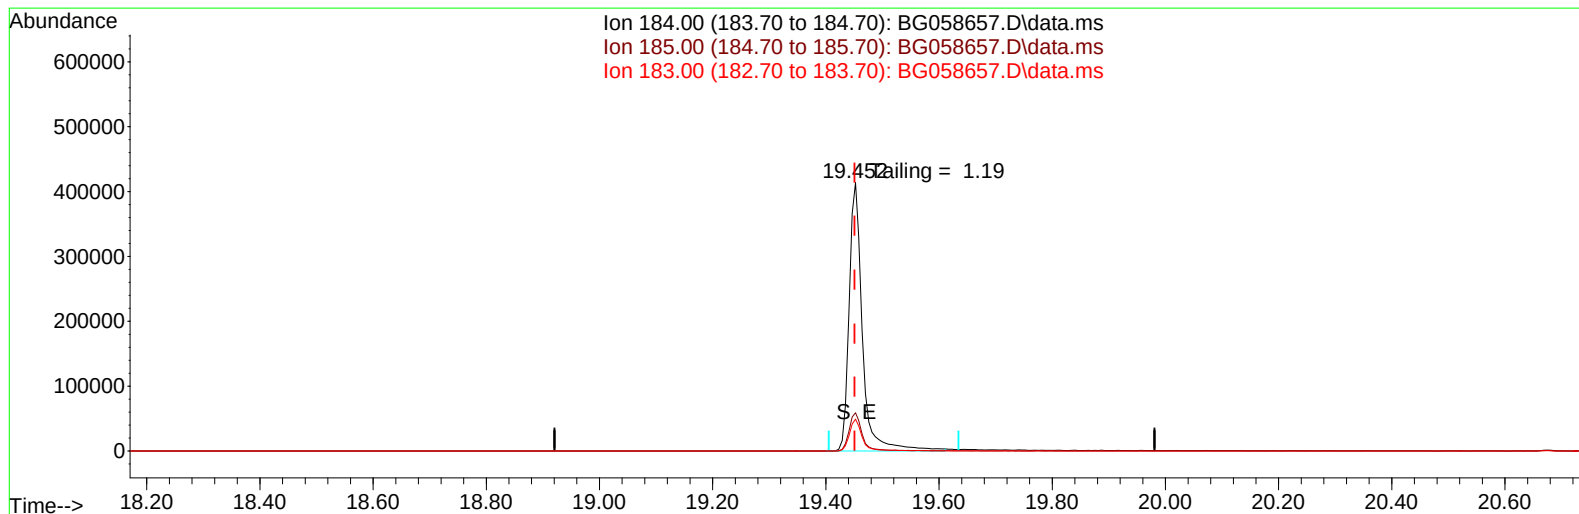

TIC: BG058657.D\data.ms

(77) Benzidine

19.452min (+ 0.002) 0.00 ng

response 682317

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.28
183.00	10.90	11.90
0.00	0.00	0.00