


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080923\
Data File : BG058649.D
Acq On : 9 Aug 2023 7:39
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 28 22:29:07 2023

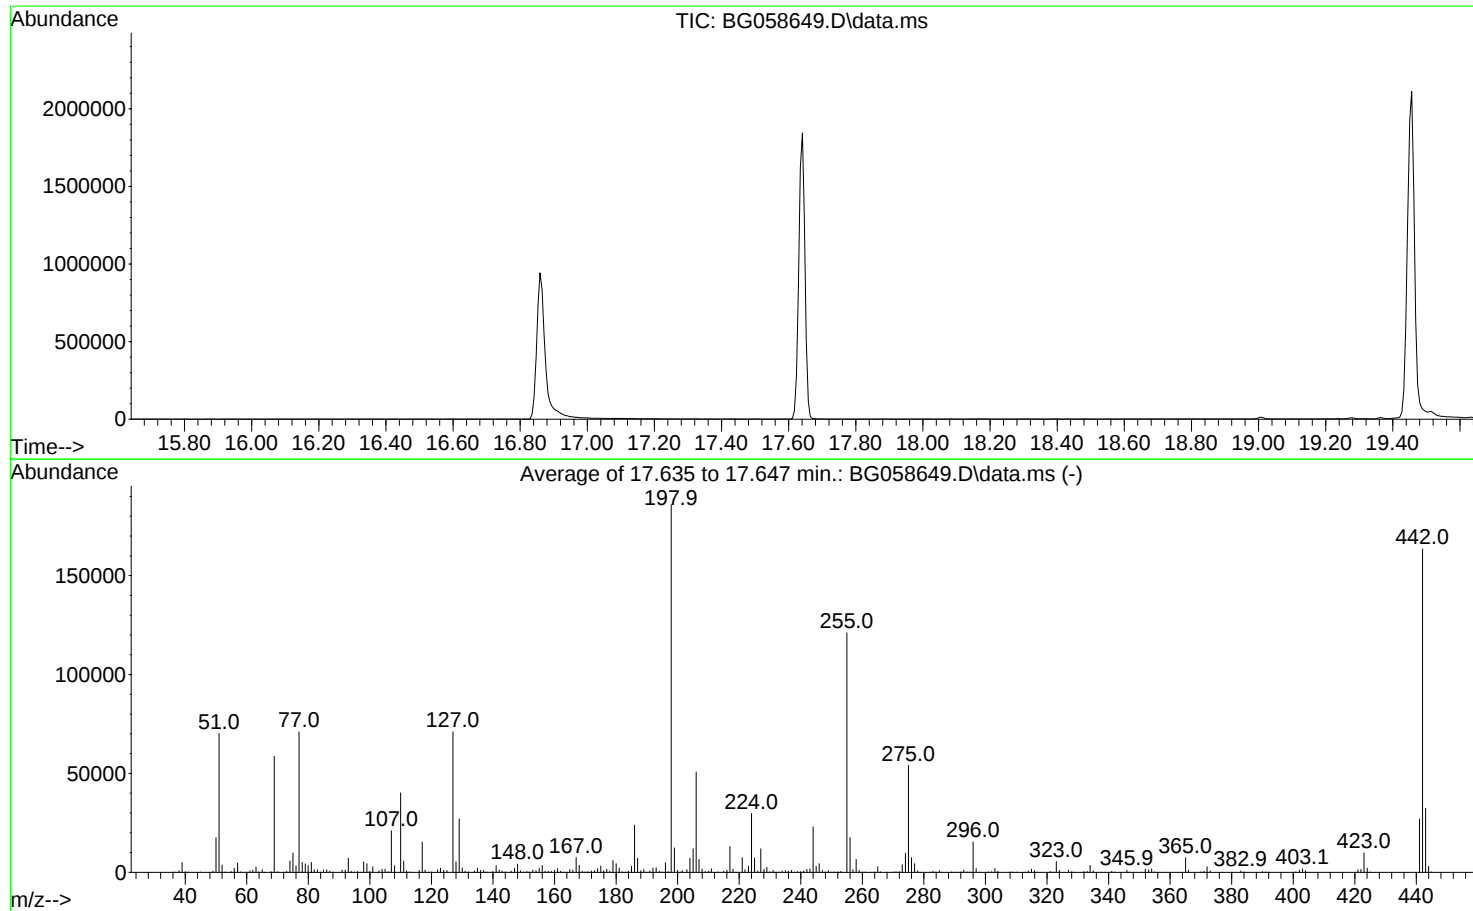




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.8	70211	PASS
68	69	0.00	2	0.6	353	PASS
69	198	0.00	100	31.6	58744	PASS
70	69	0.00	2	0.6	355	PASS
127	198	10	80	38.2	71040	PASS
197	198	0.00	2	0.2	408	PASS
198	198	100	100	100.0	185941	PASS
199	198	5	9	6.7	12386	PASS
275	198	10	60	29.0	54008	PASS
365	198	1	100	4.0	7384	PASS
441	198	0.01	100	14.5	26973	PASS
442	442	50	100	100.0	163456	PASS
443	442	15	24	19.8	32355	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080923\
Data File : BG058649.D
Acq On : 9 Aug 2023 7:39
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 09 08:14:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

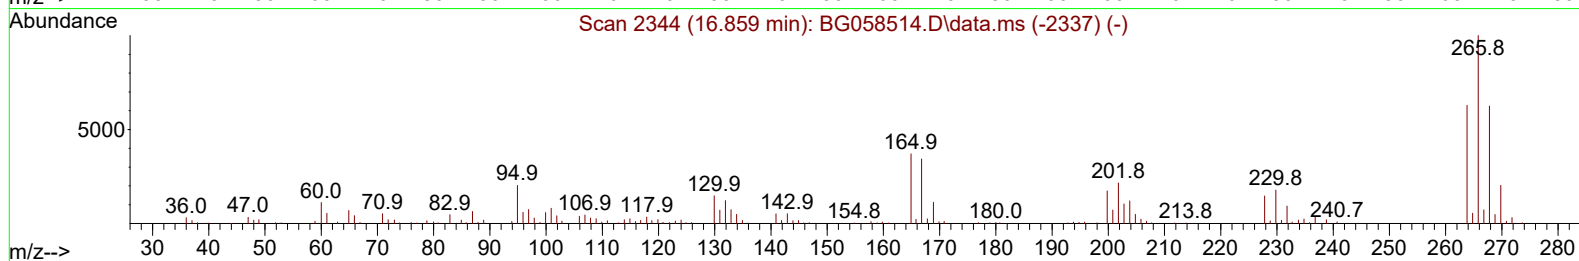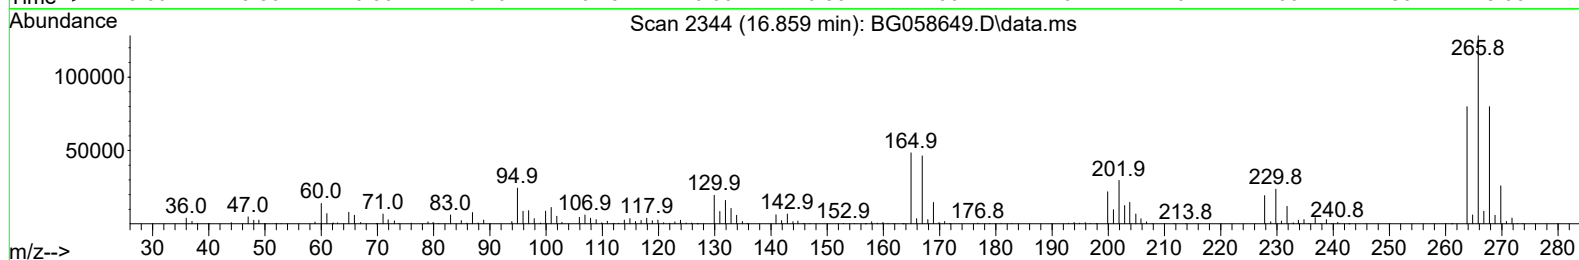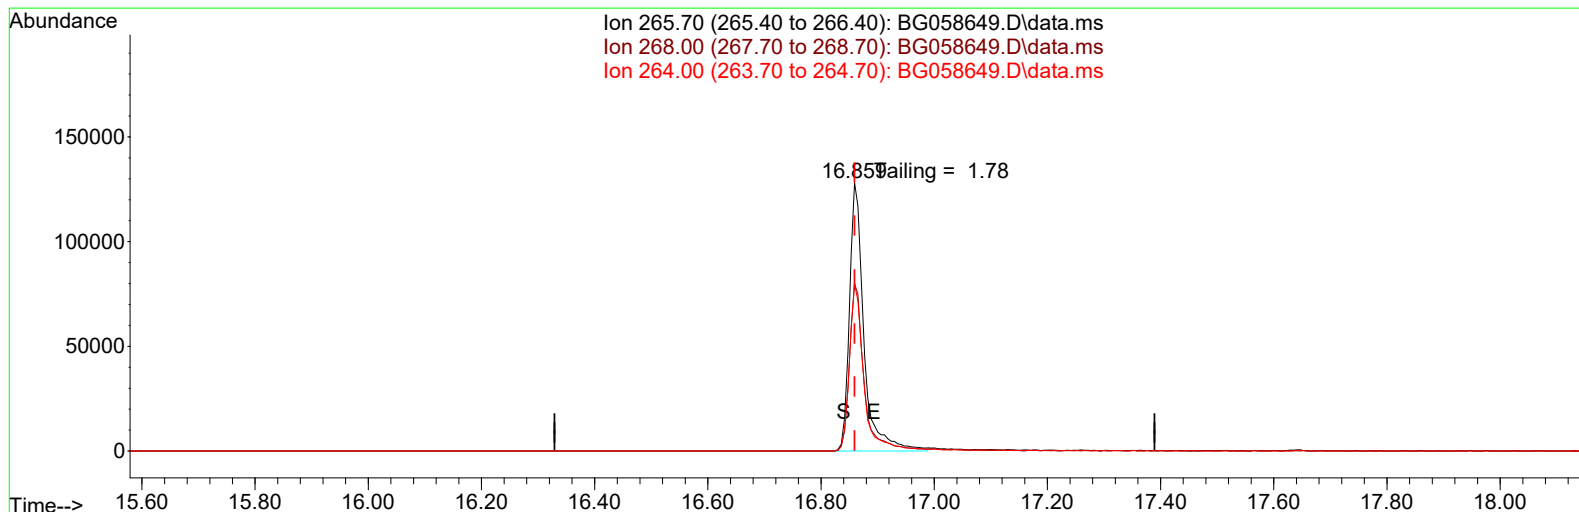

TIC: BG058649.D\data.ms

(70) Pentachlorophenol (C)

16.859min (+ 0.000) 26112.22 ng




response 227570

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	62.35
264.00	62.80	62.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080923\
Data File : BG058649.D
Acq On : 9 Aug 2023 7:39
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 09 08:14:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

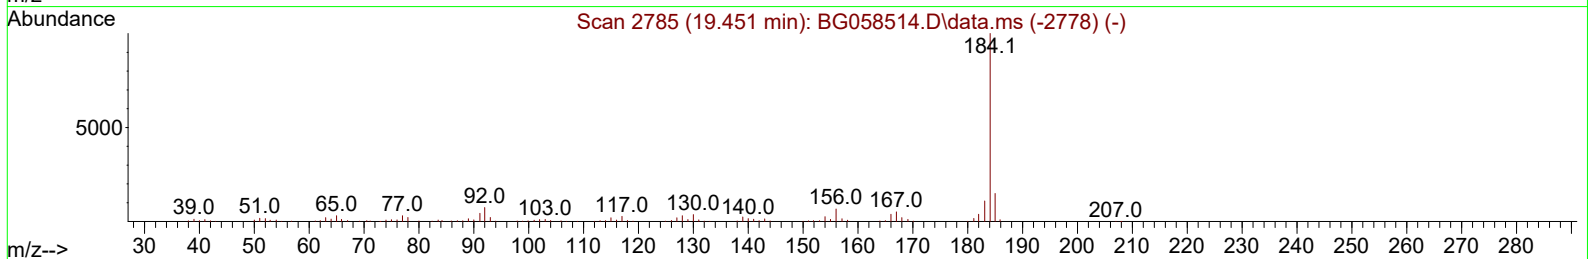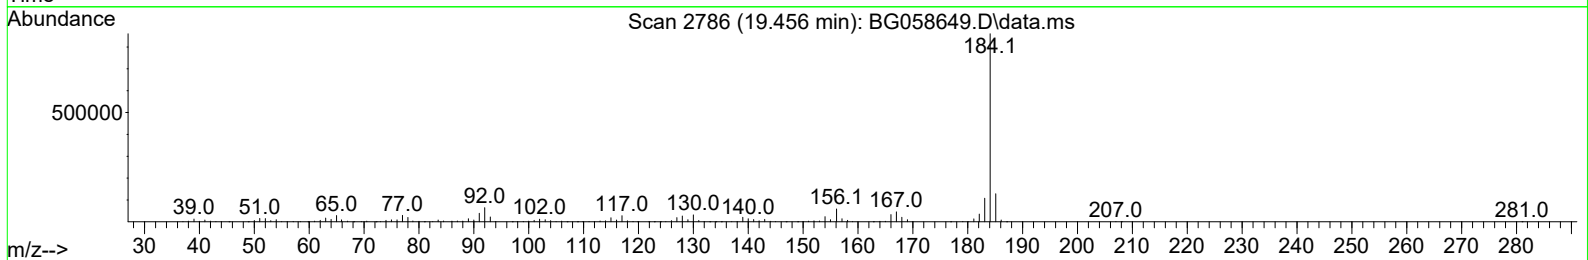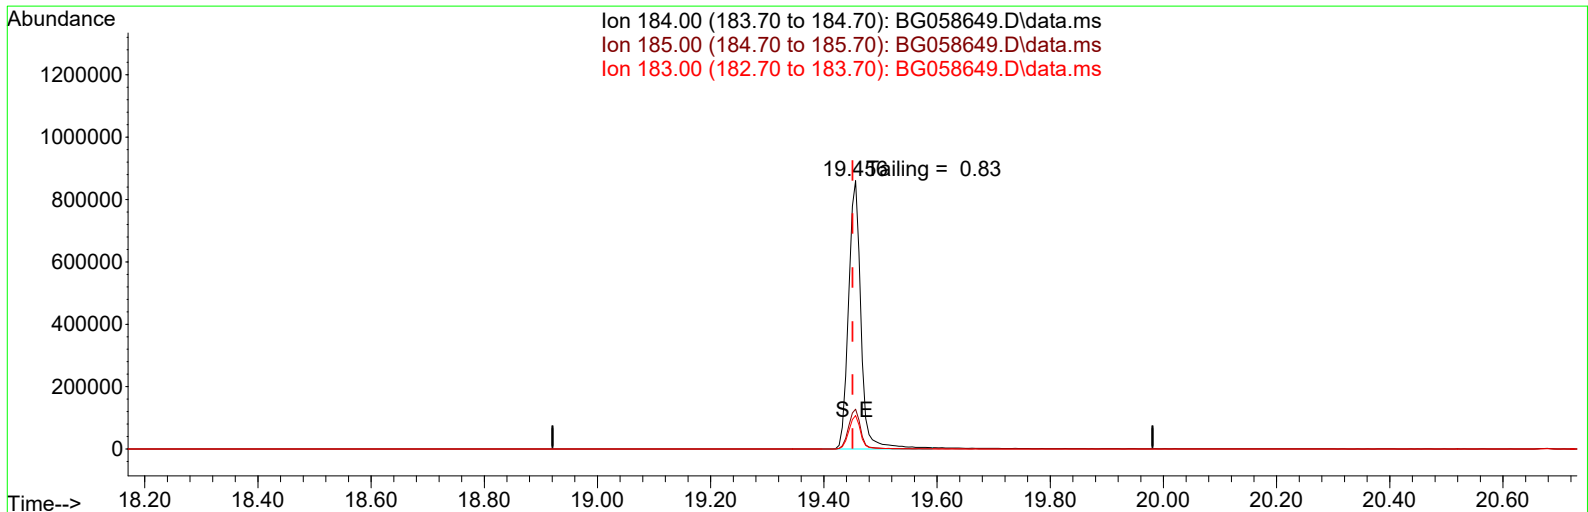

TIC: BG058649.D\data.ms

(77) Benzidine

19.456min (+ 0.006) 0.00 ng

response 1332377

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.88
183.00	10.90	12.49
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/9/2023	BNA_G	<u>BG058649.D</u>
Compound Name	Response	Retention Time
DDT	653680	20.678
DDD	14714	20.238
DDE	1542	19.732
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16256	669936	2.43

Instrument :
BNA_G
ClientSampleId :
DFTPP