


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080923\
Data File : BG058657.D
Acq On : 9 Aug 2023 13:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 28 22:29:07 2023

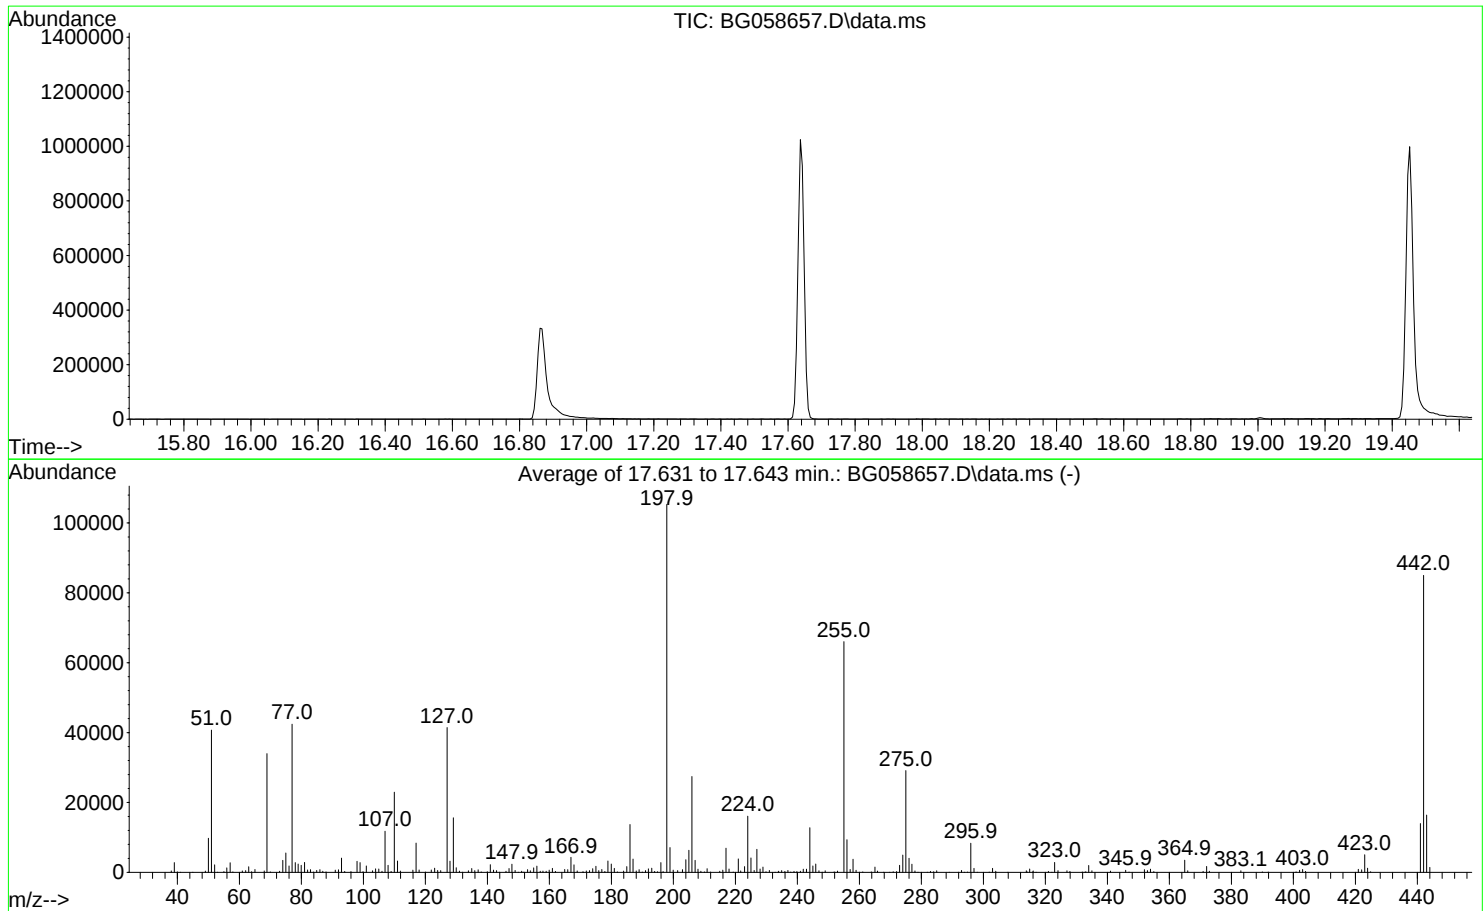




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	40728	PASS
68	69	0.00	2	1.3	438	PASS
69	198	0.00	100	32.3	33984	PASS
70	69	0.00	2	0.5	159	PASS
127	198	10	80	39.4	41467	PASS
197	198	0.00	2	0.2	237	PASS
198	198	100	100	100.0	105277	PASS
199	198	5	9	6.7	7090	PASS
275	198	10	60	27.7	29133	PASS
365	198	1	100	3.3	3503	PASS
441	198	0.01	100	13.3	13981	PASS
442	442	50	100	100.0	84997	PASS
443	442	15	24	19.3	16384	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080923\
Data File : BG058657.D
Acq On : 9 Aug 2023 13:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 09 14:22:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

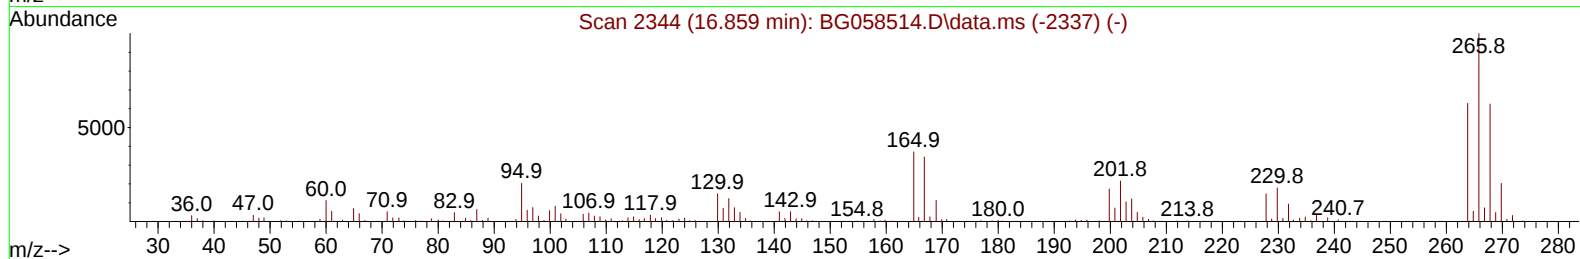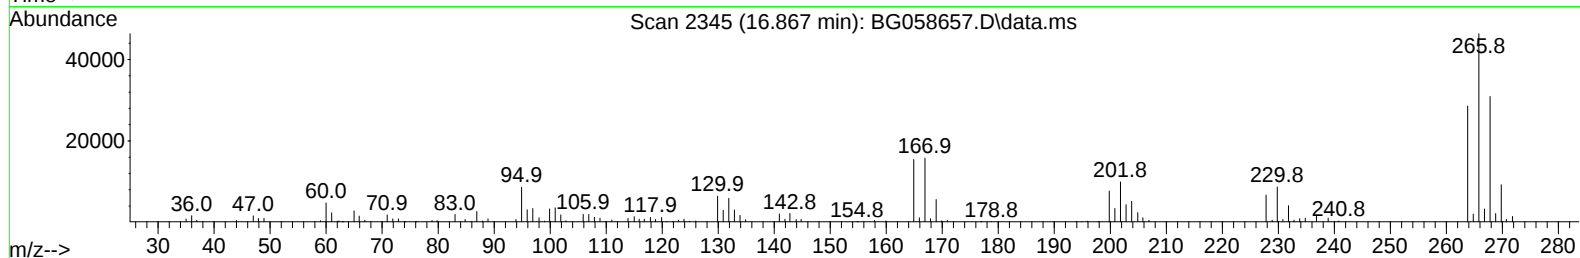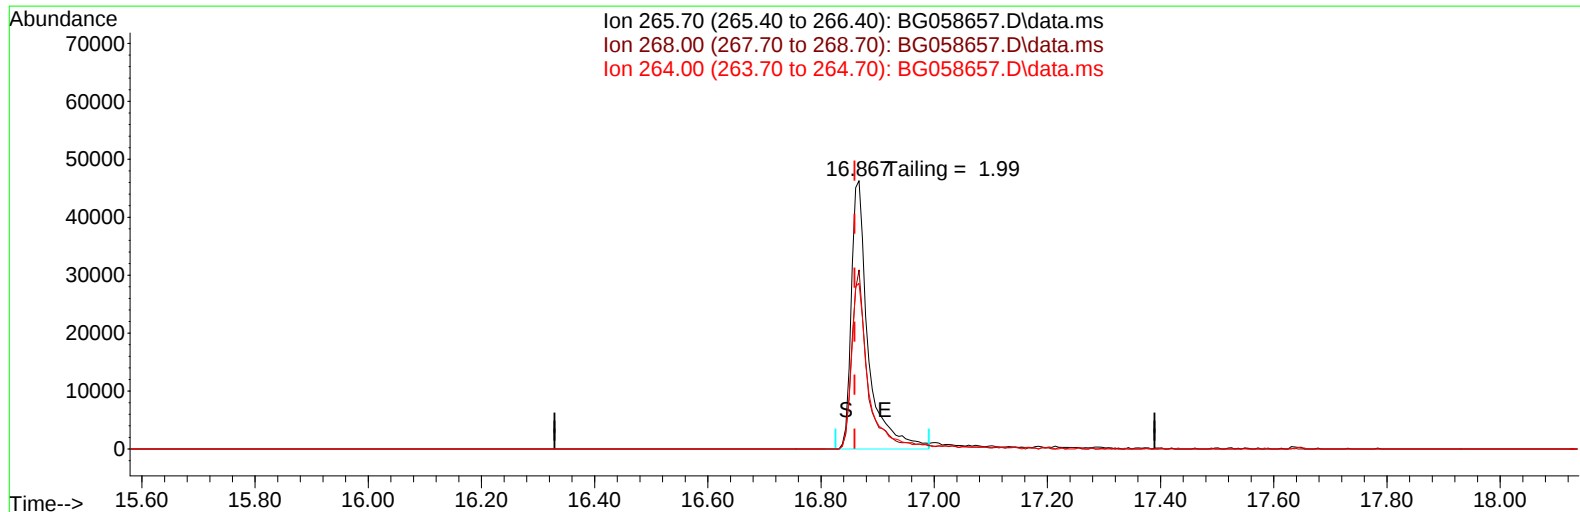

TIC: BG058657.D\data.ms

(70) Pentachlorophenol (C)

16.867min (+ 0.008) 26318.42 ng




response 96495

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	66.74
264.00	62.80	61.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080923\
Data File : BG058657.D
Acq On : 9 Aug 2023 13:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 09 14:22:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

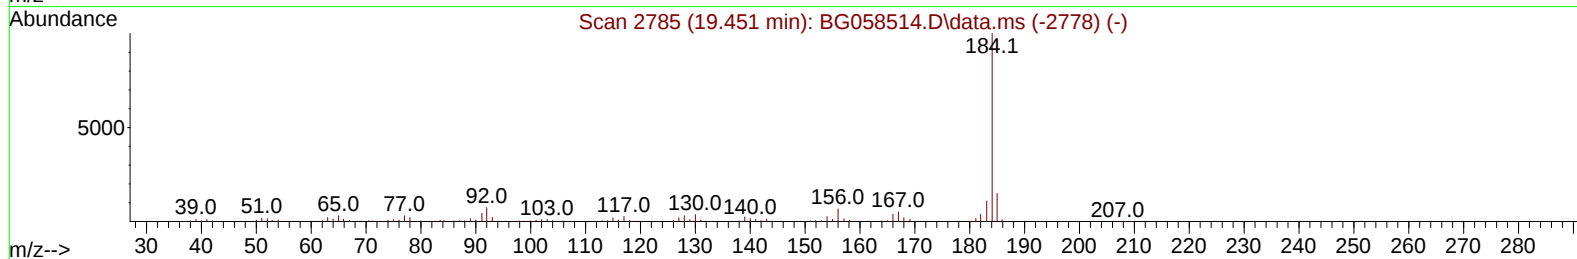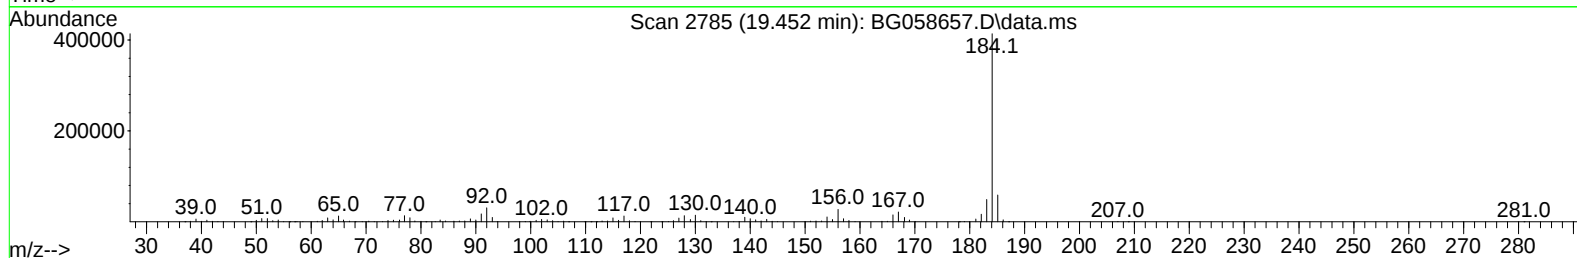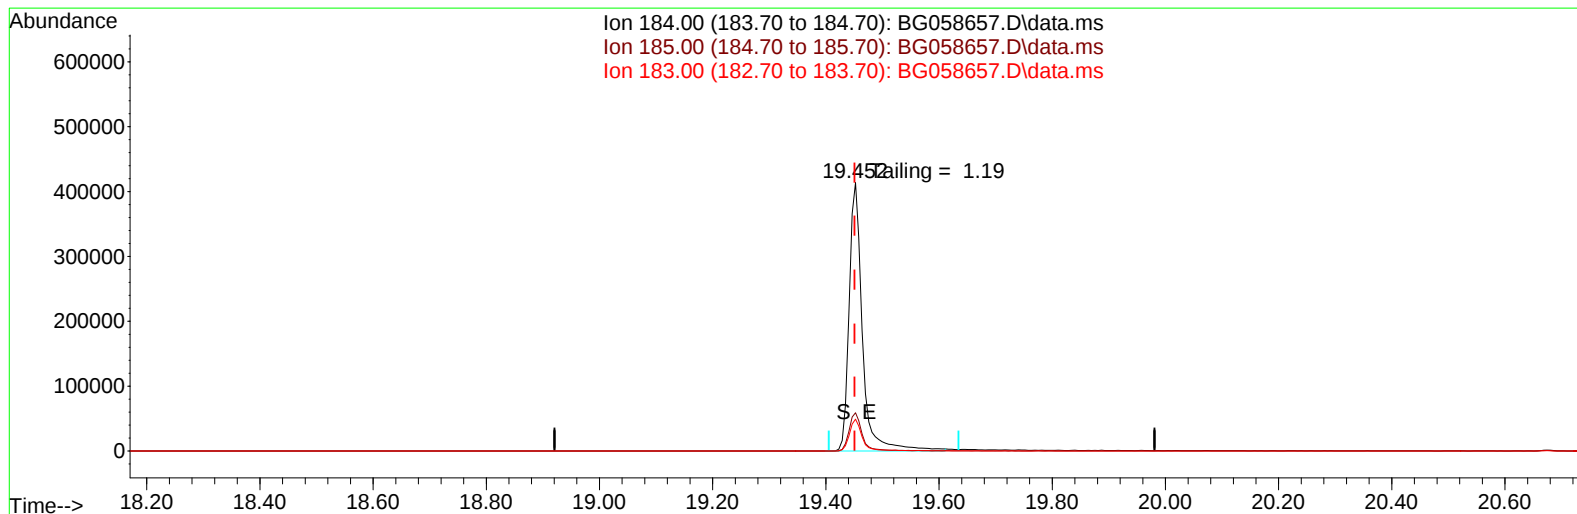

TIC: BG058657.D\data.ms

(77) Benzidine

19.452min (+ 0.002) 0.00 ng

response 682317

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.28
183.00	10.90	11.90
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/9/2023	BNA_G	<u>BG058657.D</u>
Compound Name	Response	Retention Time
DDT	355565	20.674
DDD	8635	20.24
DDE	2062	19.728
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10697	366262	2.92

Instrument :
BNA_G
ClientSampleId :
DFTPP