

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081019\
 Data File : BG042129.D
 Acq On : 10 Aug 2019 17:55
 Operator : HP/JU
 Sample : K4184-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AA9

Quant Time: Aug 11 00:01:58 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 09 16:22:05 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.02	152	76103	20.00	ng/ul	0.00
18) Naphthalene-d8	10.85	136	312149	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.69	164	215295	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.44	188	436852	20.00	ng/ul	0.00
77) Chrysene-d12	21.72	240	448736	20.00	ng/ul	0.00
85) Perylene-d12	24.99	264	492138	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.41	96	6641	3.82	ng/uL	0.00
5) Phenol-d5	7.18	99	29340	4.91	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.34	67	61635	18.45	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	91105	17.84	ng/ul	0.00
13) 4-Methylphenol-d8	8.73	113	59811	11.93	ng/ul	0.00
19) Nitrobenzene-d5	9.19	128	56146	23.89	ng/ul	0.00
22) 2-Nitrophenol-d4	9.92	143	69469	25.46	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.47	165	120117	21.81	ng/ul	0.00
29) 4-Chloroaniline-d4	11.00	131	7816	1.28	ng/ul	0.02
43) Dimethylphthalate-d6	14.09	166	429934	25.75	ng/ul	0.00
46) Acenaphthylene-d8	14.38	160	477210	25.02	ng/ul	0.00
51) 4-Nitrophenol-d4	14.90	143	11313	4.04	ng/ul	0.02
57) Fluorene-d10	15.68	176	370735	24.96	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.80	200	66137	23.60	ng/ul	0.00
70) Anthracene-d10	17.54	188	572621	27.32	ng/ul	0.00
78) Pyrene-d10	19.83	212	665654	26.58	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.76	264	726350	28.25	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	7.21	94	7920	1.285	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081019\
Data File : BG042129.D
Acq On : 10 Aug 2019 17:55
Operator : HP/JU
Sample : K4184-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AA9

Quant Time: Aug 11 00:01:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 09 16:22:05 2019
Response via : Initial Calibration

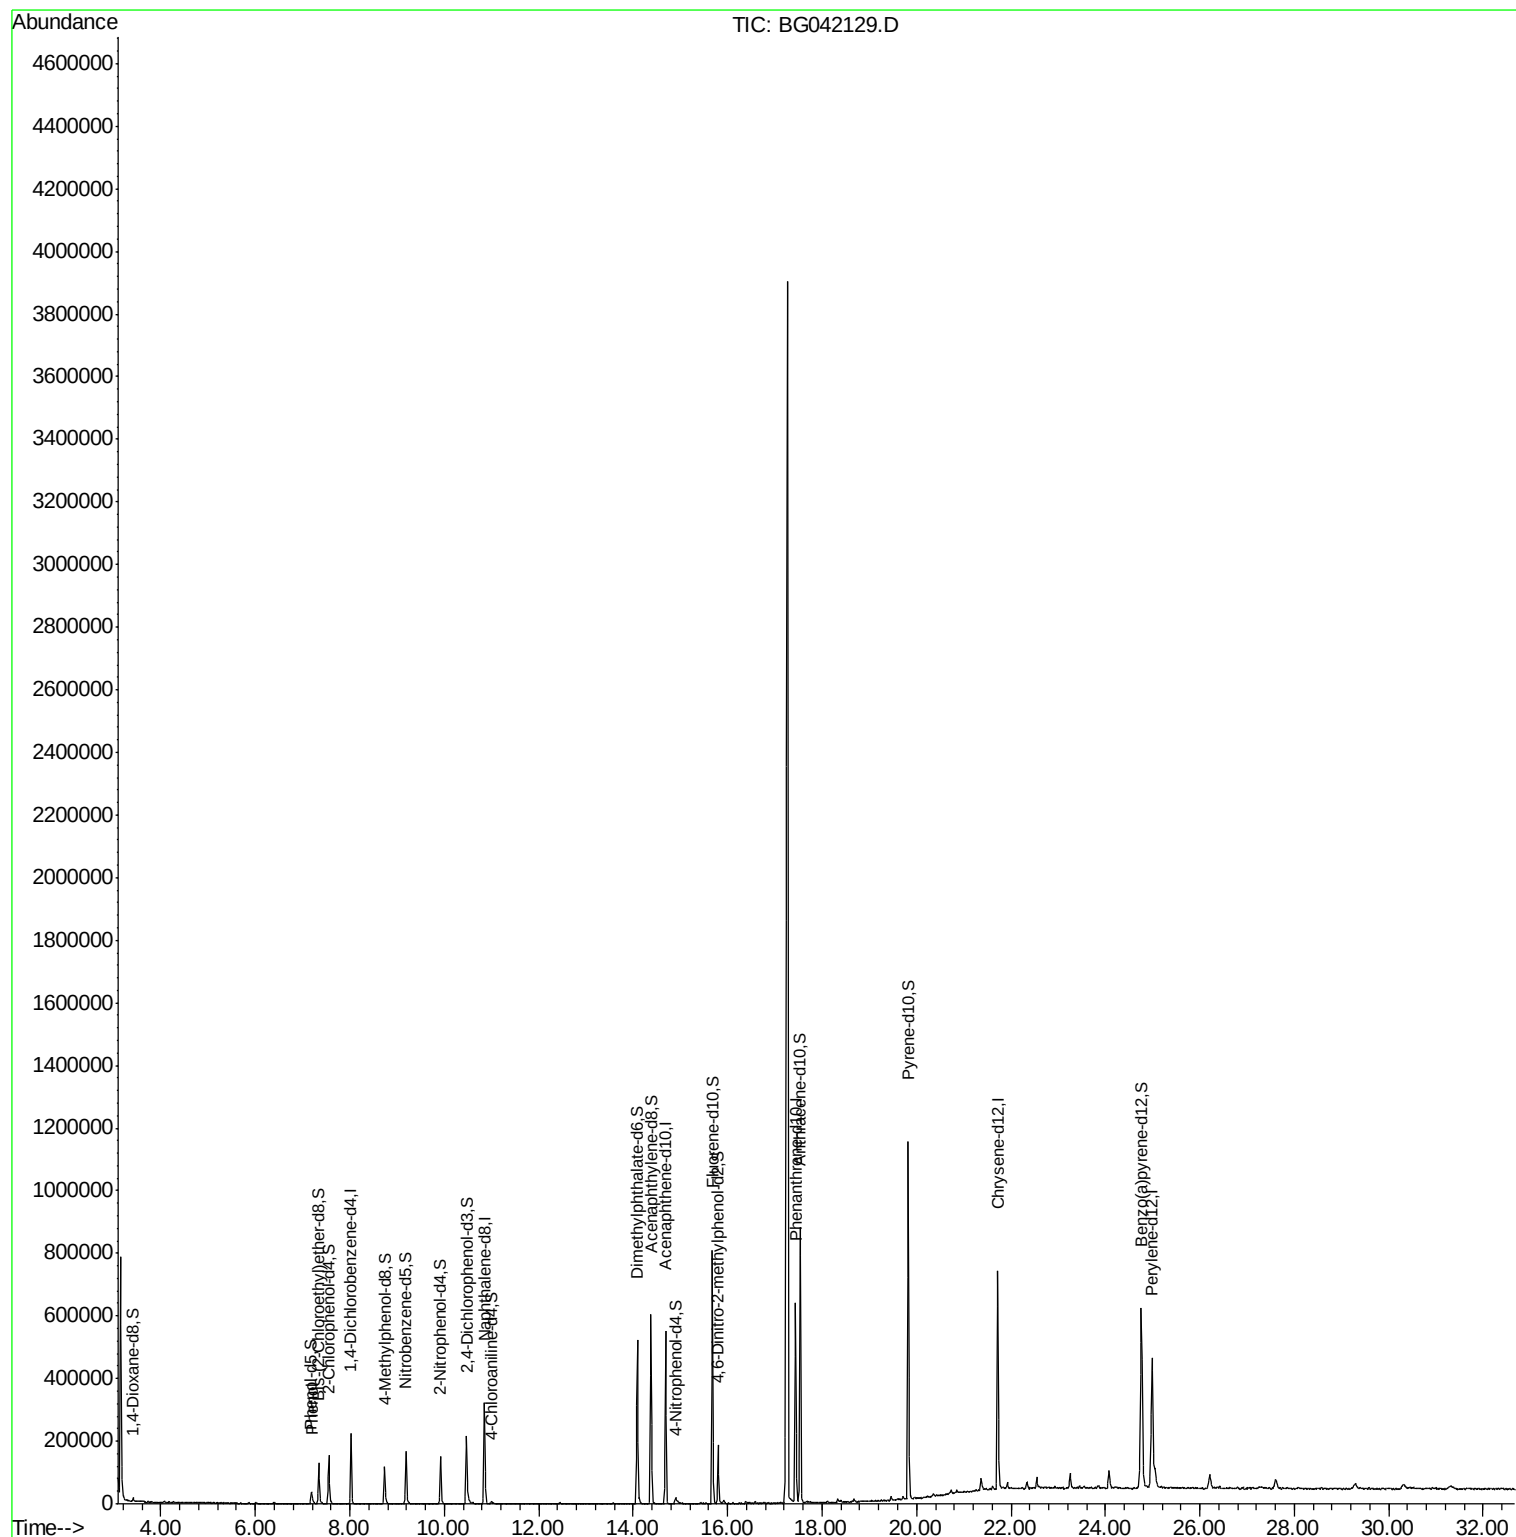

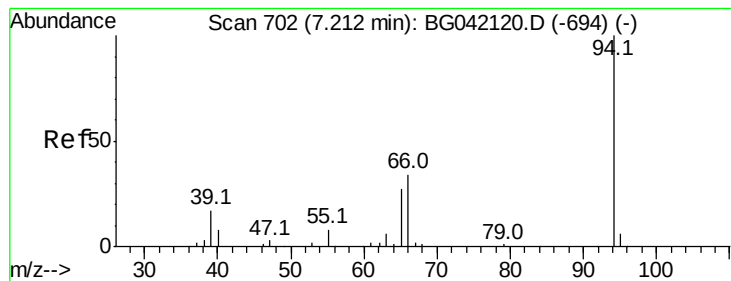

#6

Phenol

Concen: 1.285 ng/ul
 RT: 7.21 min Scan# 701
 Delta R.T. 0.00 min
 Lab File: BG042129.D
 Acq: 10 Aug 2019 17:55

Instrument :
 BNA_G
 ClientSampleId :
 C0AA9

Tot Ion: 94 Resp: 7920
 Ion Ratio Lower Upper
 94 100
 65 19.3 25.8 38.6#
 66 38.4 31.8 47.8

