
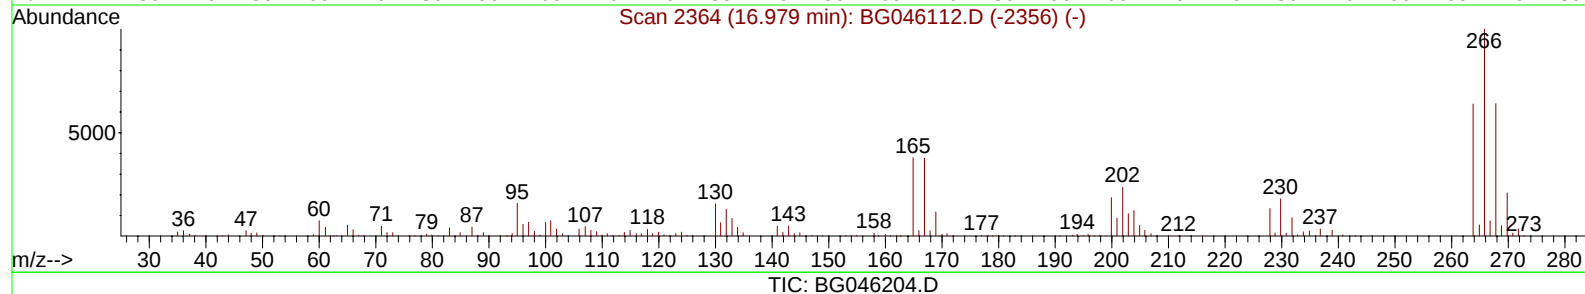
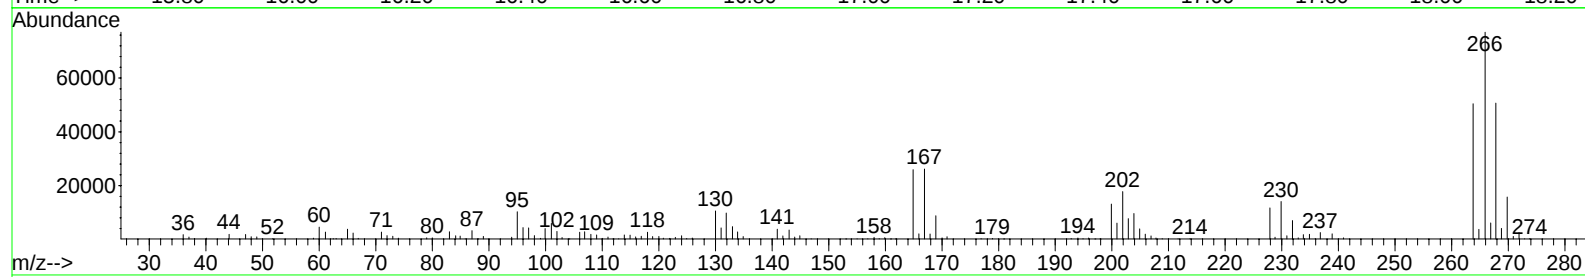


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081020\
Data File : BG046204.D
Acq On : 10 Aug 2020 12:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 16:53:05 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 30 18:43:49 2020
Response via : Initial Calibration

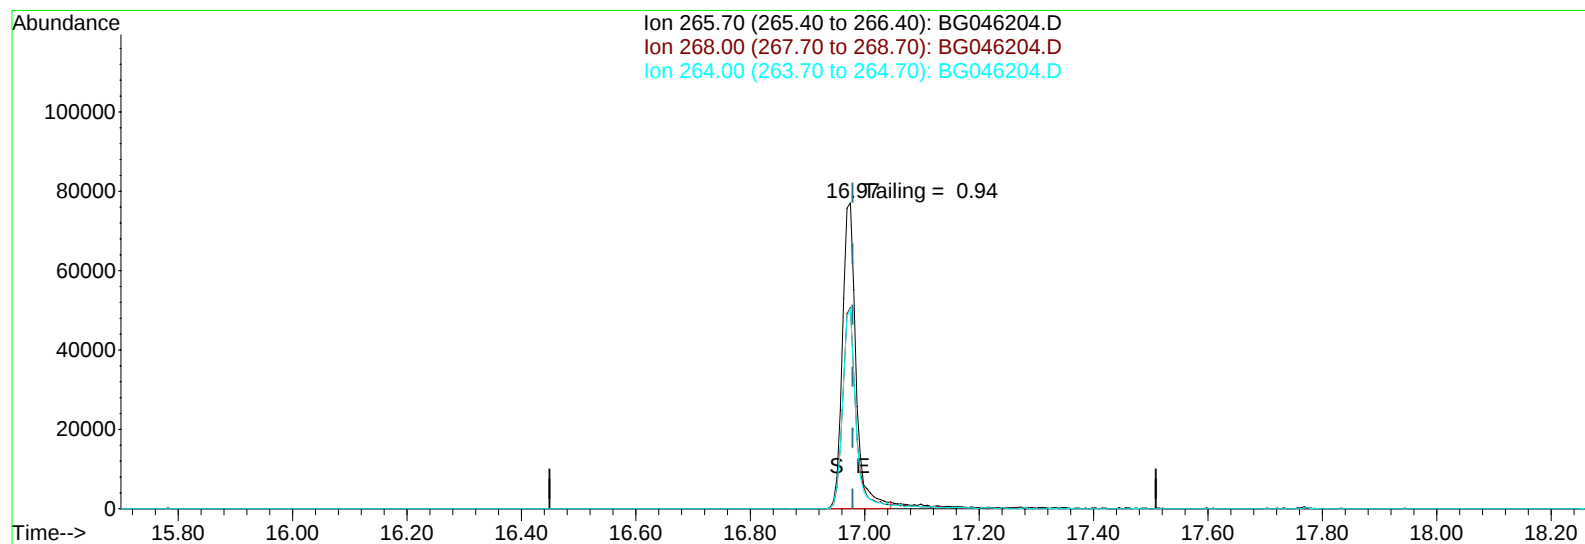

(70) Pentachlorophenol (C)




16.975min (-0.004) 31331.35ng

response 130389

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	65.77
264.00	63.90	65.47
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081020\
 Data File : BG046204.D
 Acq On : 10 Aug 2020 12:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 16:53:05 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 30 18:43:49 2020
 Response via : Initial Calibration

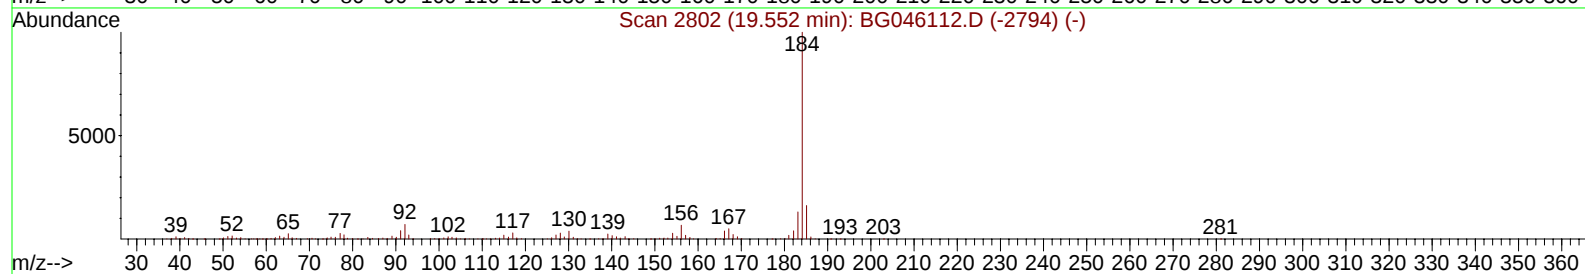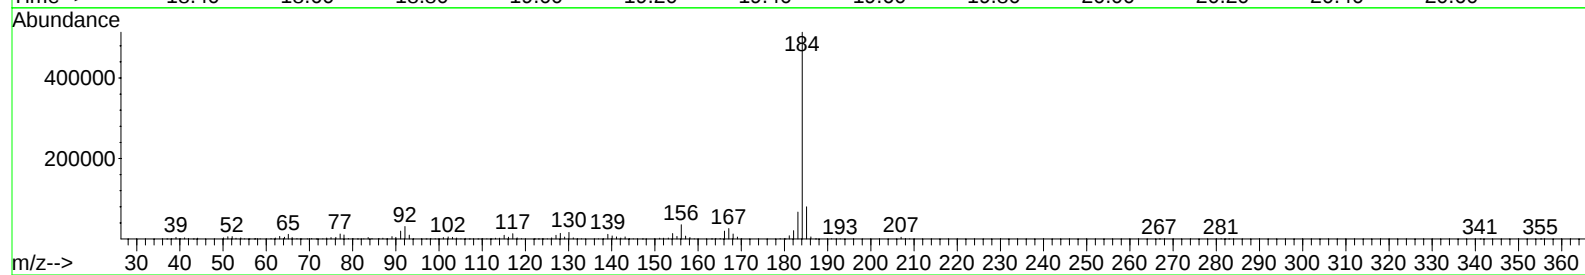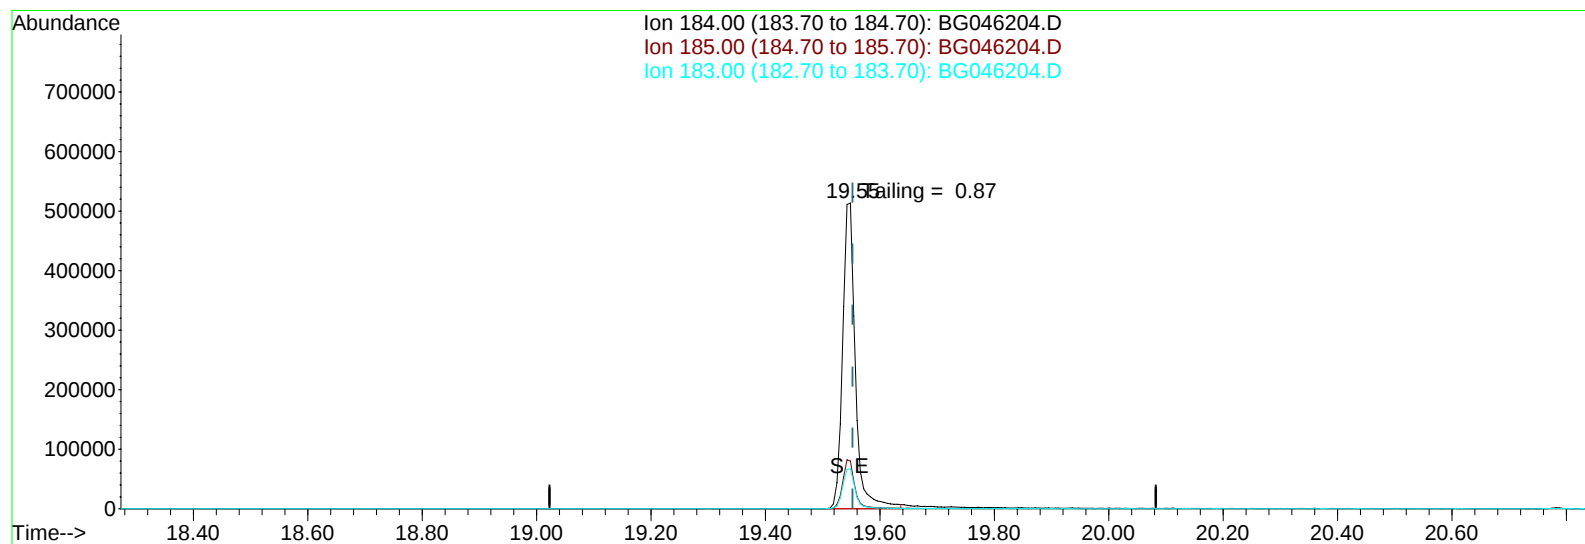

TIC: BG046204.D

(77) Benzidine

19.548min (-0.004) 0.00ng

response 817786

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	15.58
183.00	13.10	13.02
0.00	0.00	0.00