
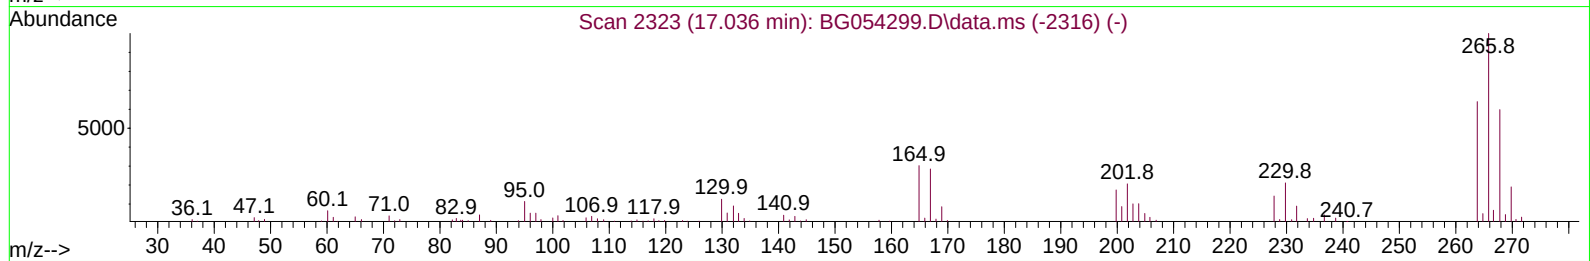
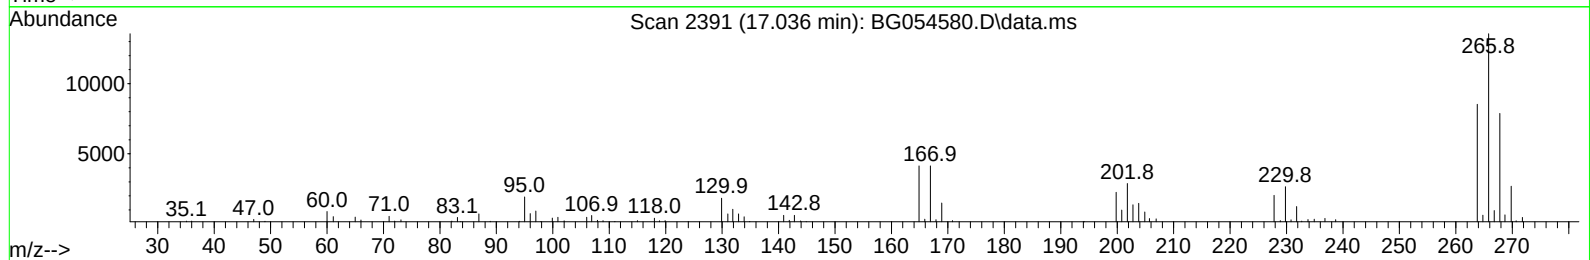


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081022\
Data File : BG054580.D
Acq On : 10 Aug 2022 9:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 18:24:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 08 14:48:51 2022
Response via : Initial Calibration

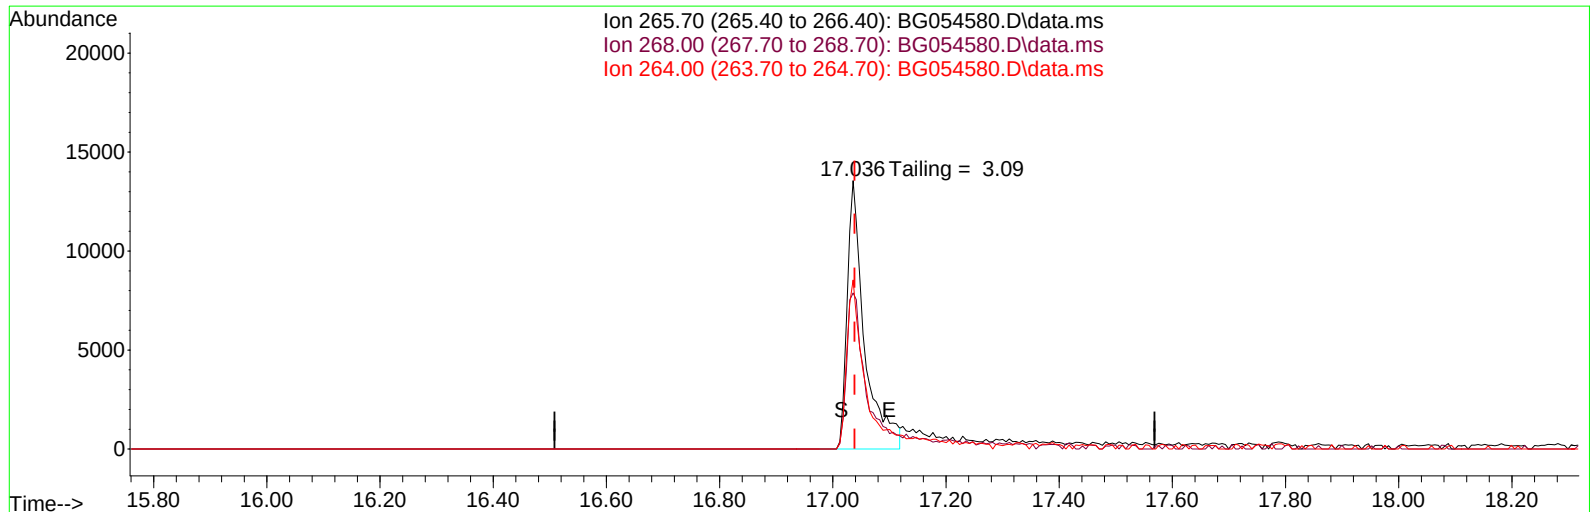

TIC: BG054580.D\data.ms

(70) Pentachlorophenol (C)




17.036min (-0.002) 14634.00 ng

response 29953

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	62.91
264.00	66.20	62.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081022\
Data File : BG054580.D
Acq On : 10 Aug 2022 9:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 18:24:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 08 14:48:51 2022
Response via : Initial Calibration

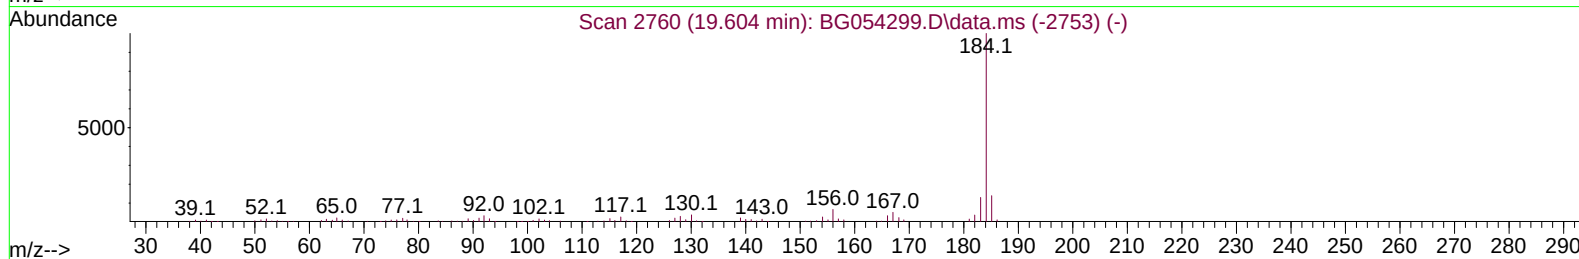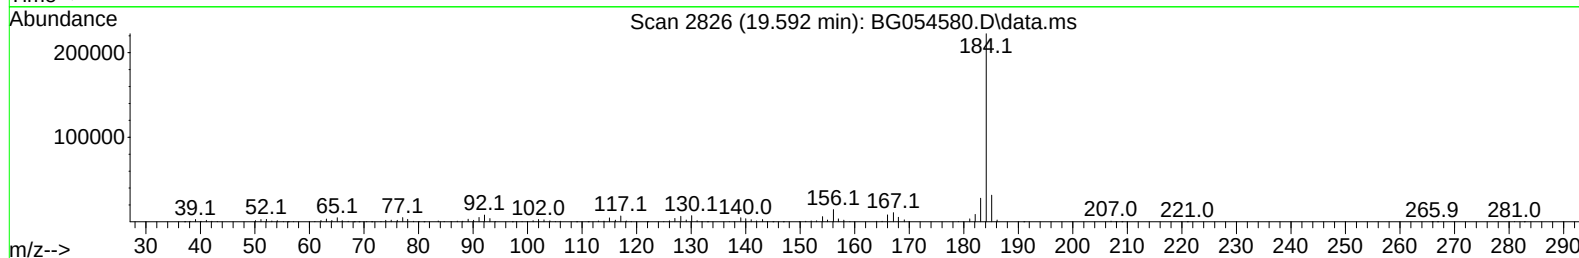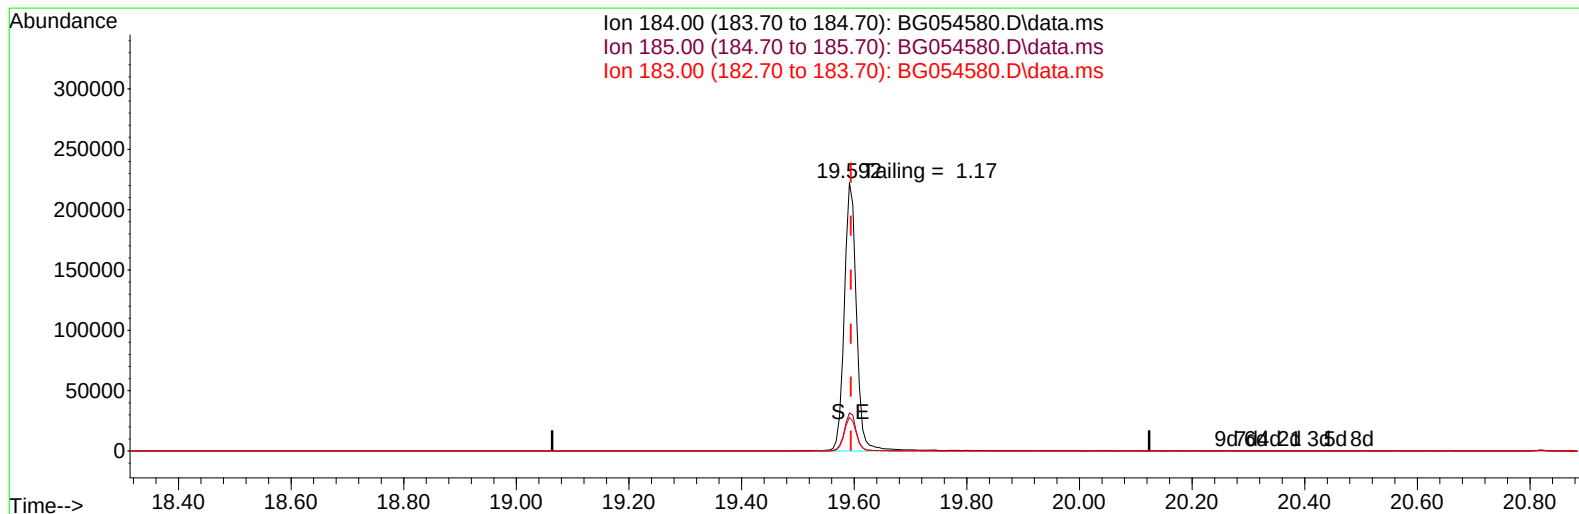

TIC: BG054580.D\data.ms

(77) Benzidine

19.592min (-0.002) 349104.95 ng m

response 341418

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.22
183.00	11.10	12.62
0.00	0.00	0.00