

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081022\
 Data File : BG054596.D
 Acq On : 10 Aug 2022 20:18
 Operator : CG/JU
 Sample : N3971-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-1R

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG054596.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.088	11	17	32	rVB	238407	463915	23.16%	5.918%
2	4.410	233	242	251	rBV	47716	87218	4.35%	1.113%
3	5.056	347	352	360	rBV2	15995	28089	1.40%	0.358%
4	5.561	432	438	451	rBV	163269	285550	14.25%	3.642%
5	6.601	609	615	625	rBV	22912	37176	1.86%	0.474%
6	7.177	707	713	724	rBV	106453	197210	9.84%	2.516%
7	7.970	841	848	854	rBV	67218	117505	5.87%	1.499%
8	8.029	854	858	868	rVB	31254	53154	2.65%	0.678%
9	9.139	1040	1047	1057	rBV	236207	422885	21.11%	5.394%
10	9.698	1134	1142	1152	rBB2	12001	21954	1.10%	0.280%
11	10.162	1217	1221	1231	rBV2	9888	20483	1.02%	0.261%
12	10.785	1319	1327	1333	rBV	87301	162628	8.12%	2.074%
13	11.713	1479	1485	1497	rVB2	21537	53111	2.65%	0.677%
14	13.229	1735	1743	1755	rBV	725285	1146320	57.22%	14.623%
15	13.464	1777	1783	1795	rBB	200191	322369	16.09%	4.112%
16	14.609	1972	1978	1985	rBV	156622	252017	12.58%	3.215%
17	16.108	2226	2233	2250	rBV2	624681	988946	49.37%	12.615%
18	17.359	2439	2446	2455	rBV	203811	320723	16.01%	4.091%
19	18.011	2549	2557	2562	rBV2	23244	28114	1.40%	0.359%
20	19.968	2884	2890	2896	rBV	1464600	2003242	100.00%	25.553%
21	21.625	3166	3172	3179	rVB2	248649	404123	20.17%	5.155%
22	24.833	3708	3718	3729	rVB2	141198	422687	21.10%	5.392%




Sum of corrected areas: 7839419

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081022\
Data File : BG054596.D
Acq On : 10 Aug 2022 20:18
Operator : CG/JU
Sample : N3971-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-1R

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

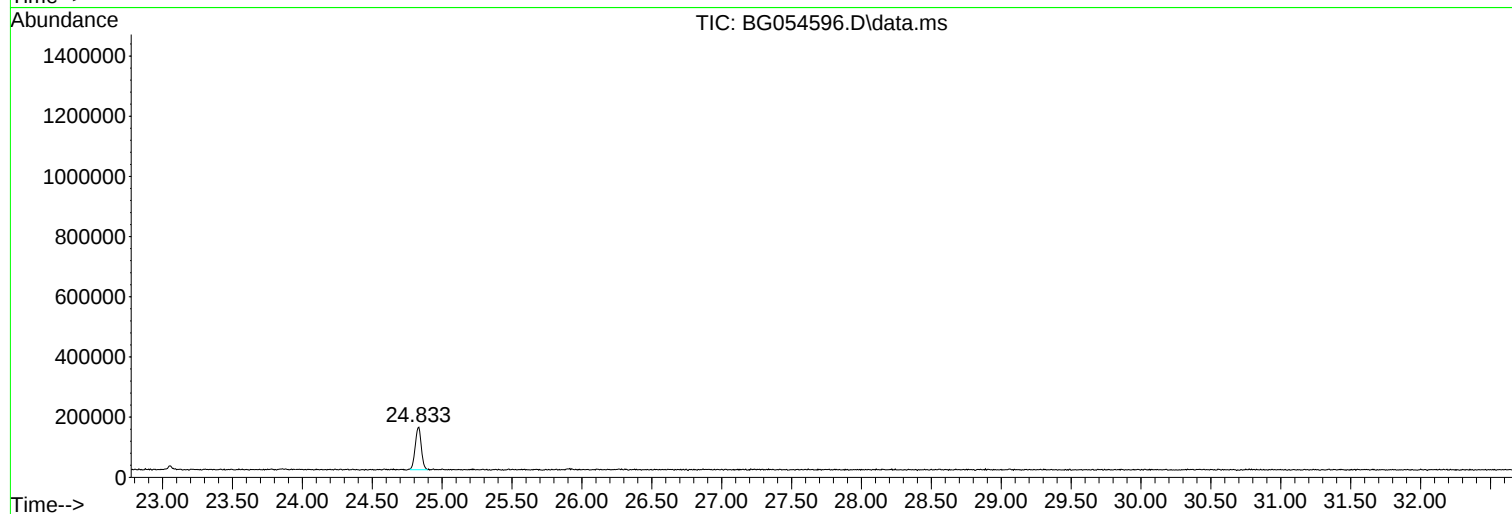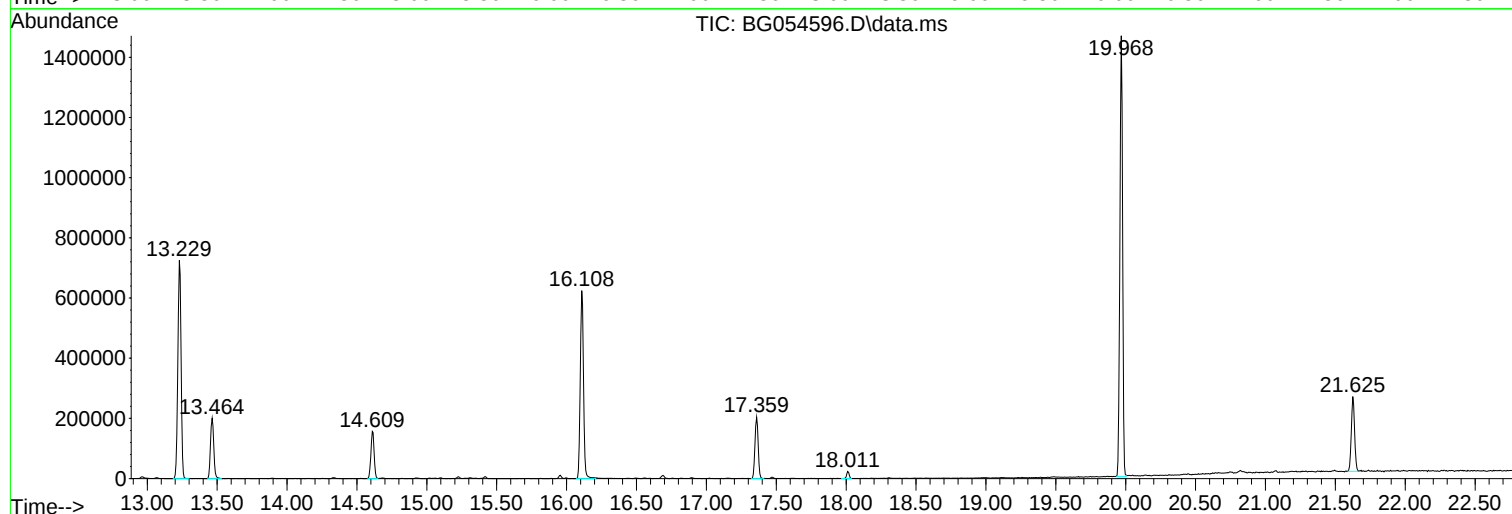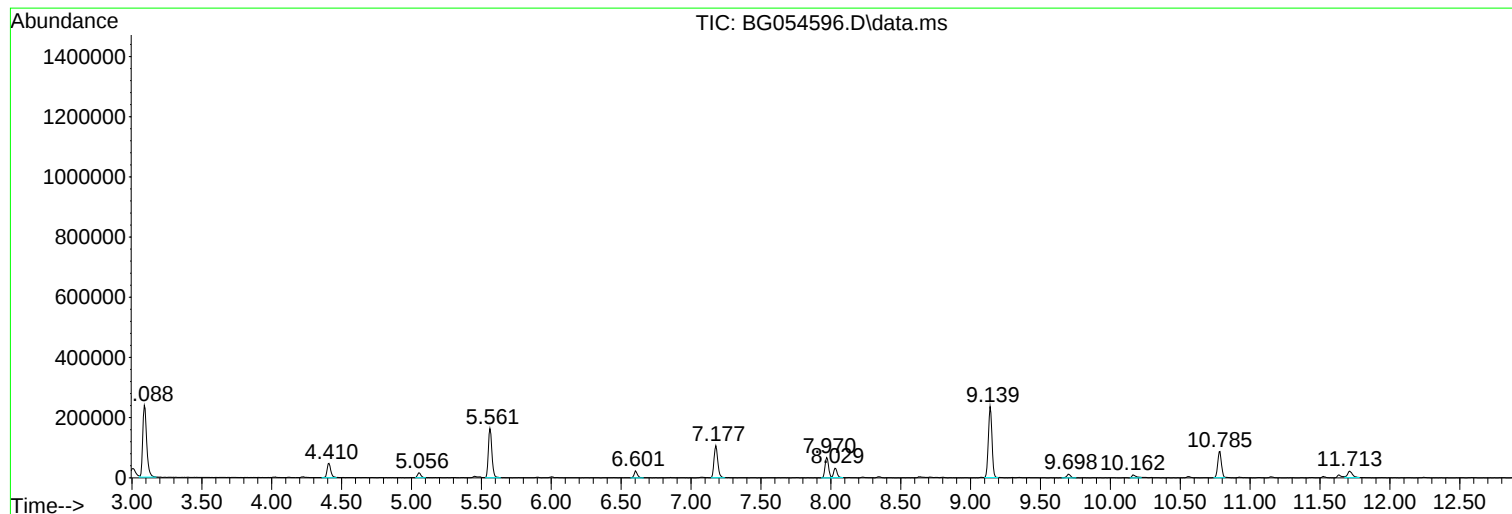

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081022\
Data File : BG054596.D
Acq On : 10 Aug 2022 20:18
Operator : CG/JU
Sample : N3971-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-1R

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081022\
Data File : BG054596.D
Acq On : 10 Aug 2022 20:18
Operator : CG/JU
Sample : N3971-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-1R

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc