
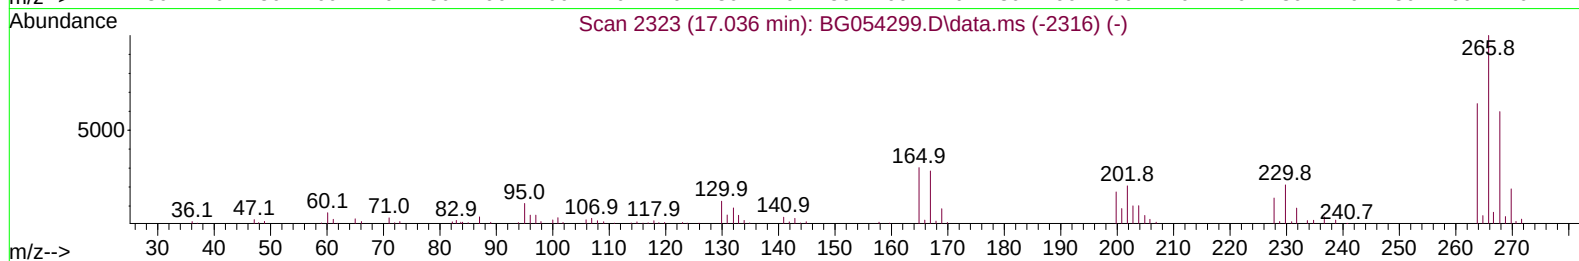
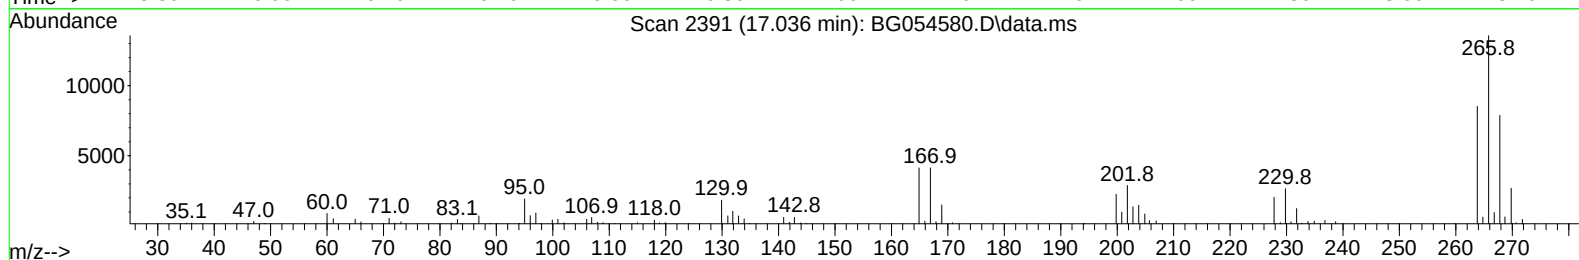


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081022\
 Data File : BG054580.D
 Acq On : 10 Aug 2022 9:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Aug 10 18:24:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 08 14:48:51 2022
 Response via : Initial Calibration

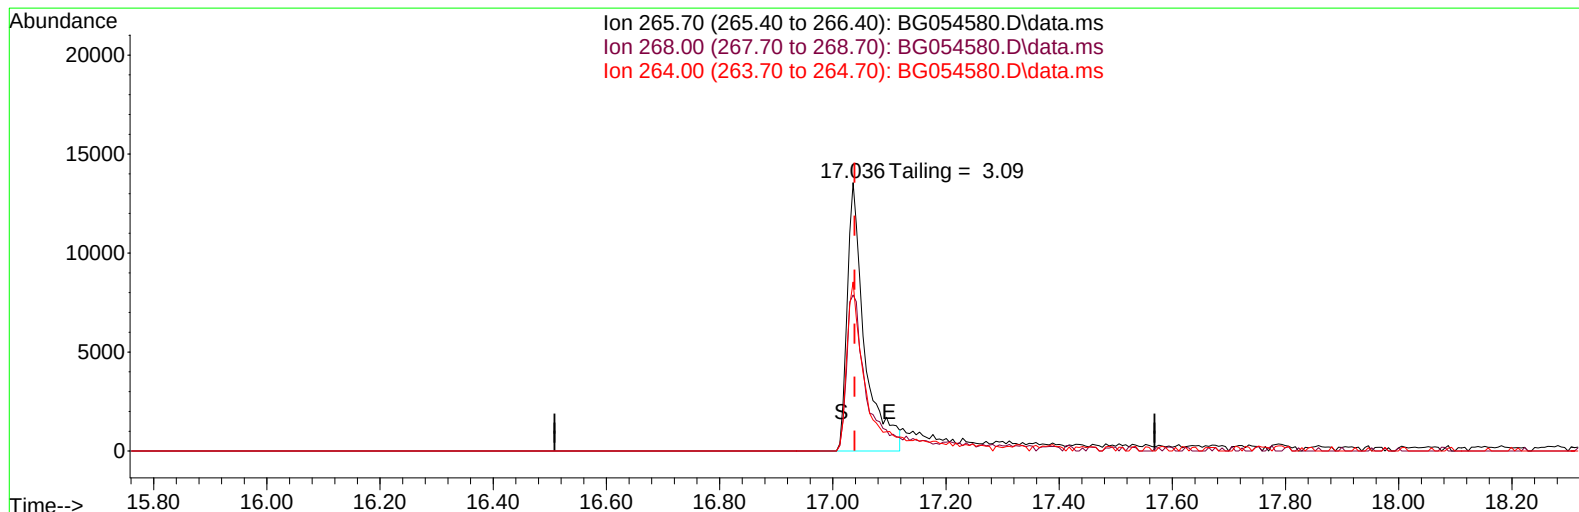

TIC: BG054580.D\data.ms

(70) Pentachlorophenol (C)

17.036min (-0.002) 14634.00 ng




response 29953

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	62.91
264.00	66.20	62.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081022\
Data File : BG054580.D
Acq On : 10 Aug 2022 9:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 10 18:24:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 08 14:48:51 2022
Response via : Initial Calibration

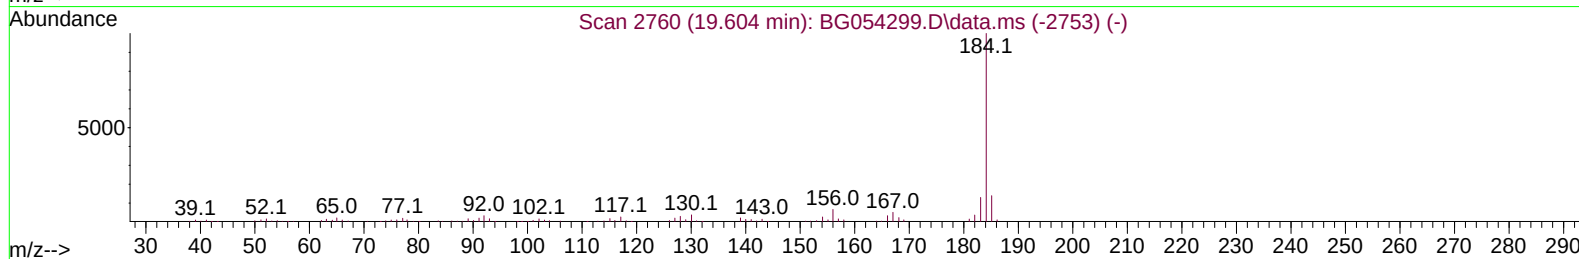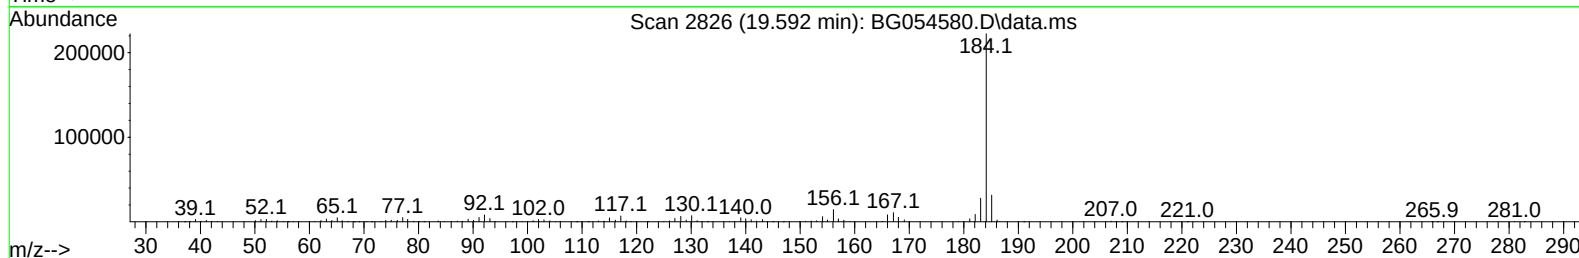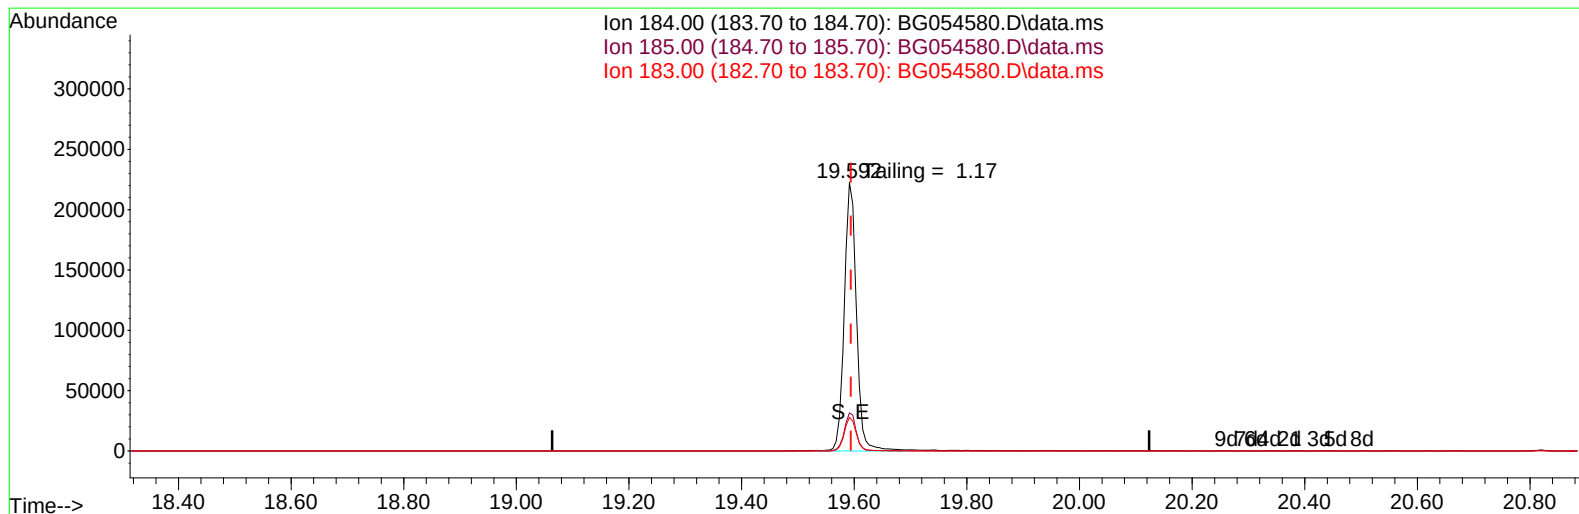

TIC: BG054580.D\data.ms

(77) Benzidine

19.592min (-0.002) 349104.95 ng m

response 341418


Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.22
183.00	11.10	12.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081022\
Data File : BG054580.D
Acq On : 10 Aug 2022 9:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 08 14:48:51 2022

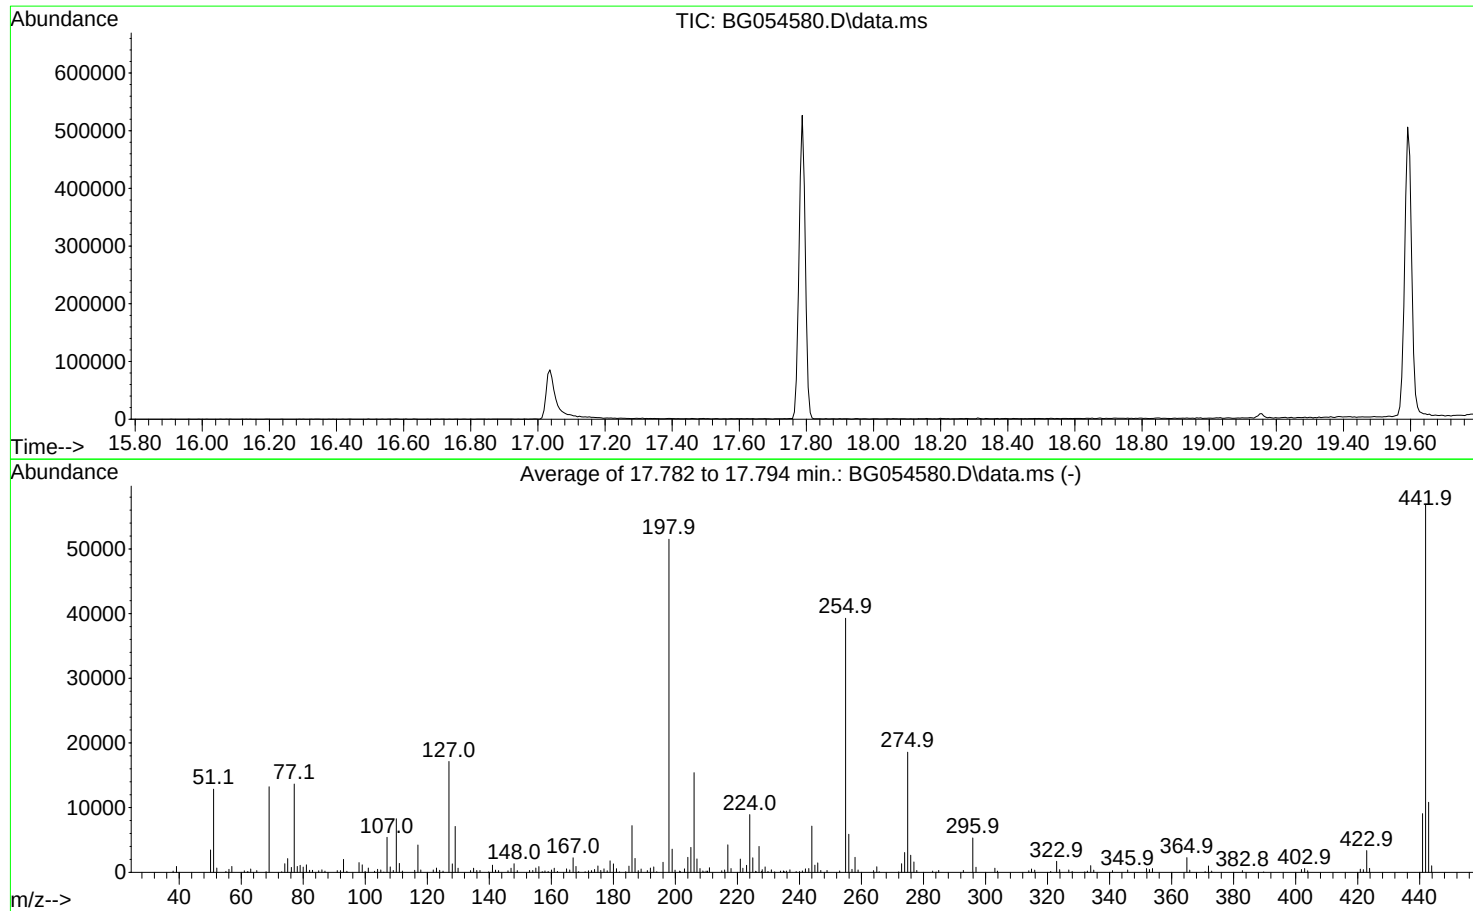

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2511

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.0	12854	PASS
68	69	0.00	2	0.7	94	PASS
69	198	0.00	100	25.7	13215	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	33.3	17127	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51509	PASS
199	198	5	9	7.0	3582	PASS
275	198	10	60	36.0	18563	PASS
365	198	1	100	4.4	2269	PASS
441	198	0.01	100	17.6	9069	PASS
442	442	50	100	100.0	56883	PASS
443	442	15	24	19.0	10826	PASS

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/10/2022	BNA_G	BG054580.D
Compound Name	Response	Retention Time
DDT	186234	20.81
DDD	8958	20.39
DDE	703	19.87
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9661	195895	4.93

Instrument :
BNA_G
ClientSampleId :
DFTPP