
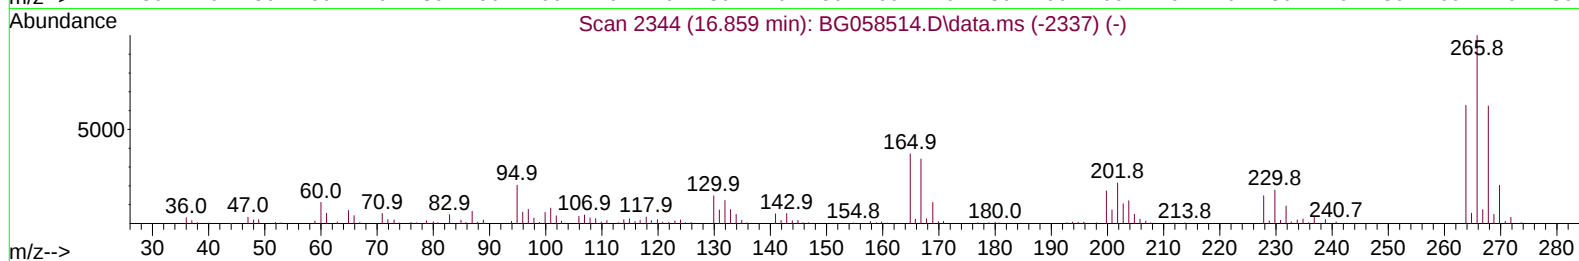
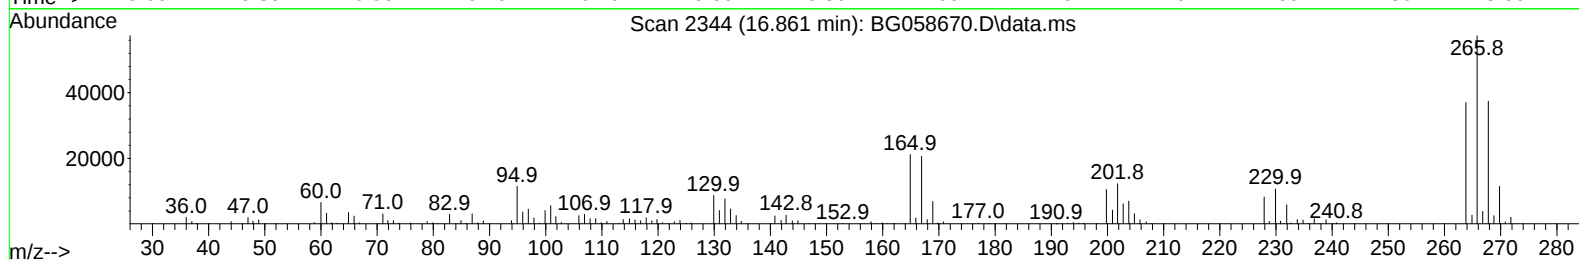


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081023\
Data File : BG058670.D
Acq On : 10 Aug 2023 7:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 11 03:04:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

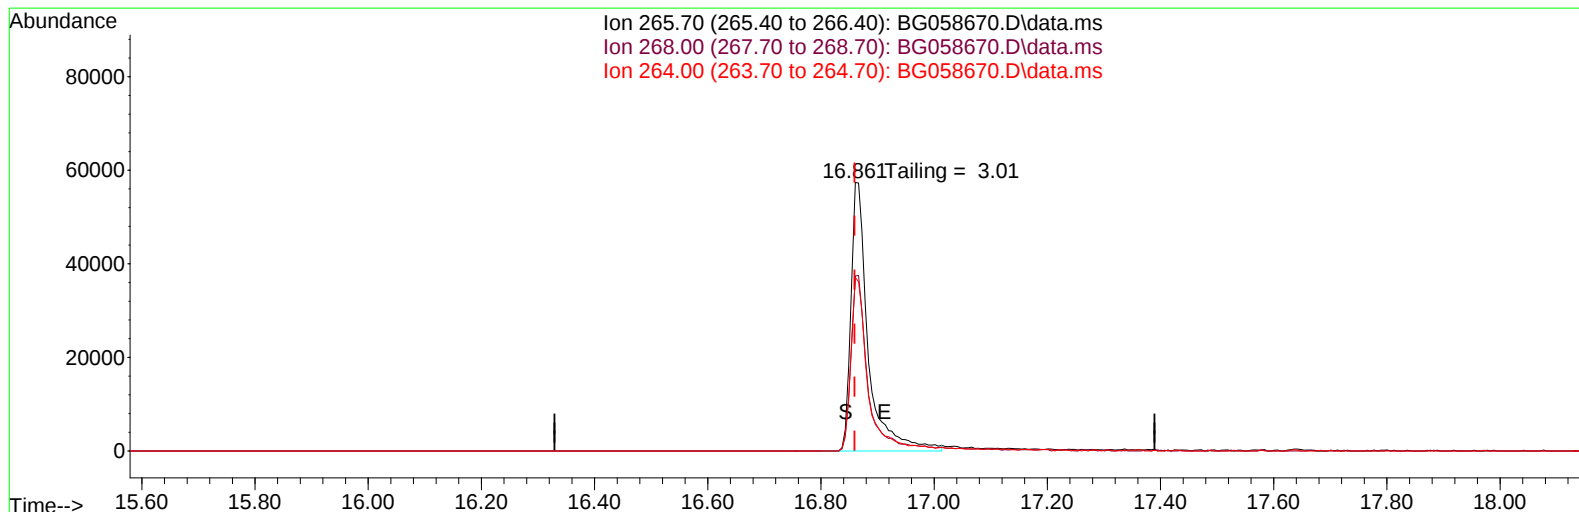

TIC: BG058670.D\data.ms

(70) Pentachlorophenol (C)




16.861min (+ 0.002) 33788.82 ng

response 123639

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	65.20
264.00	62.80	64.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081023\
Data File : BG058670.D
Acq On : 10 Aug 2023 7:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 11 03:04:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

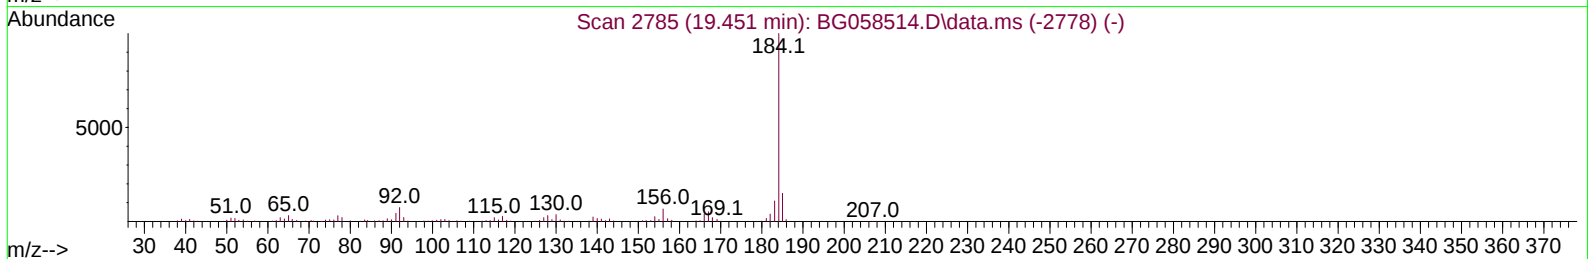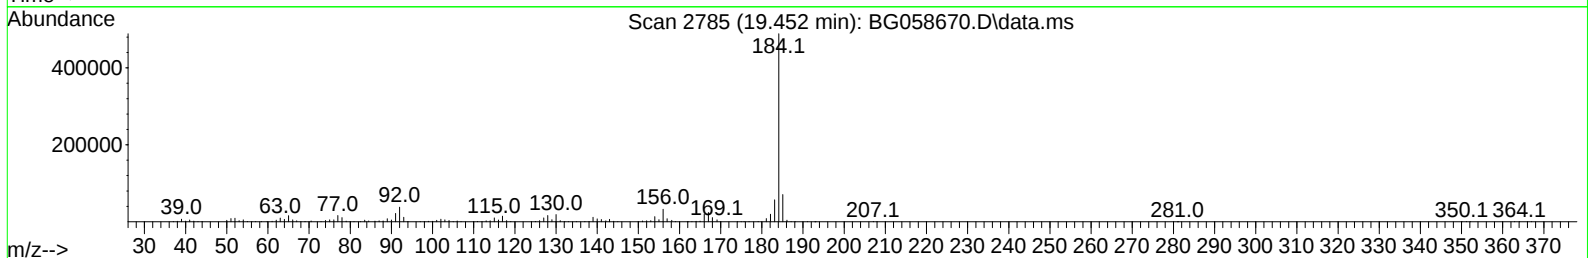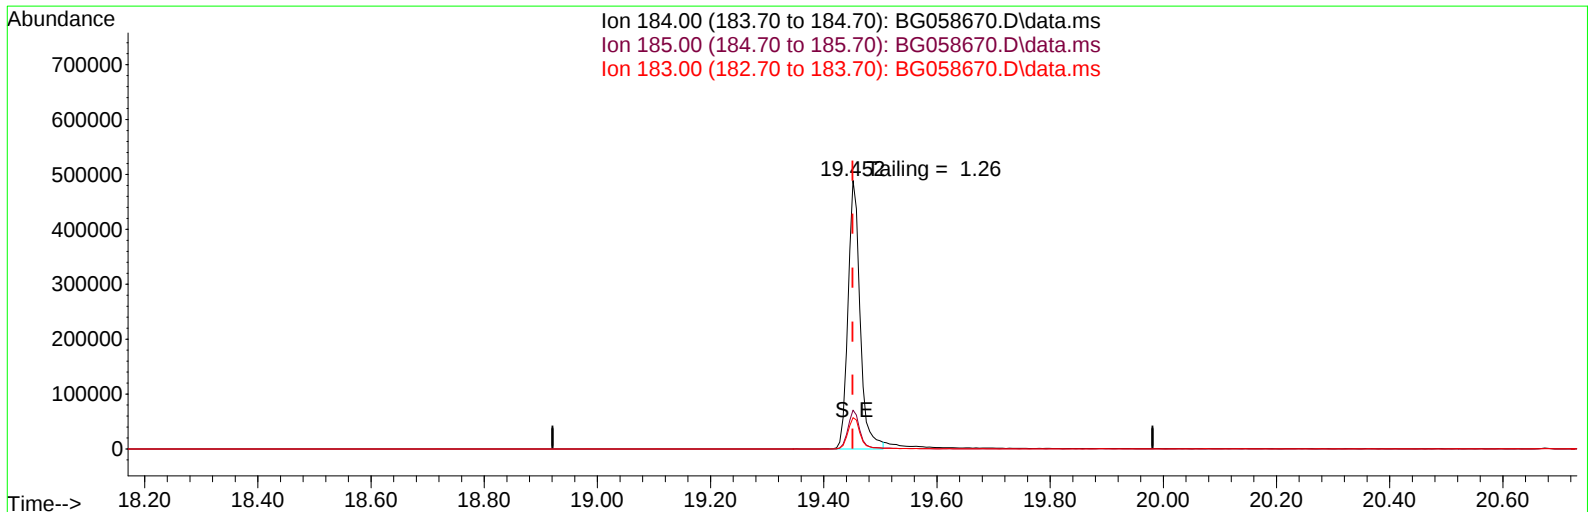

TIC: BG058670.D\data.ms

(77) Benzidine**19.452min (+ 0.001) 779667.83 ng****response 744844**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.48
183.00	10.90	11.68
0.00	0.00	0.00