


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081023\
Data File : BG058670.D
Acq On : 10 Aug 2023 7:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 28 22:29:07 2023

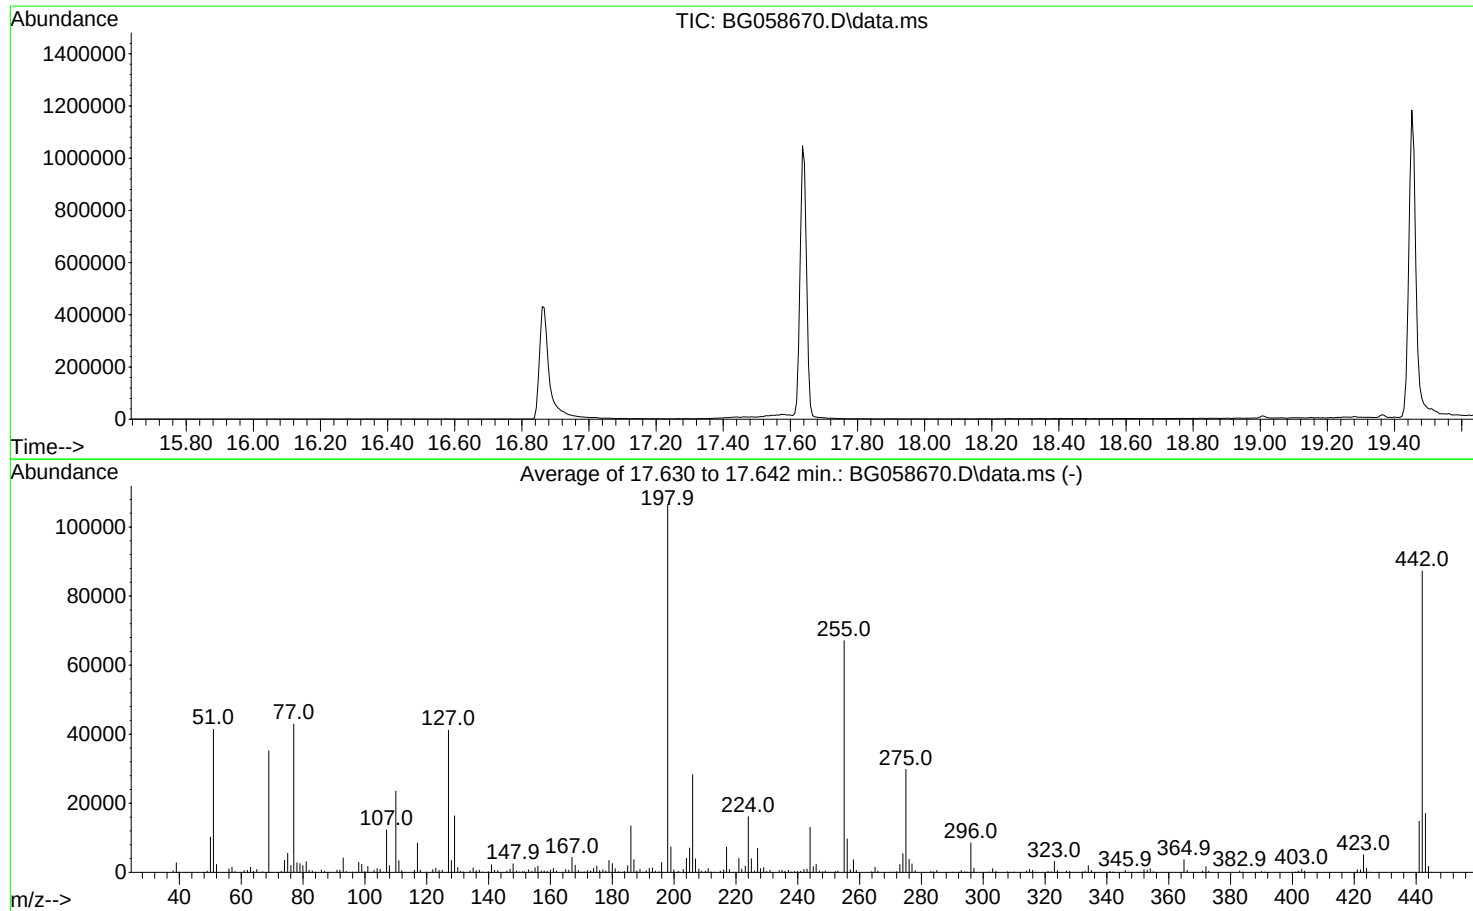




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.9	41432	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.0	35182	PASS
70	69	0.00	2	0.2	59	PASS
127	198	10	80	38.6	41144	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	106523	PASS
199	198	5	9	7.0	7417	PASS
275	198	10	60	28.0	29837	PASS
365	198	1	100	3.4	3657	PASS
441	198	0.01	100	13.9	14770	PASS
442	442	50	100	100.0	87267	PASS
443	442	15	24	19.6	17071	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081023\
Data File : BG058670.D
Acq On : 10 Aug 2023 7:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 11 03:04:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

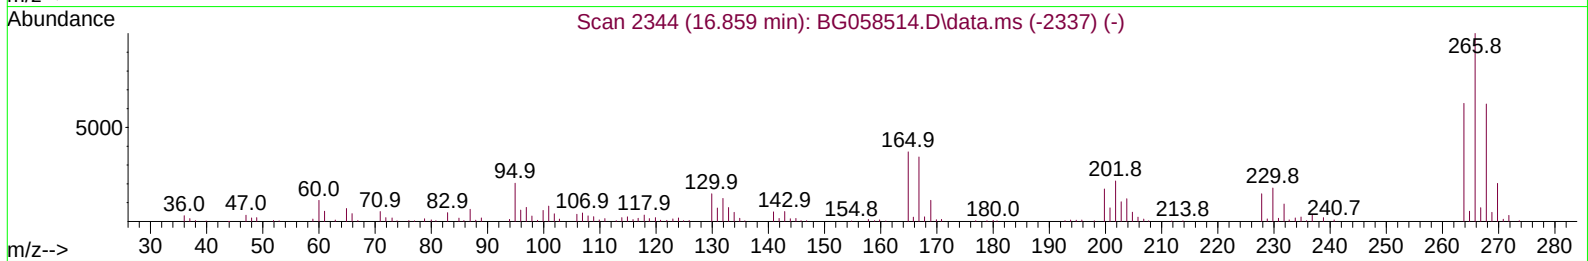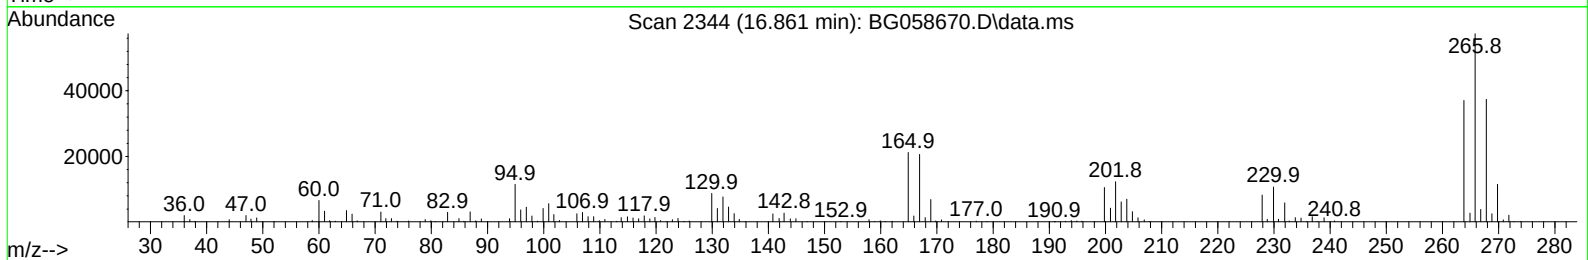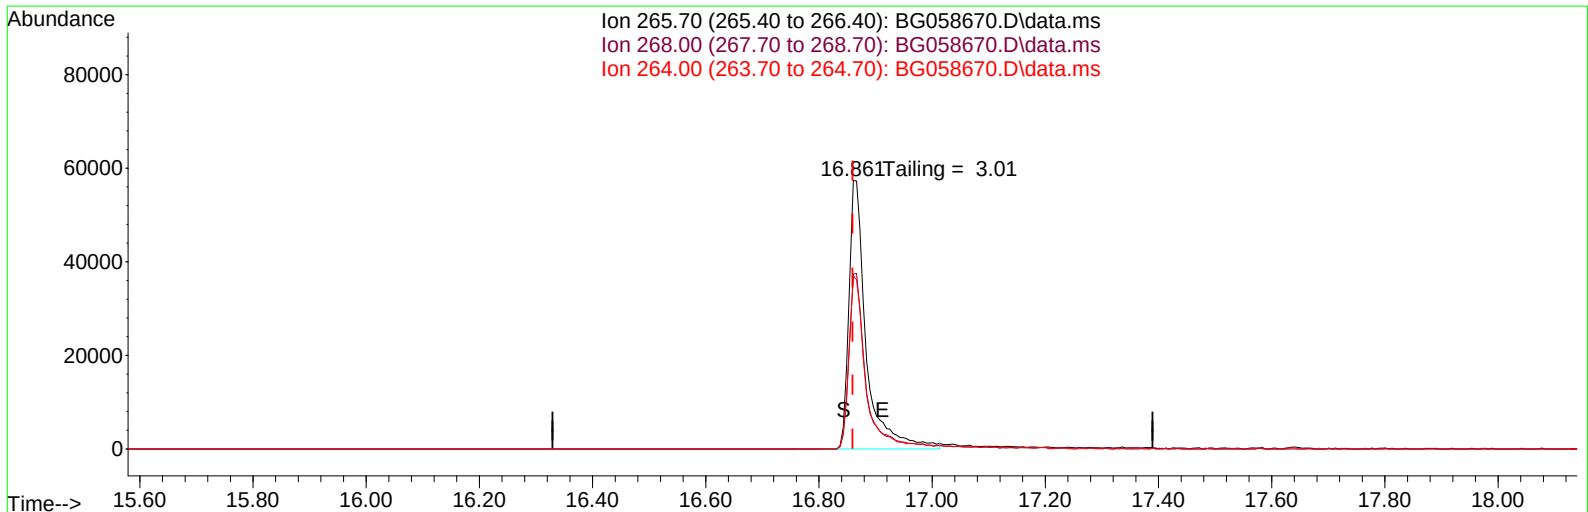

TIC: BG058670.D\data.ms

(70) Pentachlorophenol (C)

16.861min (+ 0.002) 33788.82 ng




response 123639

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	65.20
264.00	62.80	64.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081023\
 Data File : BG058670.D
 Acq On : 10 Aug 2023 7:50
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Aug 11 03:04:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 28 22:29:07 2023
 Response via : Initial Calibration

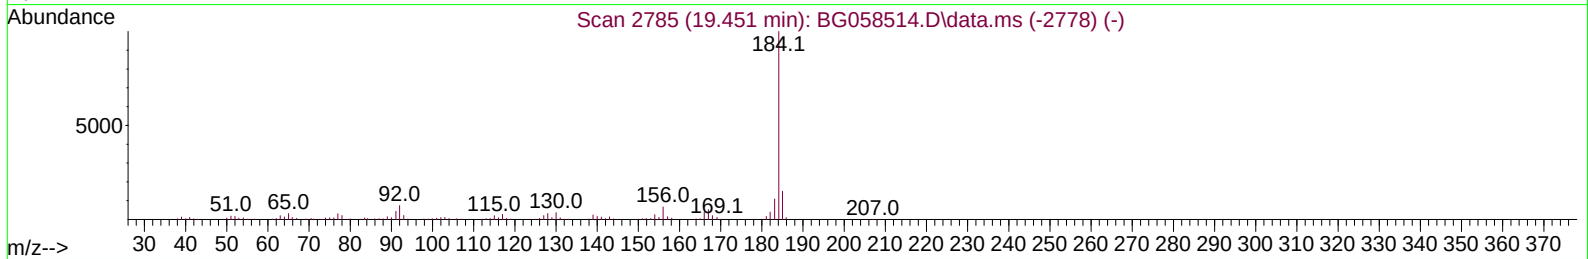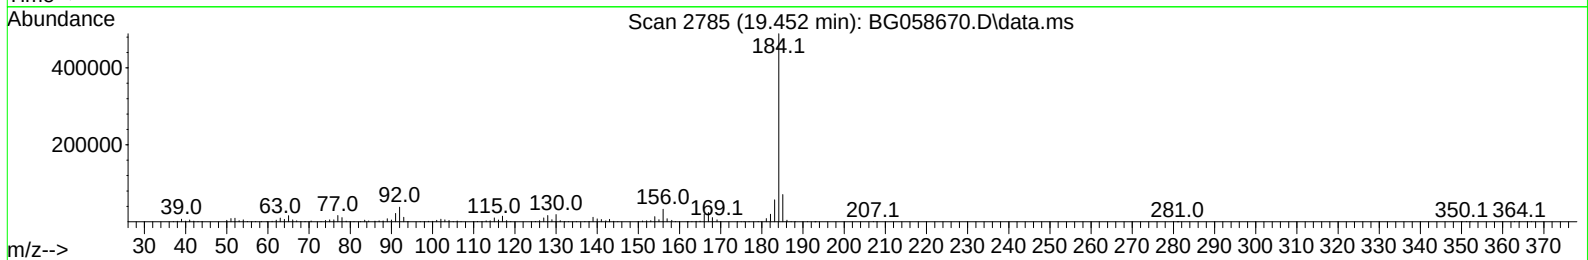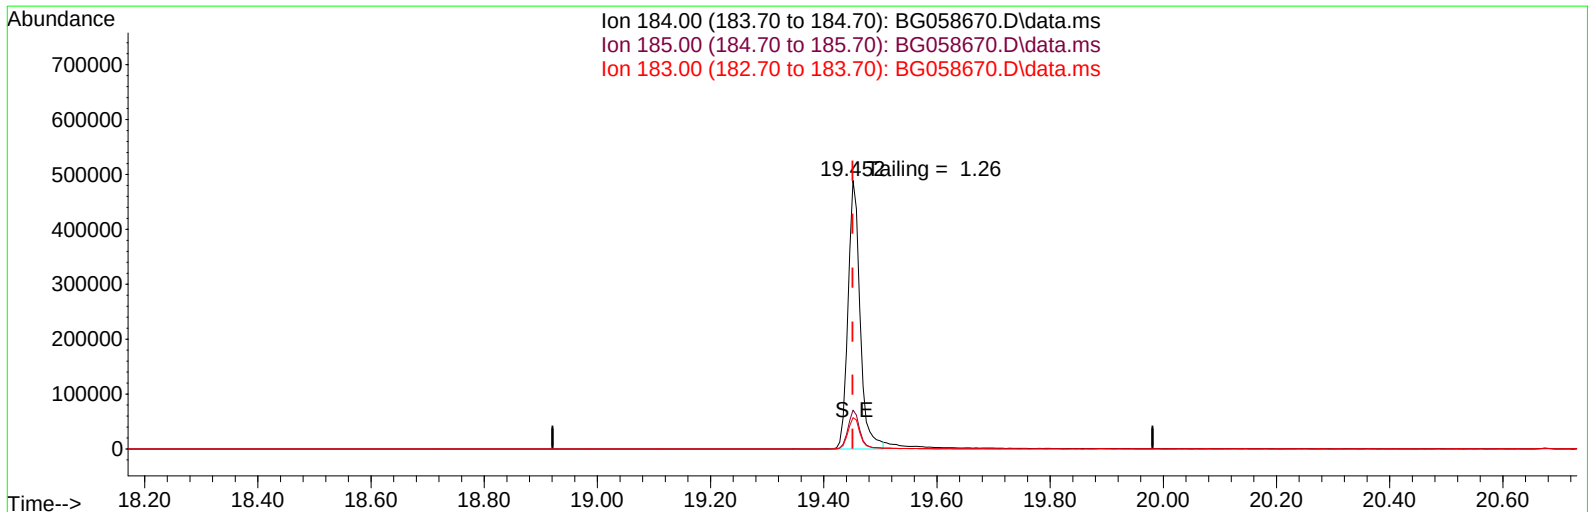

TIC: BG058670.D\data.ms

(77) Benzidine

19.452min (+ 0.001) 779667.83 ng

response 744844

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.48
183.00	10.90	11.68
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/10/2023	BNA_G	<u>BG058670.D</u>
Compound Name	Response	Retention Time
DDT	349608	20.674
DDD	9609	20.239
DDE	1107	19.734
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10716	360324	2.97

Instrument :
BNA_G
ClientSampleId :
DFTPP