
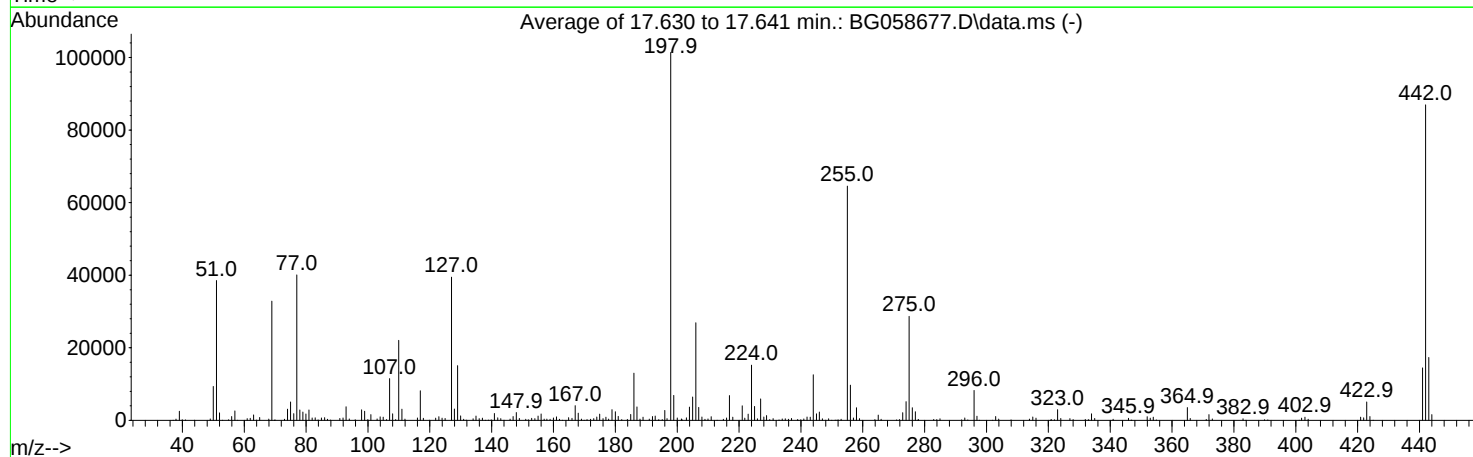


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081023\
Data File : BG058677.D
Acq On : 10 Aug 2023 13:32
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 28 22:29:07 2023

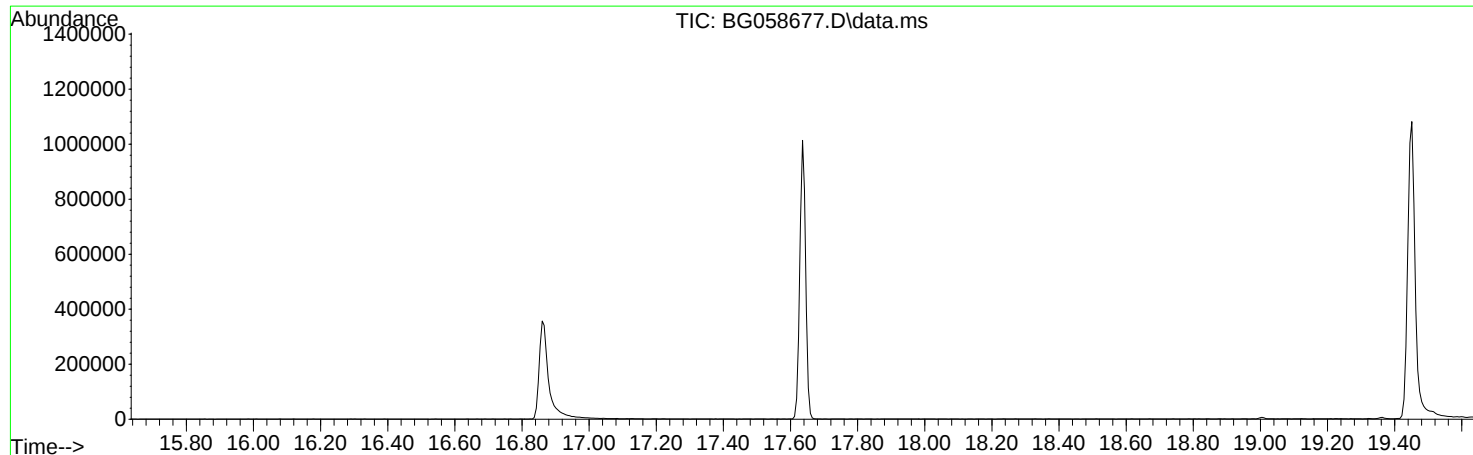




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	38541	PASS
68	69	0.00	2	1.1	357	PASS
69	198	0.00	100	32.4	32861	PASS
70	69	0.00	2	0.4	136	PASS
127	198	10	80	38.9	39483	PASS
197	198	0.00	2	0.5	504	PASS
198	198	100	100	100.0	101376	PASS
199	198	5	9	6.8	6897	PASS
275	198	10	60	28.3	28680	PASS
365	198	1	100	3.5	3545	PASS
441	198	0.01	100	14.3	14458	PASS
442	442	50	100	100.0	86960	PASS
443	442	15	24	19.9	17344	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081023\
Data File : BG058677.D
Acq On : 10 Aug 2023 13:32
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 11 03:06:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

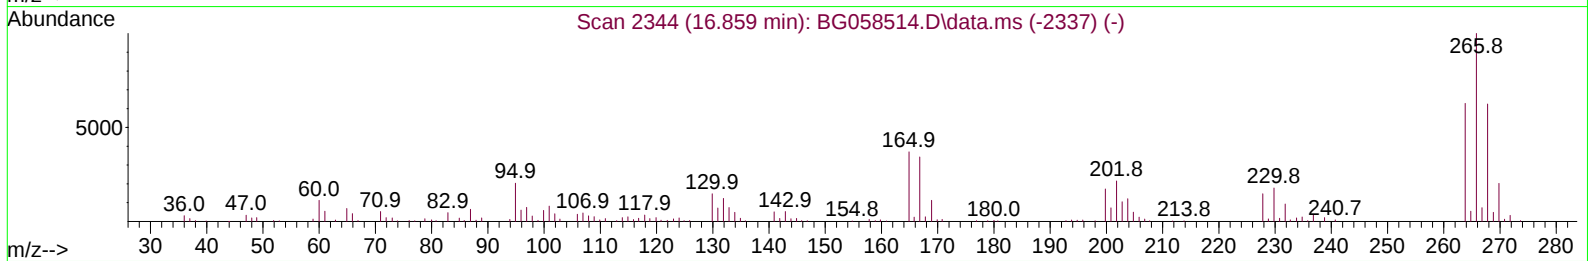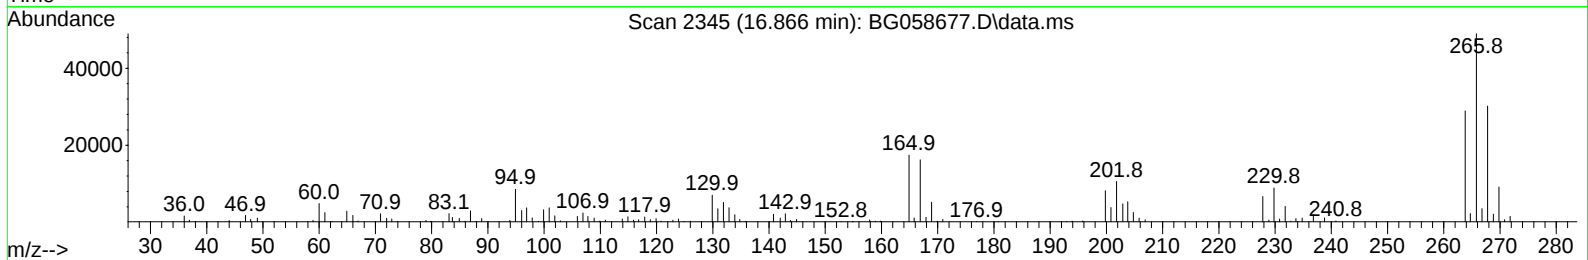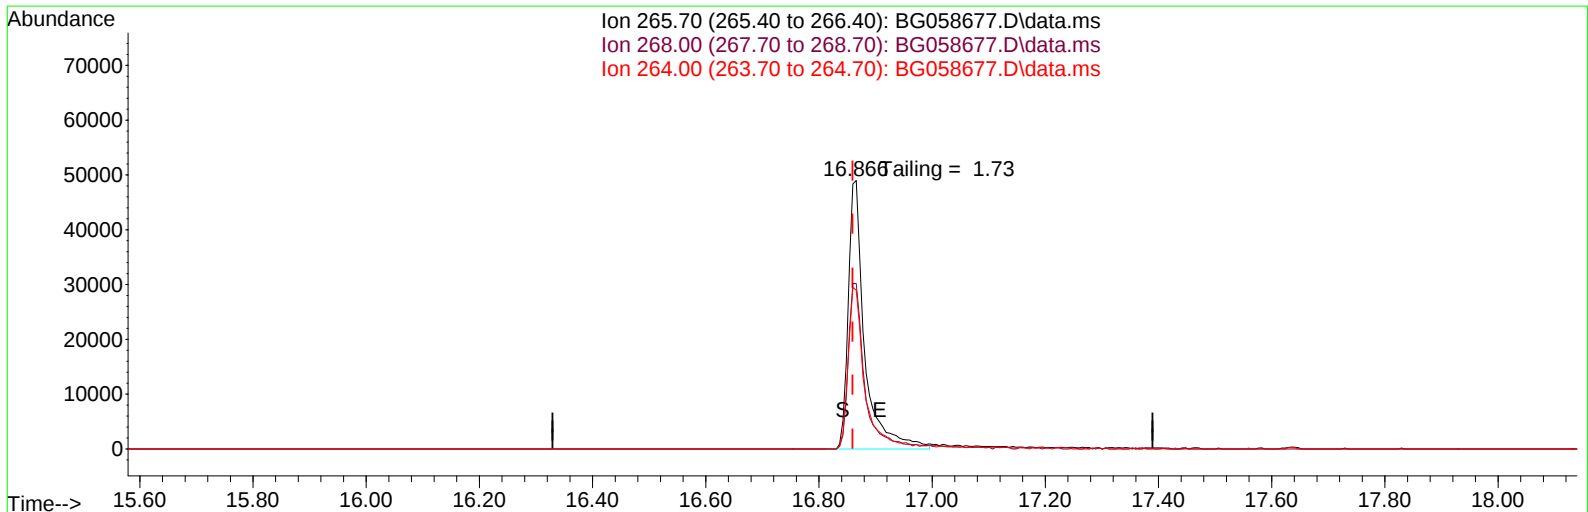

TIC: BG058677.D\data.ms

(70) Pentachlorophenol (C)

16.866min (+ 0.007) 26627.37 ng




response 98790

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	61.61
264.00	62.80	63.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081023\
Data File : BG058677.D
Acq On : 10 Aug 2023 13:32
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 11 03:06:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

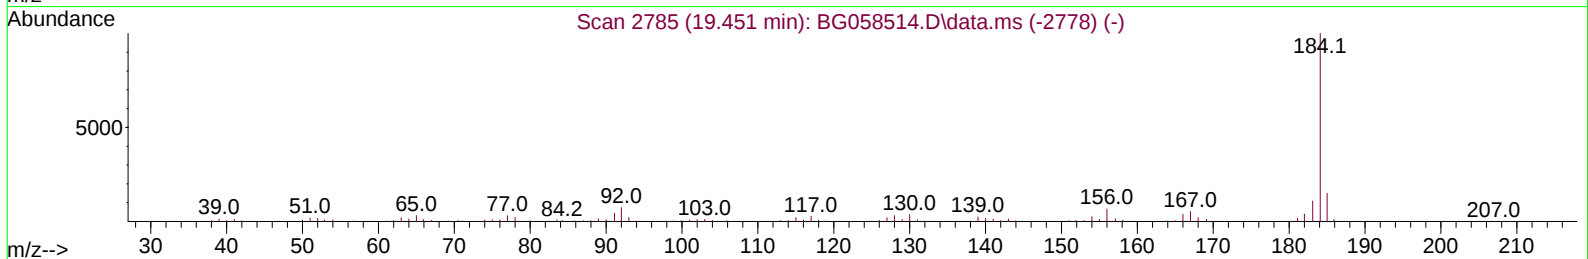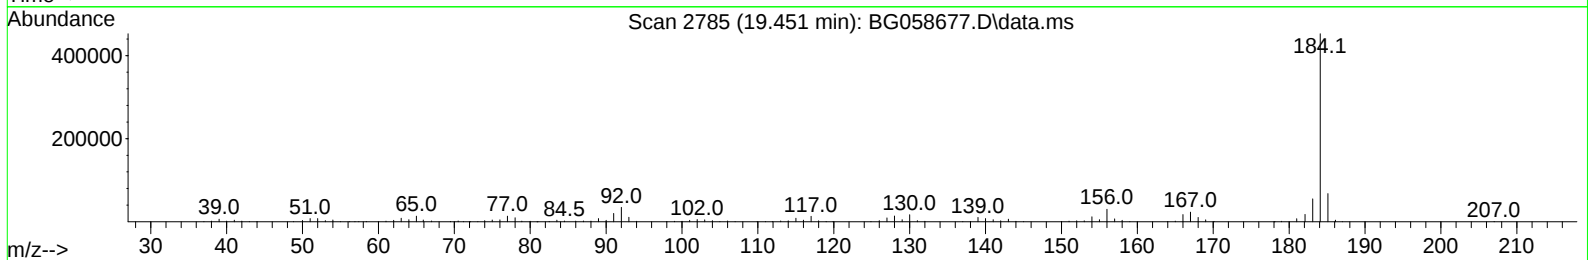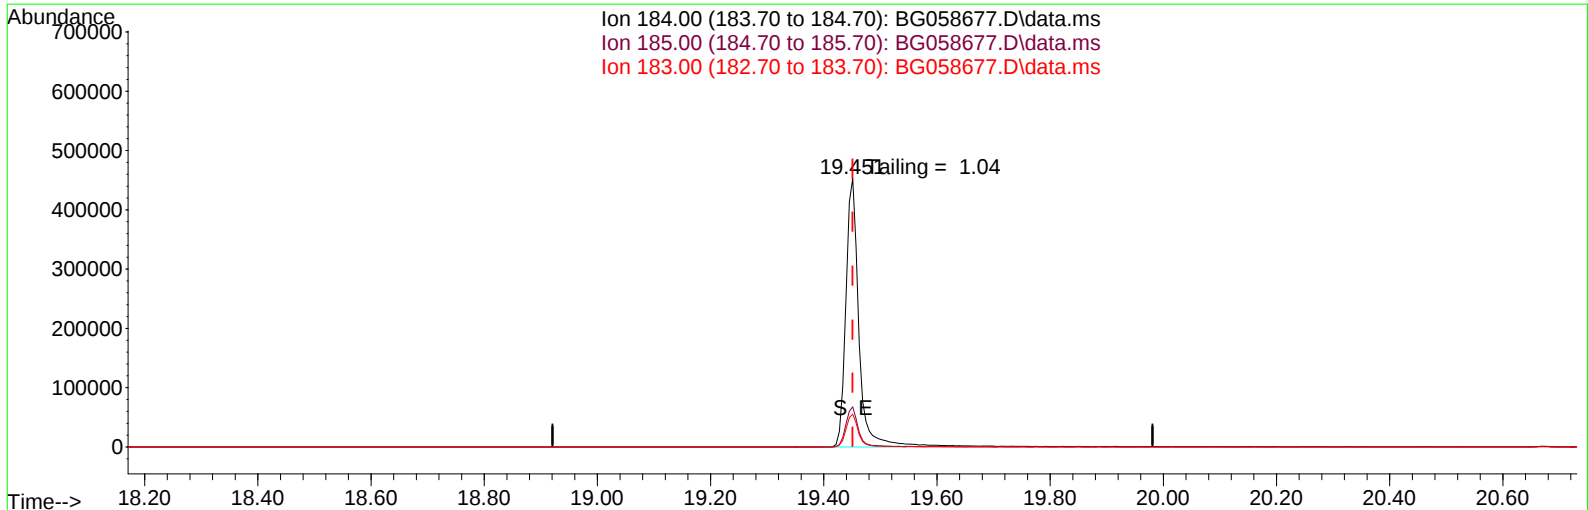

TIC: BG058677.D\data.ms

(77) Benzidine

19.451min (+ 0.001) 76109.67 ng

response 732873

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.97
183.00	10.90	12.18
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/10/2023	BNA_G	<u>BG058677.D</u>
Compound Name	Response	Retention Time
DDT	347736	20.673
DDD	7146	20.238
DDE	576	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7722	355458	2.17

Instrument :
BNA_G
ClientSampleId :
DFTPP