
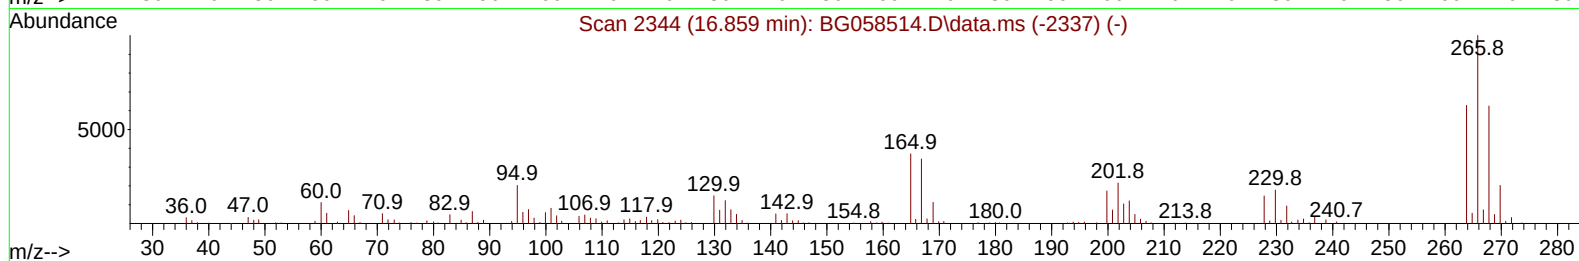
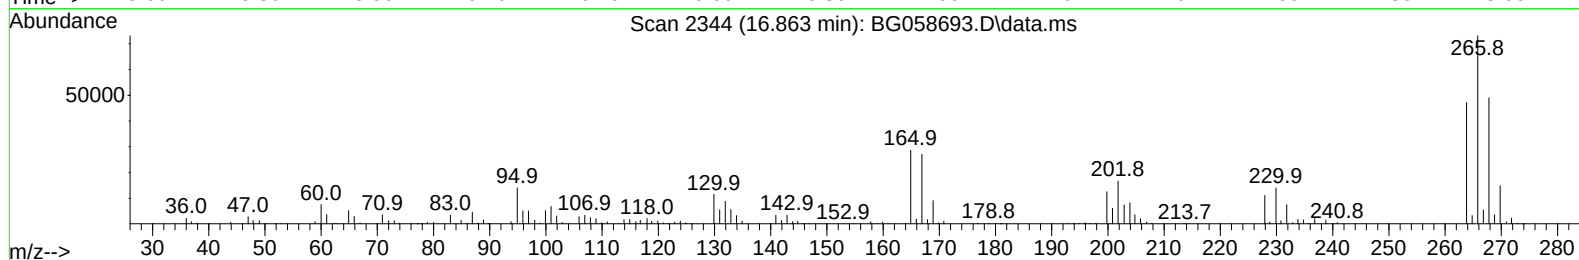


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081123\
Data File : BG058693.D
Acq On : 11 Aug 2023 7:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 11 11:28:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

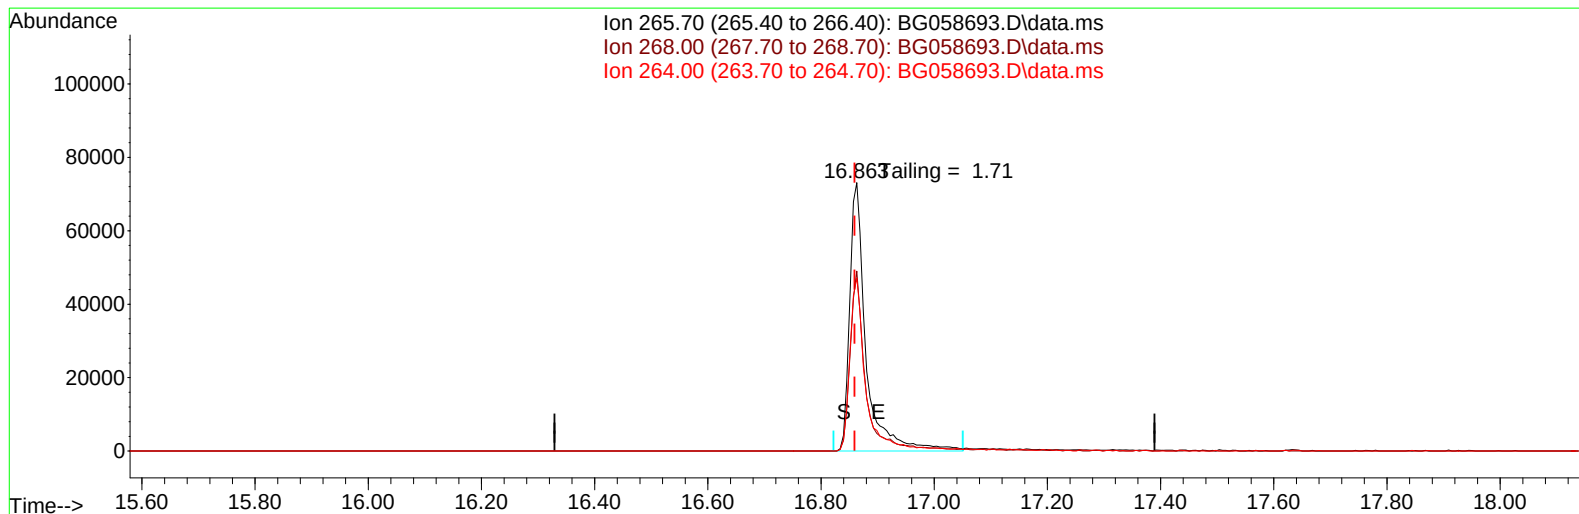

TIC: BG058693.D\data.ms

(70) Pentachlorophenol (C)




16.863min (+ 0.004) 24181.70 ng m

response 147944

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	67.04
264.00	62.80	64.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081123\
Data File : BG058693.D
Acq On : 11 Aug 2023 7:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 11 11:28:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

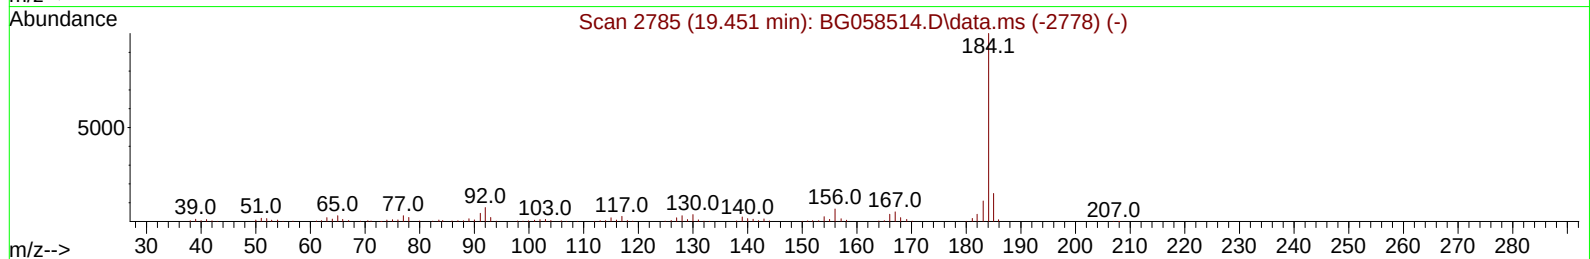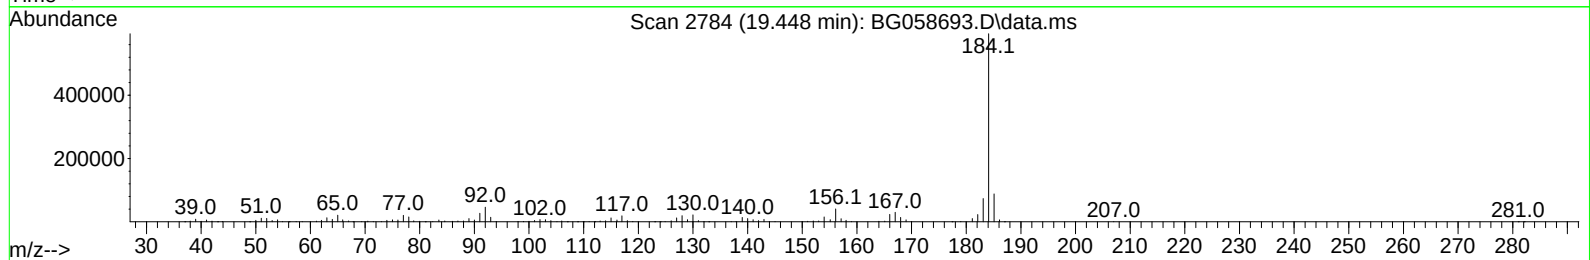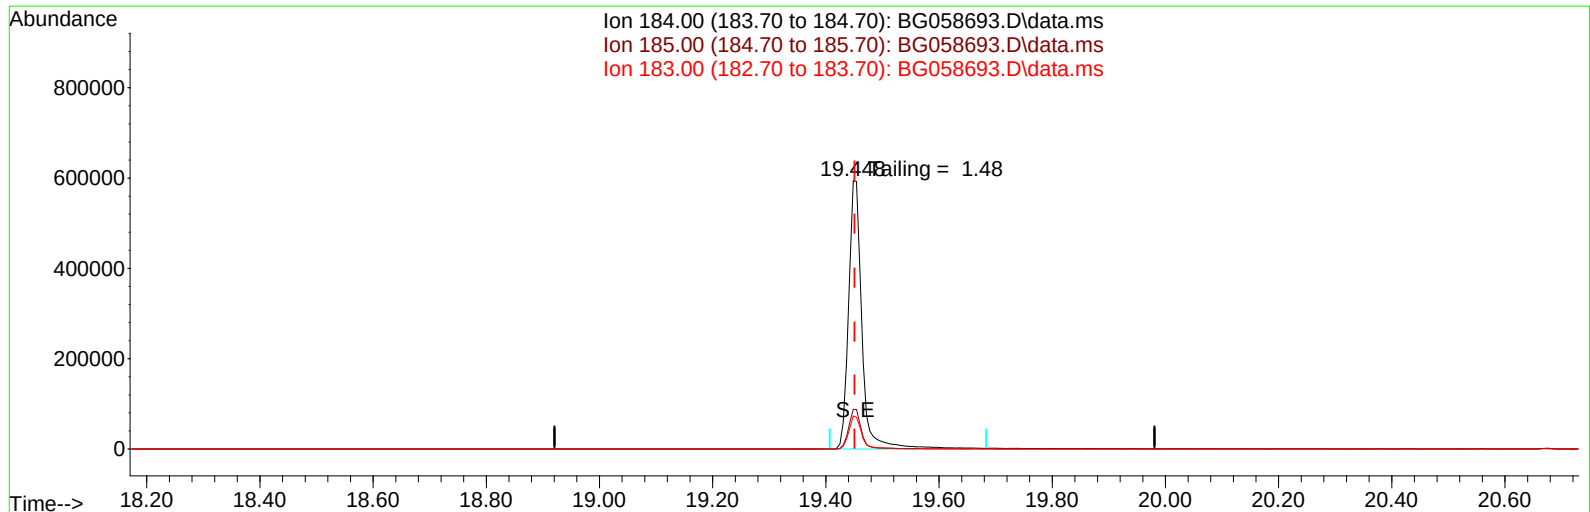

TIC: BG058693.D\data.ms

(77) Benzidine

19.448min (-0.002) 0.00 ng

response 983545

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.83
183.00	10.90	12.33
0.00	0.00	0.00