
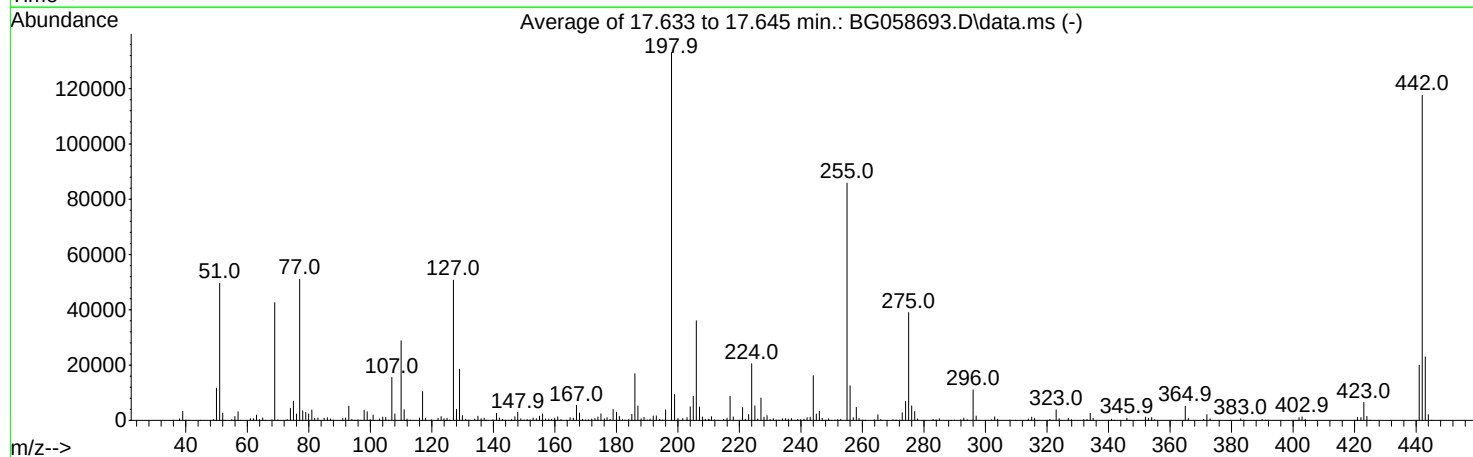


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081123\
Data File : BG058693.D
Acq On : 11 Aug 2023 7:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 28 22:29:07 2023

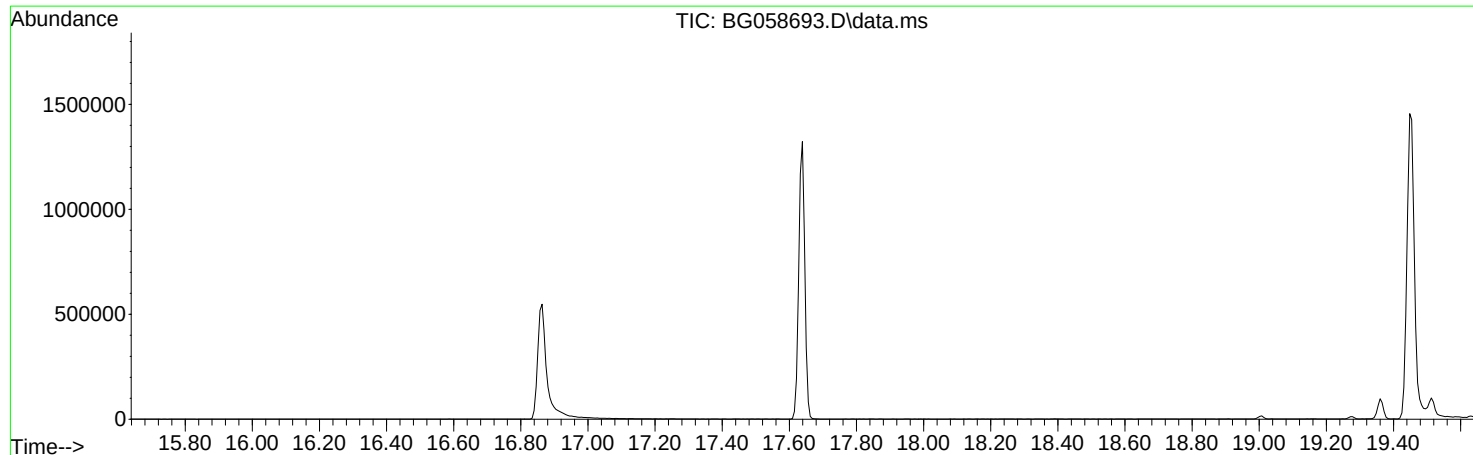




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	49576	PASS
68	69	0.00	2	0.4	188	PASS
69	198	0.00	100	32.0	42600	PASS
70	69	0.00	2	0.5	199	PASS
127	198	10	80	38.1	50728	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	133099	PASS
199	198	5	9	7.0	9349	PASS
275	198	10	60	29.3	39045	PASS
365	198	1	100	3.9	5153	PASS
441	198	0.01	100	15.0	19955	PASS
442	442	50	100	100.0	117600	PASS
443	442	15	24	19.5	22965	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081123\
Data File : BG058693.D
Acq On : 11 Aug 2023 7:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 11 11:28:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

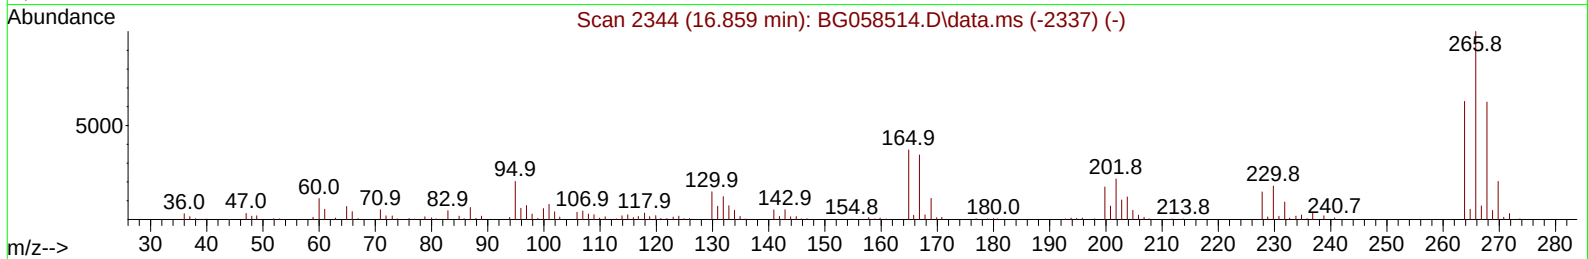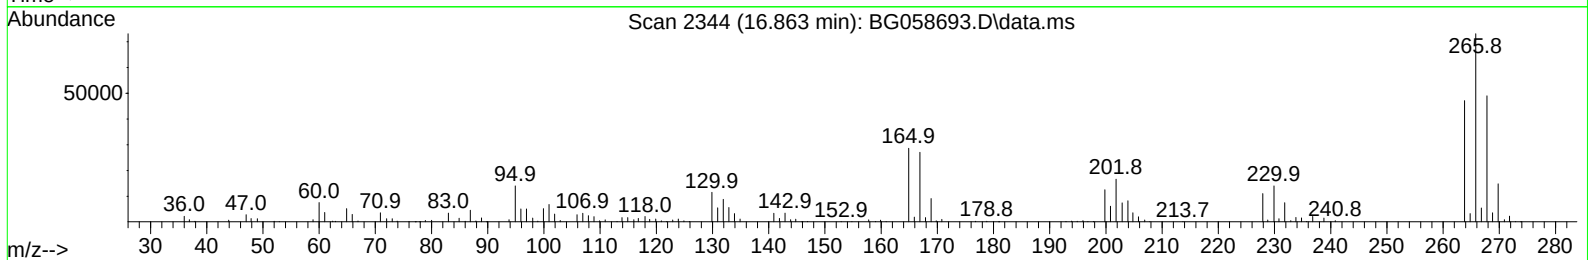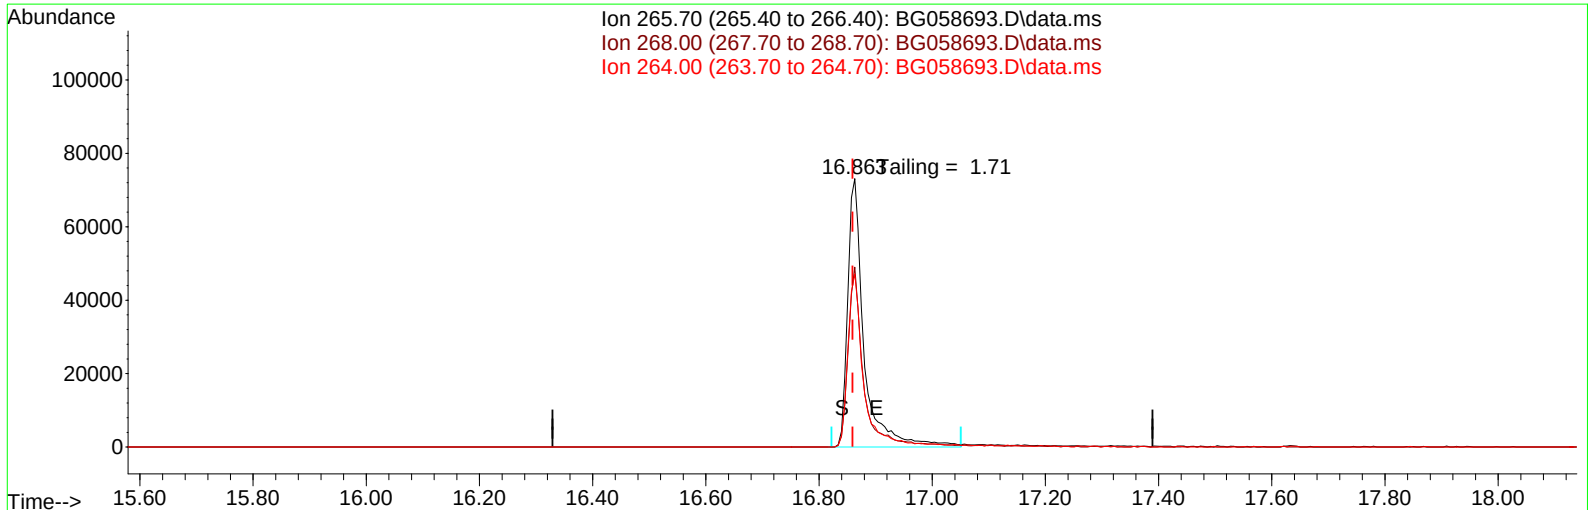

TIC: BG058693.D\data.ms

(70) Pentachlorophenol (C)

16.863min (+ 0.004) 24181.70 ng m




response 147944

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	67.04
264.00	62.80	64.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081123\
Data File : BG058693.D
Acq On : 11 Aug 2023 7:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 11 11:28:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

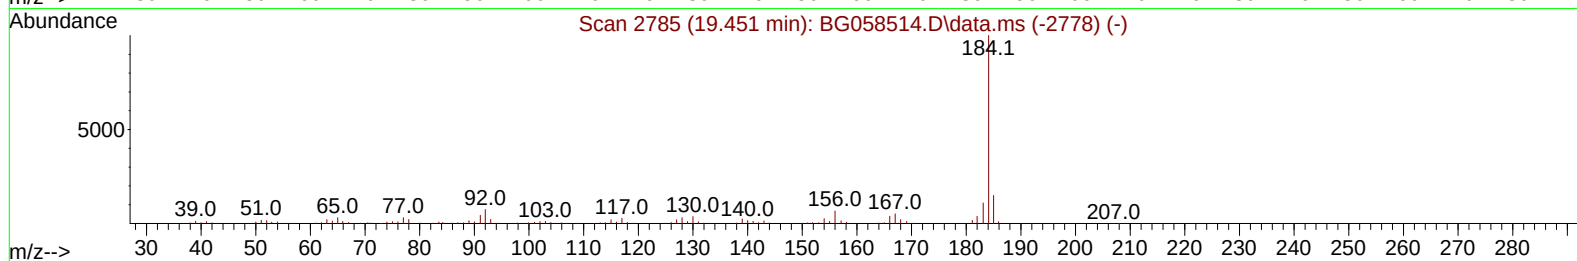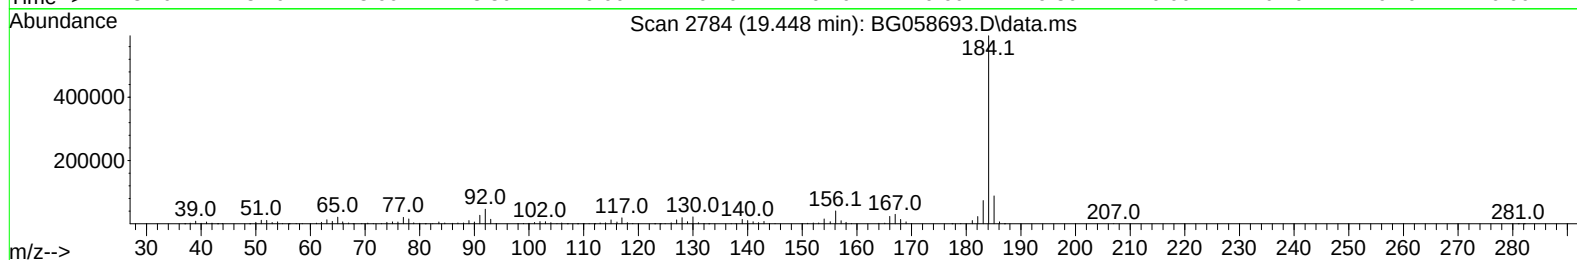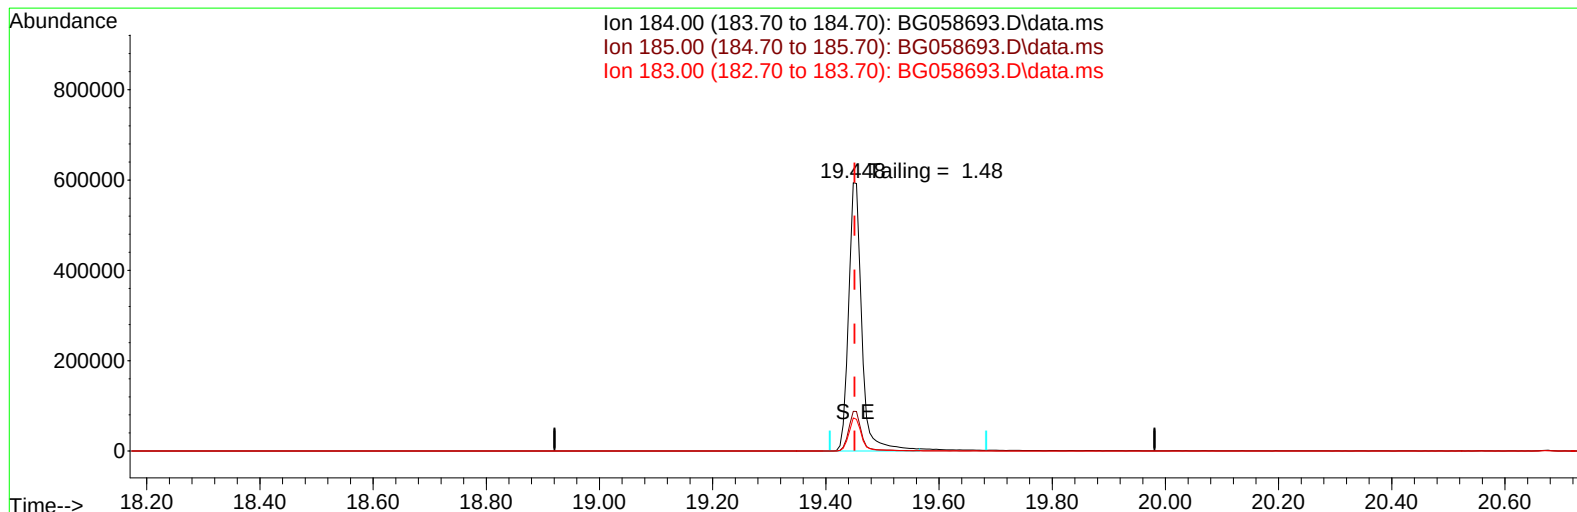

TIC: BG058693.D\data.ms

(77) Benzidine

19.448min (-0.002) 0.00 ng

response 983545

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.83
183.00	10.90	12.33
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/11/2023	BNA_G	<u>BG058693.D</u>
Compound Name	Response	Retention Time
DDT	488735	20.676
DDD	10177	20.236
DDE	871	19.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11048	499783	2.21

Instrument :
BNA_G
ClientSampleId :
DFTPP