
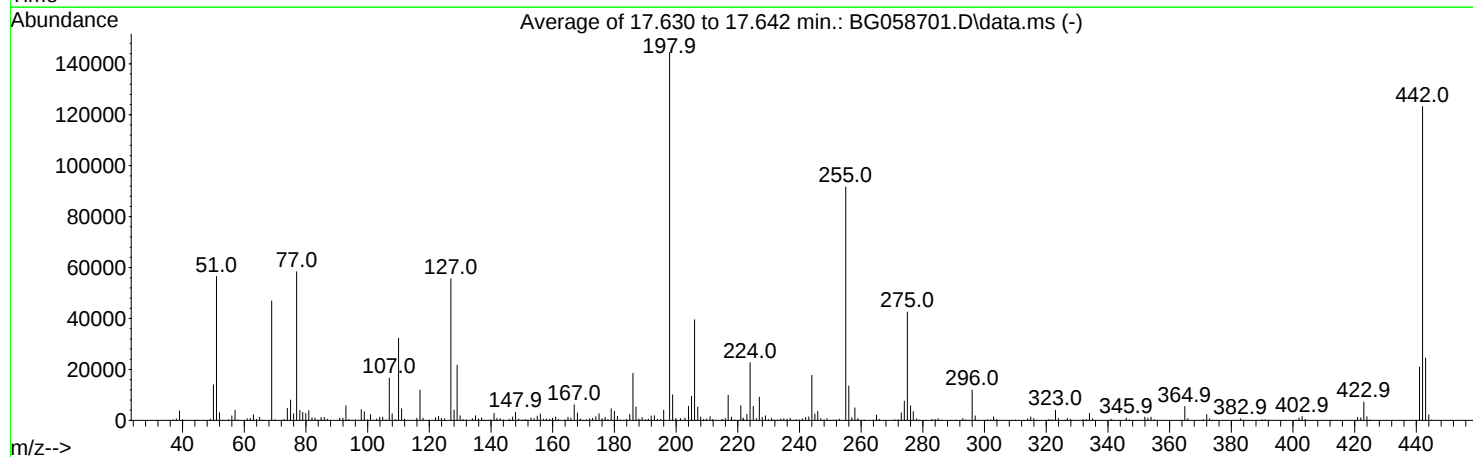


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081123\
Data File : BG058701.D
Acq On : 11 Aug 2023 13:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 28 22:29:07 2023

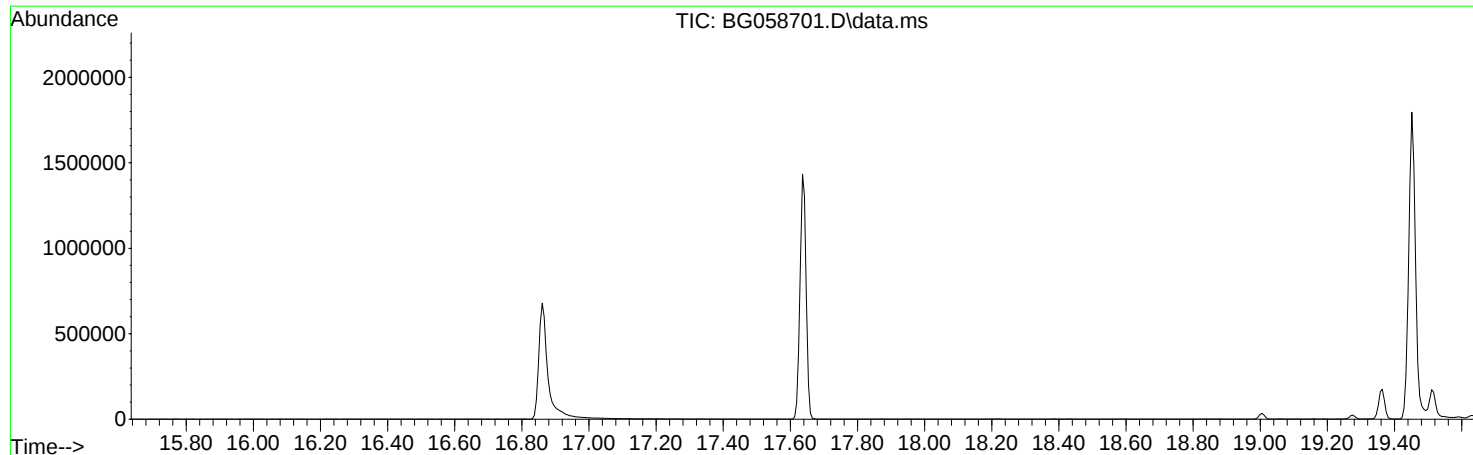




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	56472	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.4	46848	PASS
70	69	0.00	2	0.5	221	PASS
127	198	10	80	38.5	55579	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	144443	PASS
199	198	5	9	6.9	10038	PASS
275	198	10	60	29.4	42531	PASS
365	198	1	100	3.8	5453	PASS
441	198	0.01	100	14.5	20954	PASS
442	442	50	100	100.0	123216	PASS
443	442	15	24	19.9	24525	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081123\
Data File : BG058701.D
Acq On : 11 Aug 2023 13:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 11 19:04:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

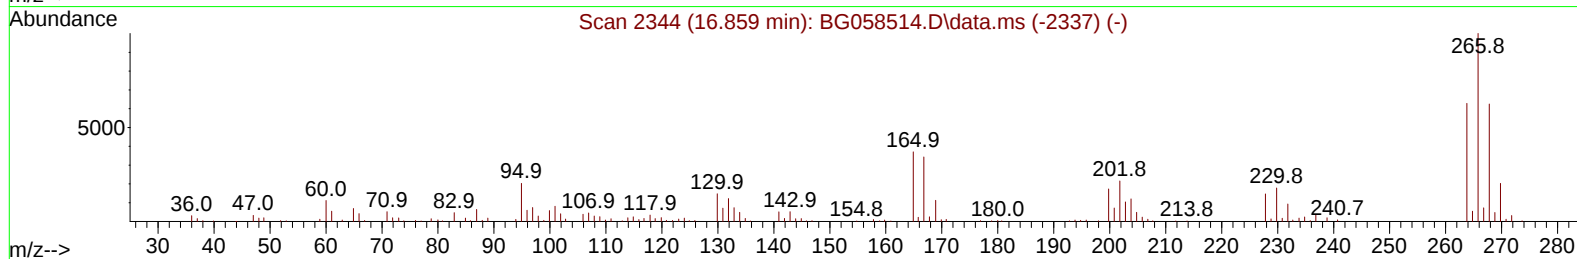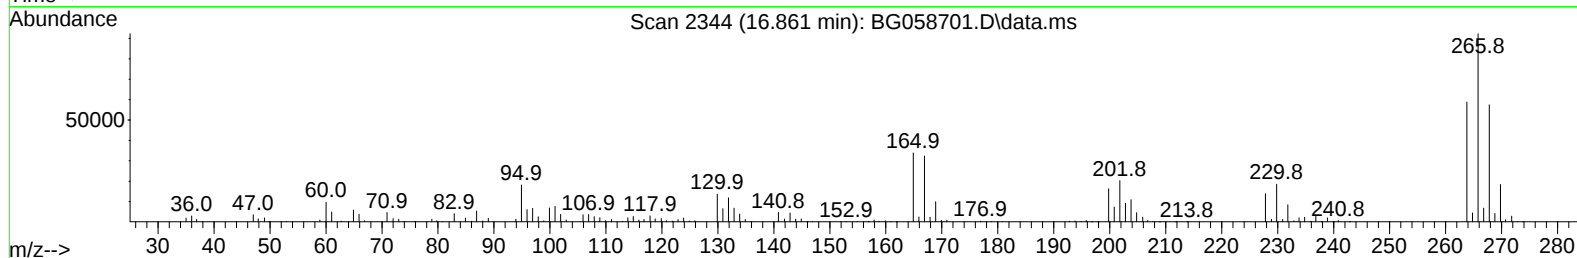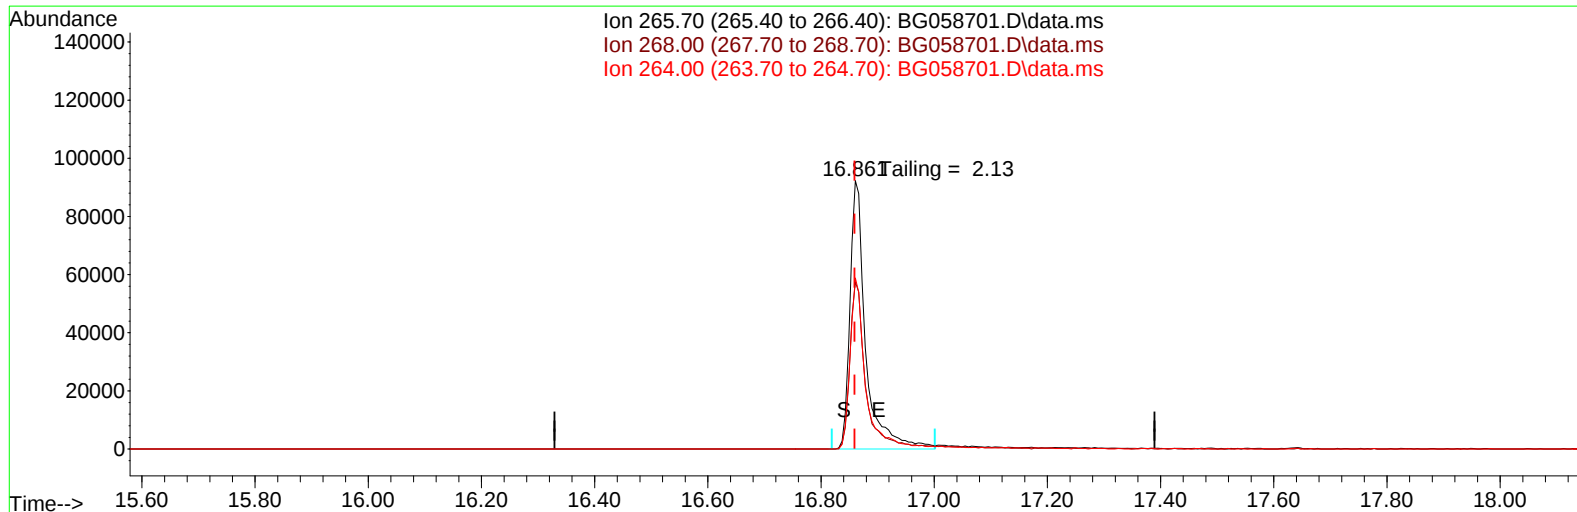

TIC: BG058701.D\data.ms

(70) Pentachlorophenol (C)

16.861min (+ 0.002) 32152.66 ng




response 178934

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	62.28
264.00	62.80	63.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081123\
Data File : BG058701.D
Acq On : 11 Aug 2023 13:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 11 19:04:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

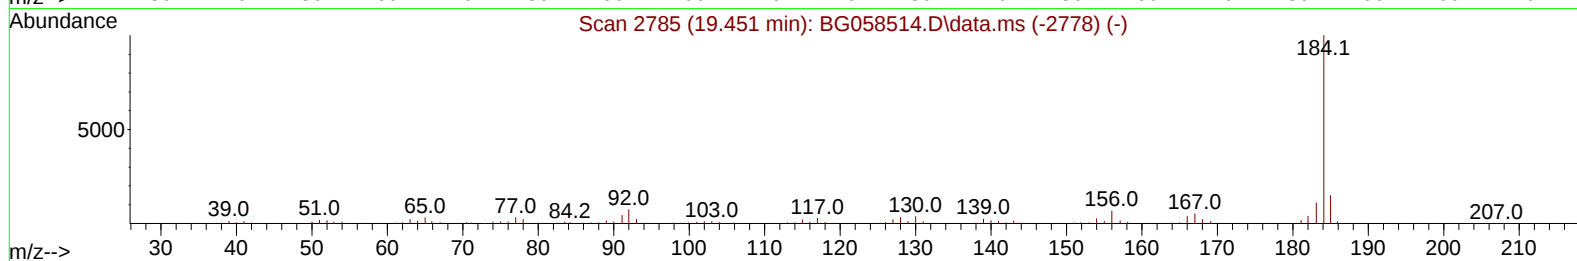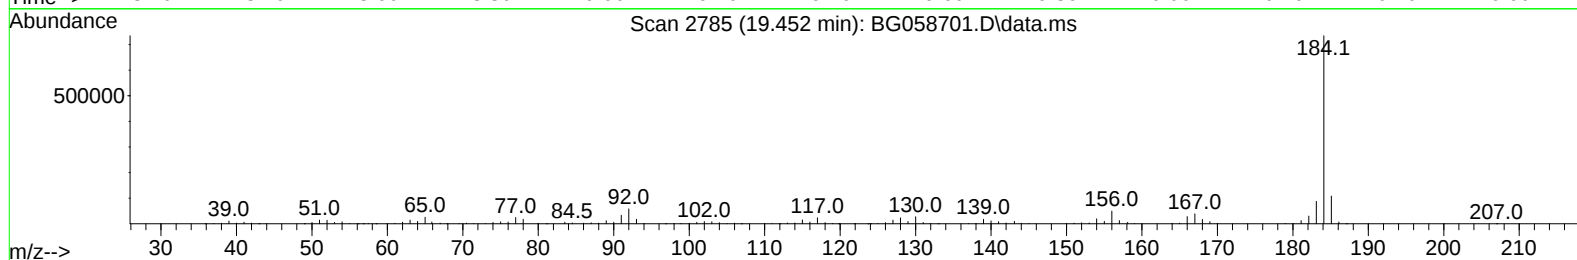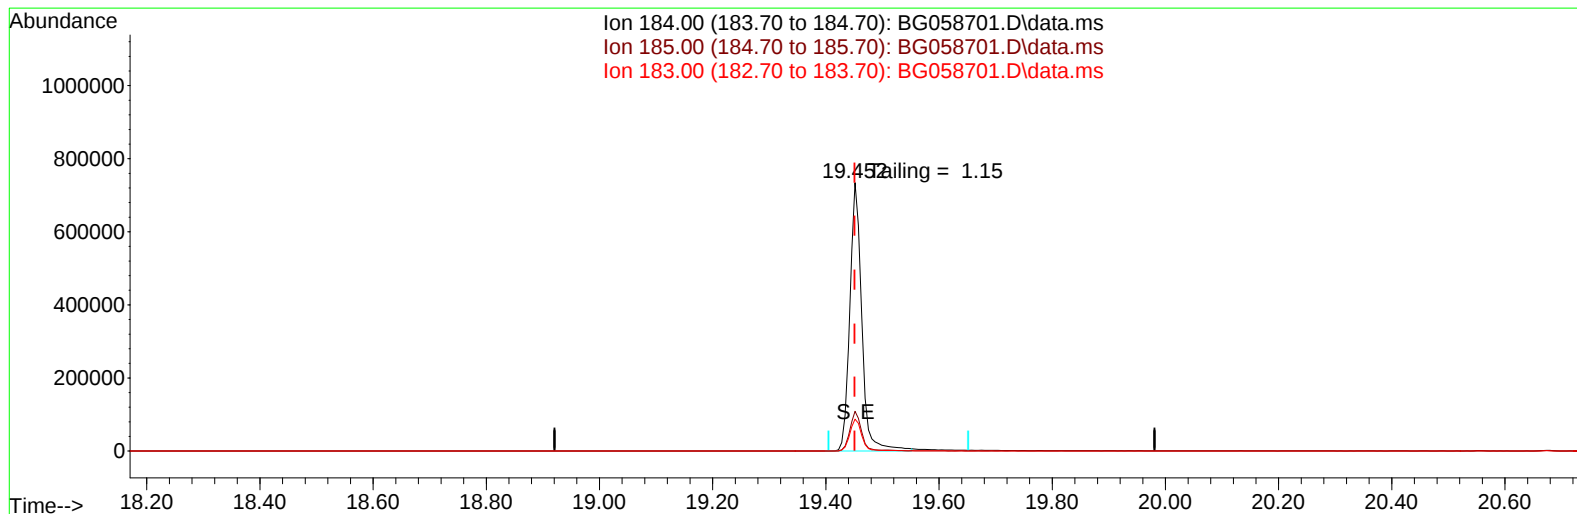

TIC: BG058701.D\data.ms

(77) Benzidine

19.452min (+ 0.001) 0.00 ng

response 1100223

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.79
183.00	10.90	11.91
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/11/2023	BNA_G	<u>BG058701.D</u>
Compound Name	Response	Retention Time
DDT	576458	20.674
DDD	14146	20.239
DDE	2112	19.734
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16258	592716	2.74

Instrument :
BNA_G
ClientSampleId :
DFTPP