
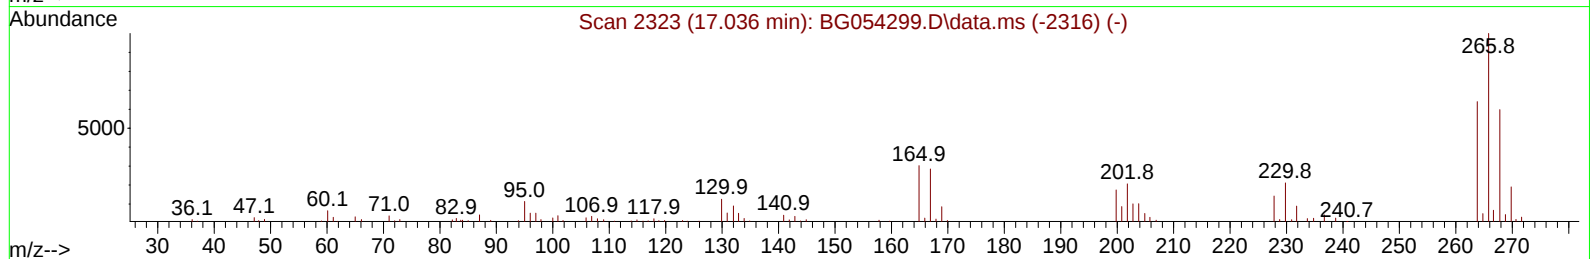
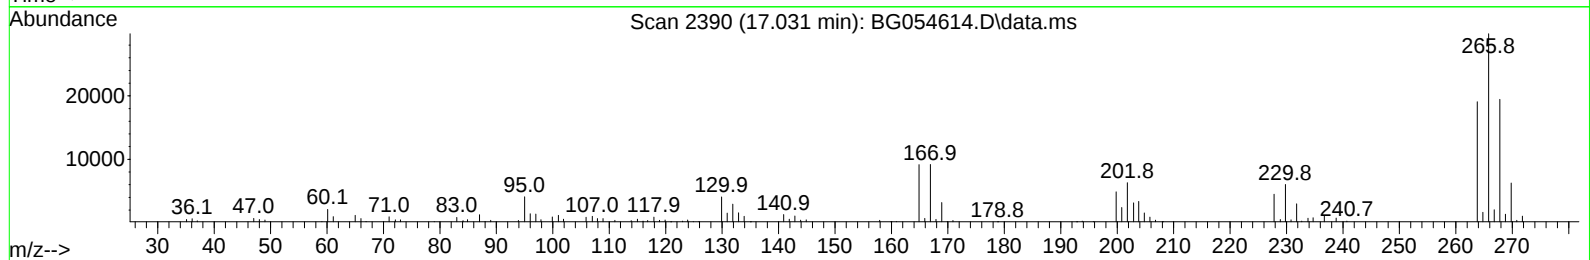


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081222\
Data File : BG054614.D
Acq On : 12 Aug 2022 9:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 09:46:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 08 14:48:51 2022
Response via : Initial Calibration

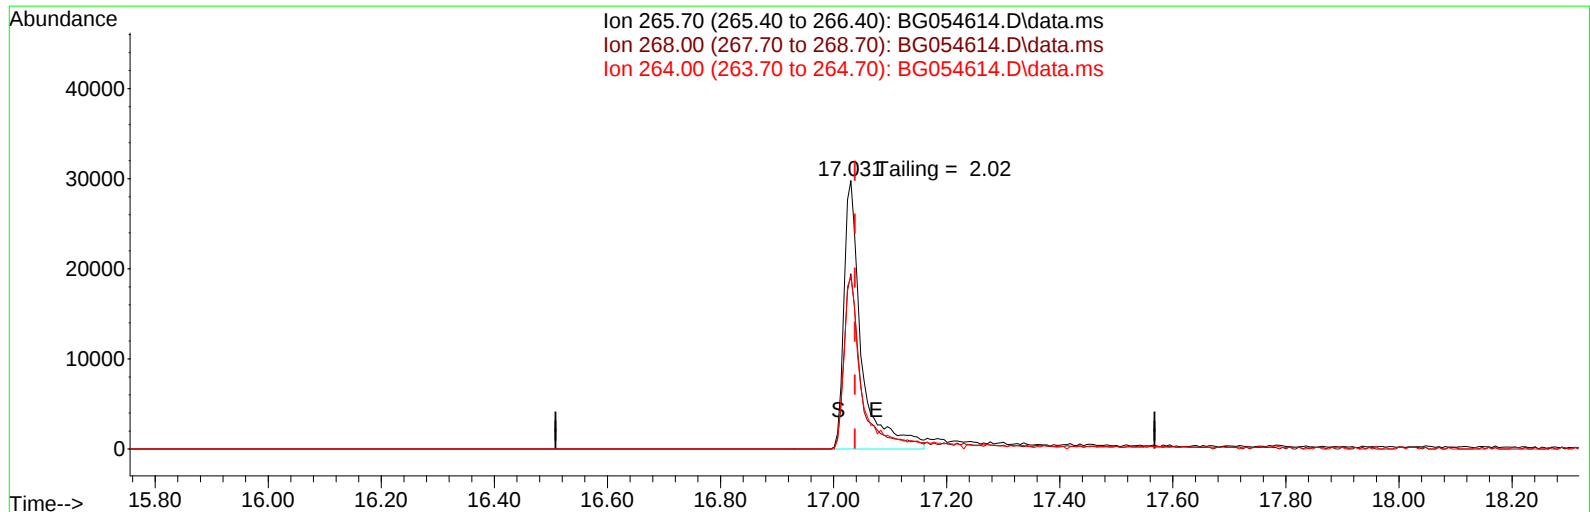

TIC: BG054614.D\data.ms

(70) Pentachlorophenol (C)




17.031min (-0.008) 17367.63 ng

response 61831

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	65.28
264.00	66.20	64.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081222\
Data File : BG054614.D
Acq On : 12 Aug 2022 9:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 09:46:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 08 14:48:51 2022
Response via : Initial Calibration

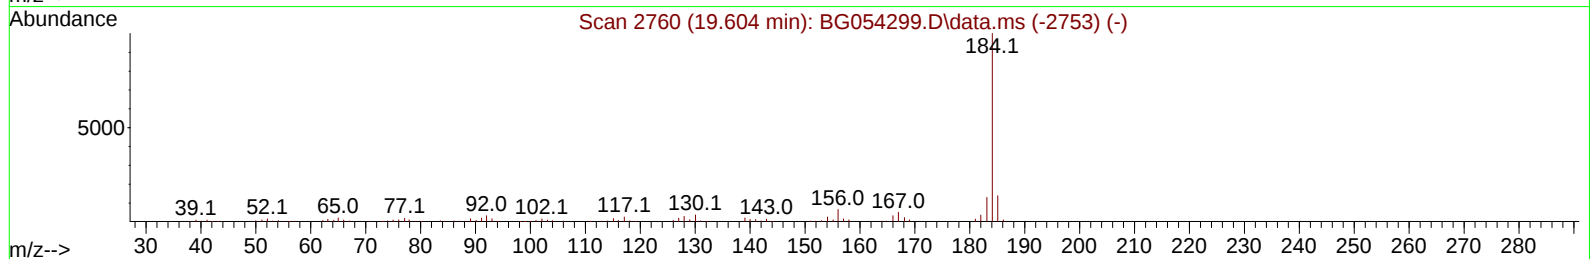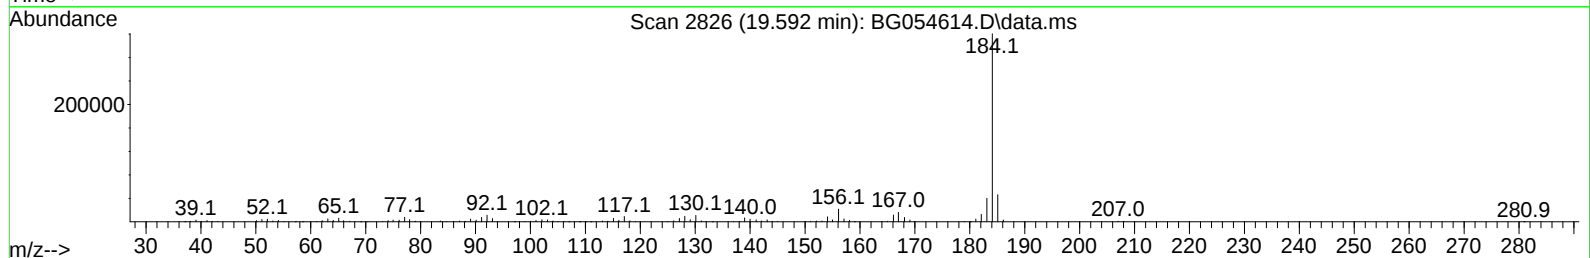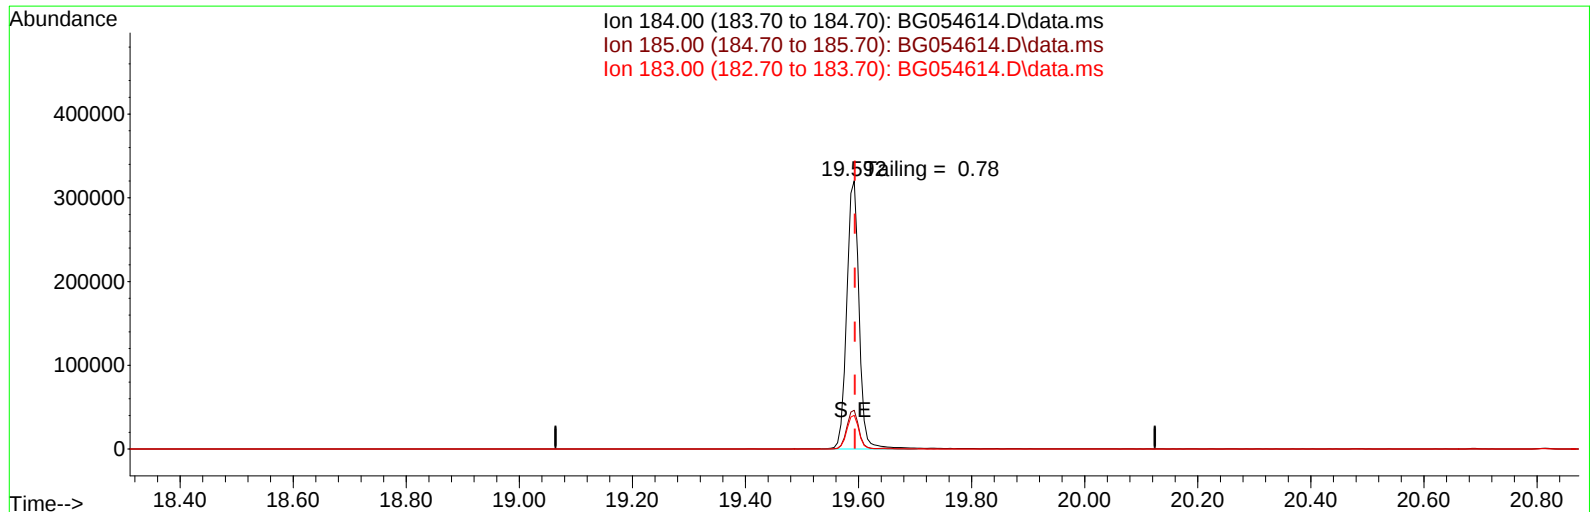

TIC: BG054614.D\data.ms

(77) Benzidine**19.592min (-0.002) 177037.47 ng****response 487355**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.44
183.00	11.10	12.54
0.00	0.00	0.00