


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081222\
Data File : BG054614.D
Acq On : 12 Aug 2022 9:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Aug 13 00:32:40 2022

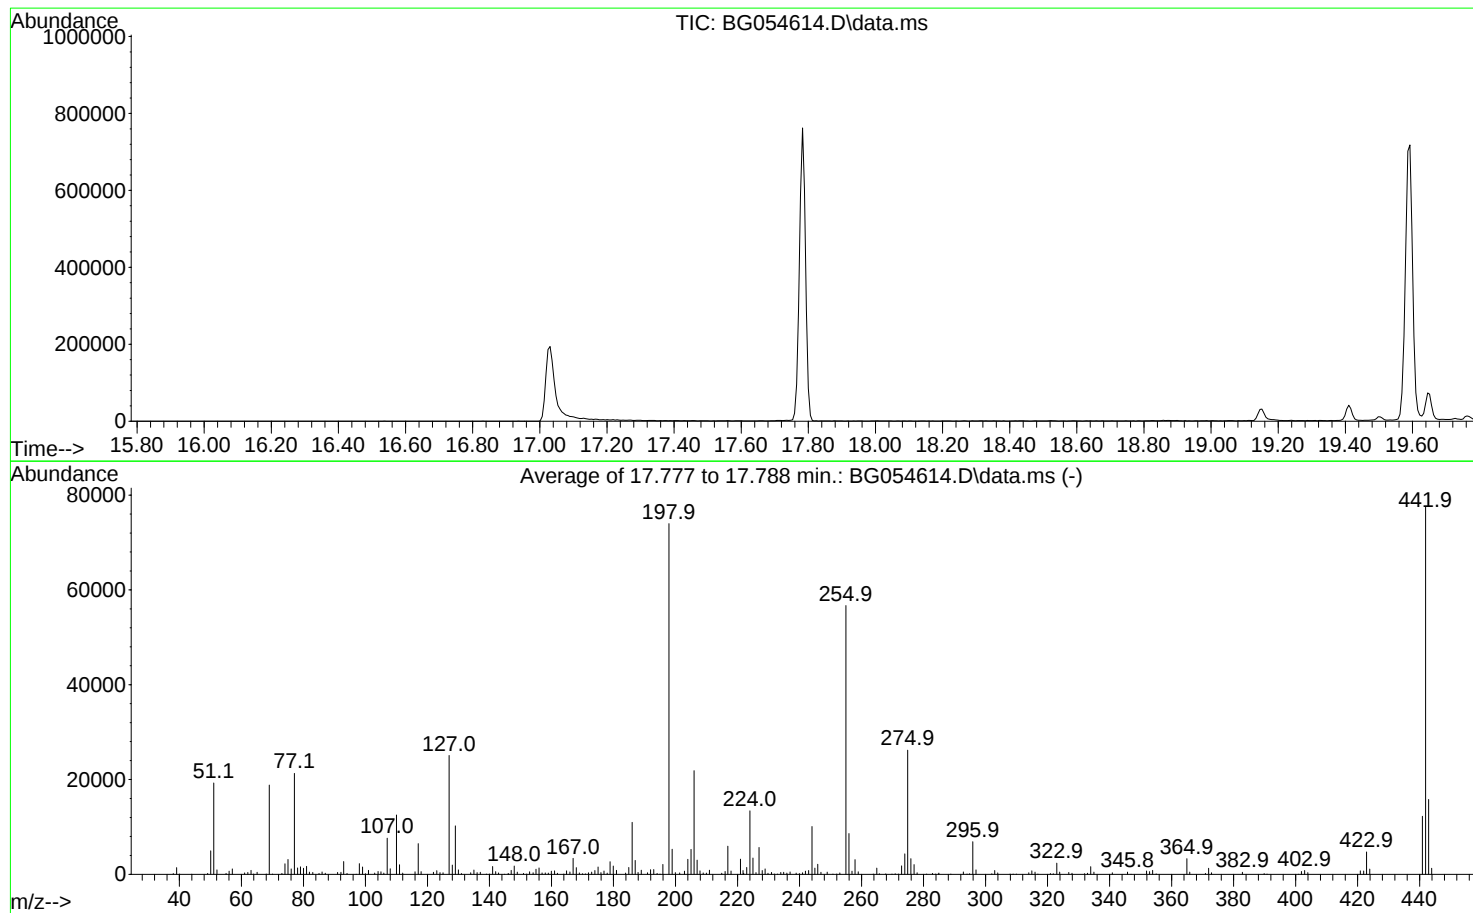




AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.1	19277	PASS
68	69	0.00	2	0.4	76	PASS
69	198	0.00	100	25.5	18850	PASS
70	69	0.00	2	0.3	54	PASS
127	198	10	80	33.9	25085	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	73992	PASS
199	198	5	9	7.2	5306	PASS
275	198	10	60	35.4	26208	PASS
365	198	1	100	4.5	3303	PASS
441	198	0.01	100	16.6	12253	PASS
442	442	50	100	100.0	77603	PASS
443	442	15	24	20.4	15793	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081222\
 Data File : BG054614.D
 Acq On : 12 Aug 2022 9:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Aug 12 09:46:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 08 14:48:51 2022
 Response via : Initial Calibration

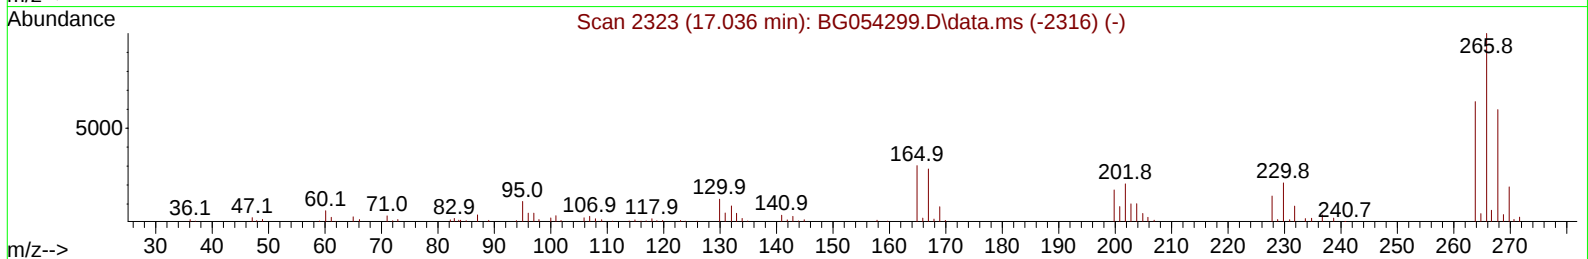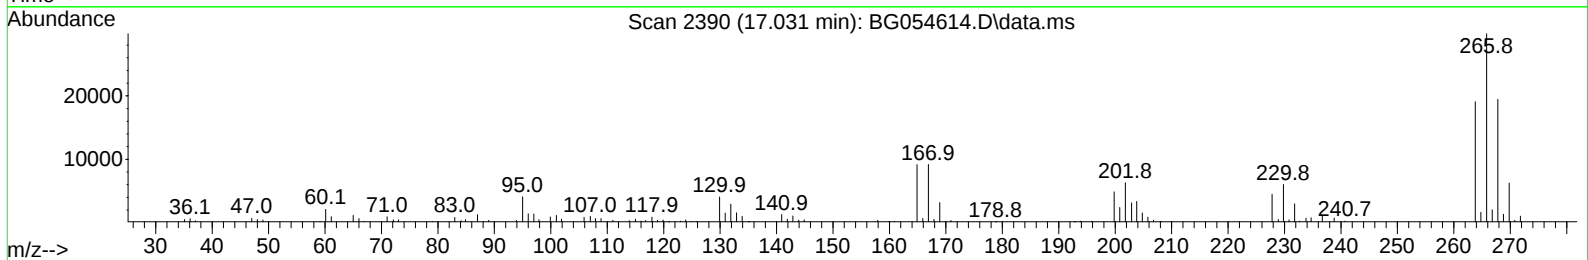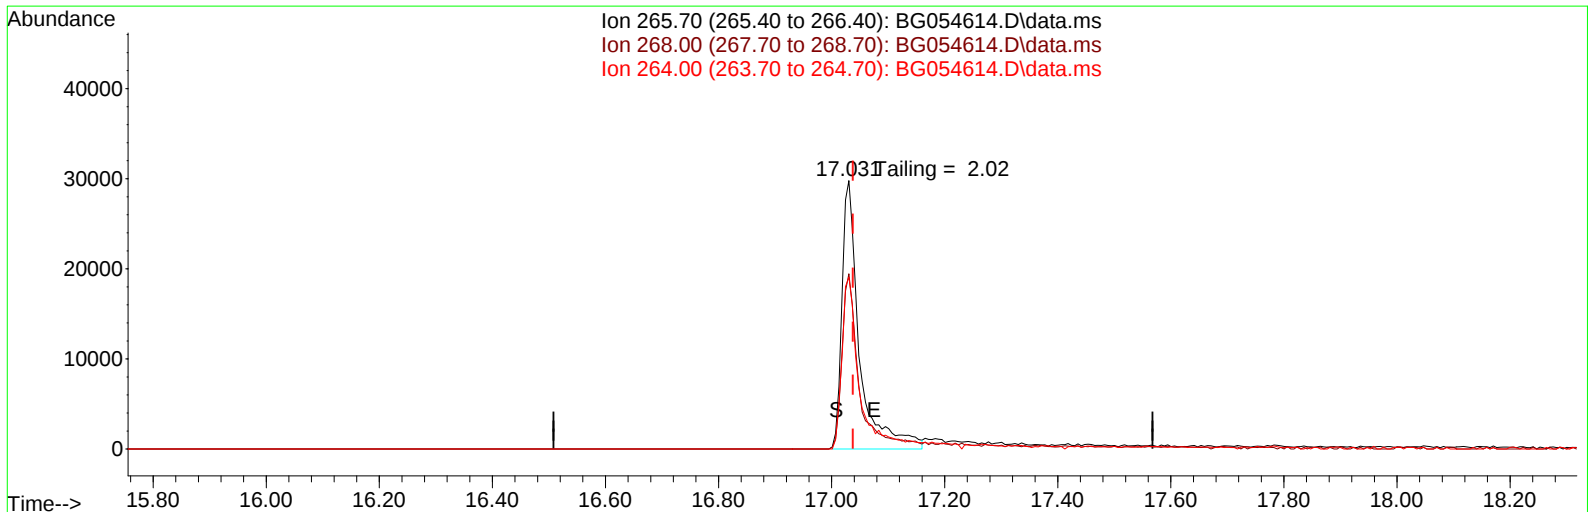

TIC: BG054614.D\data.ms

(70) Pentachlorophenol (C)

17.031min (-0.008) 17367.63 ng




response 61831

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	65.28
264.00	66.20	64.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081222\
Data File : BG054614.D
Acq On : 12 Aug 2022 9:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 12 09:46:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 08 14:48:51 2022
Response via : Initial Calibration

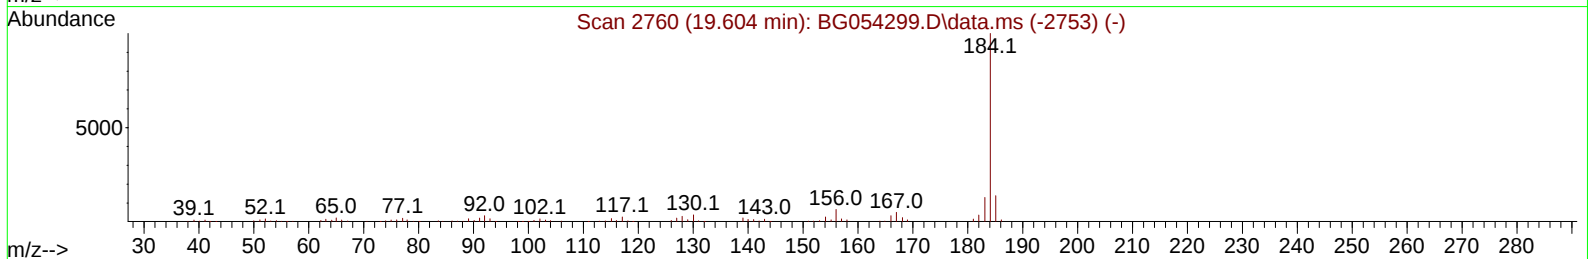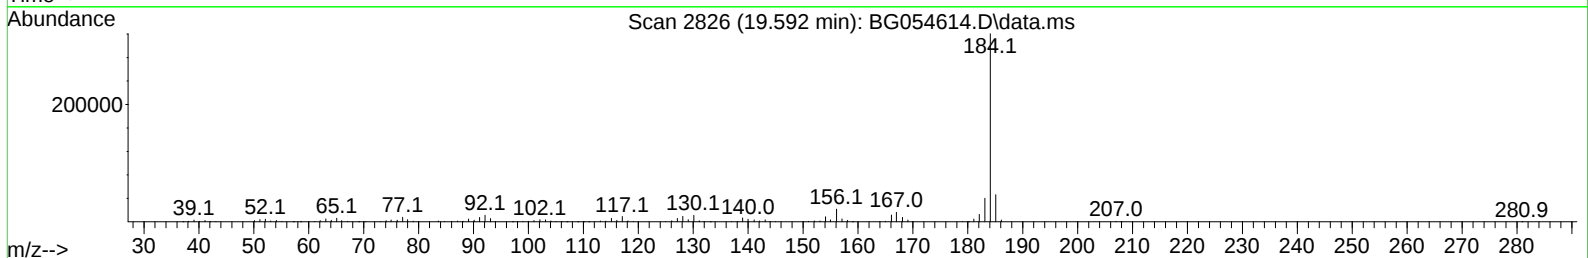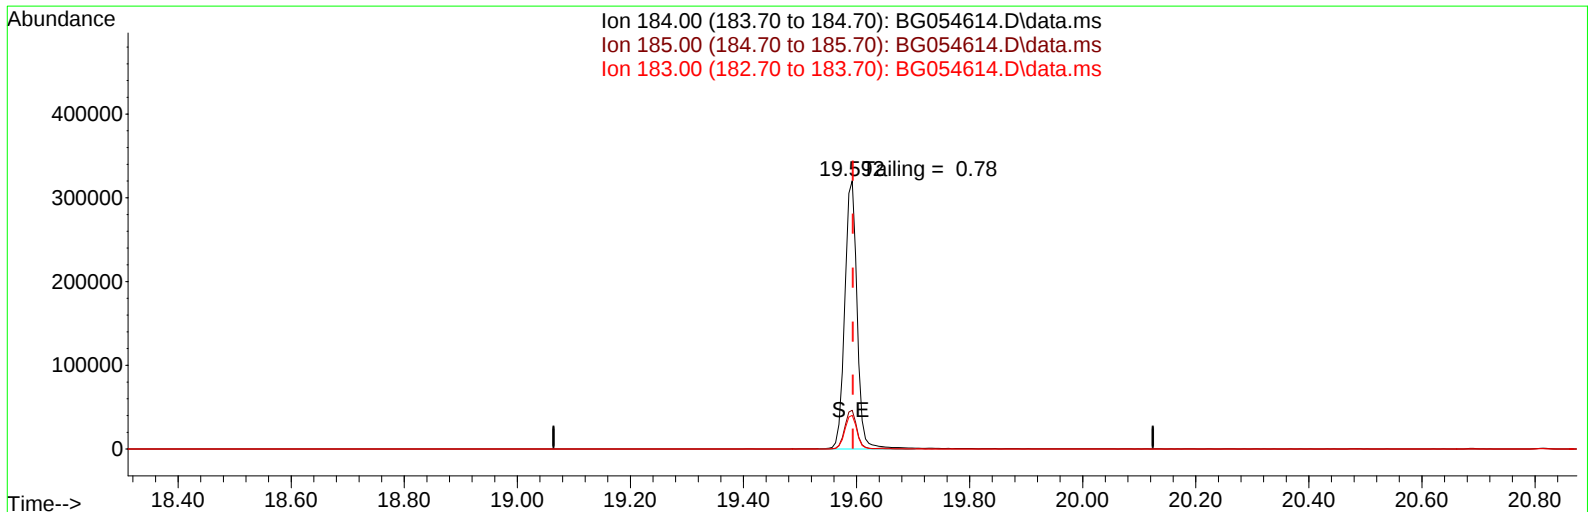

TIC: BG054614.D\data.ms

(77) Benzidine

19.592min (-0.002) 177037.47 ng

response 487355

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.44
183.00	11.10	12.54
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/12/2022	BNA_G	<u>BG054614.D</u>
Compound Name	Response	Retention Time
DDT	287170	20.814
DDD	14381	20.38
DDE	777	19.874
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15158	302328	5.01

Instrument :
BNA_G
ClientSampleId :
DFTPP