
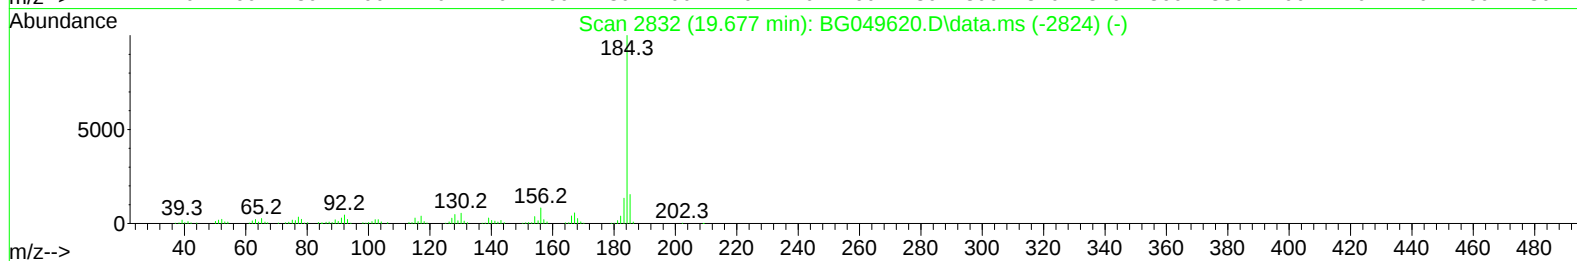
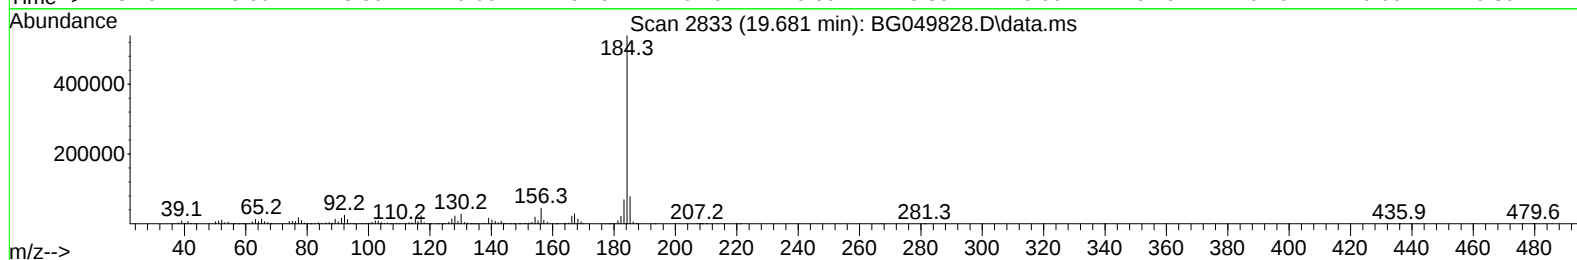


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081321\
Data File : BG049828.D
Acq On : 13 Aug 2021 9:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 13 10:53:42 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 15:15:33 2021
Response via : Initial Calibration

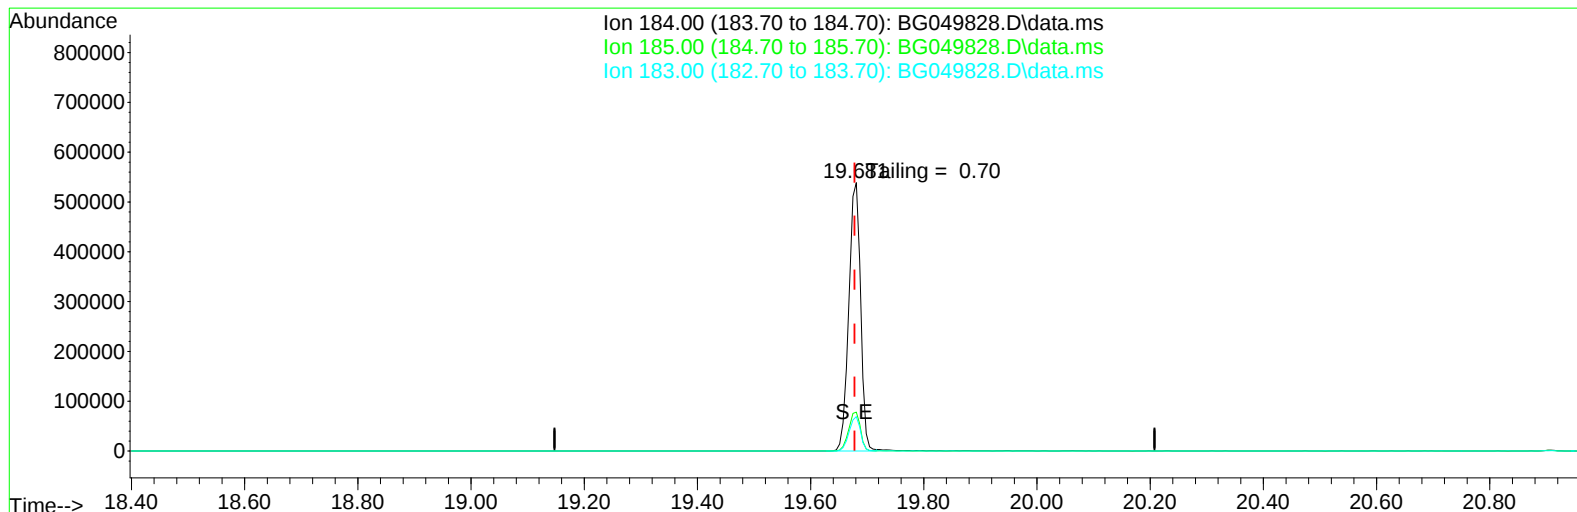

TIC: BG049828.D\data.ms

(77) Benzidine




19.681min (+ 0.003) 525703.44 ng

response 781239

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.53
183.00	11.70	12.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081321\
 Data File : BG049828.D
 Acq On : 13 Aug 2021 9:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 13 10:53:42 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 03 15:15:33 2021
 Response via : Initial Calibration

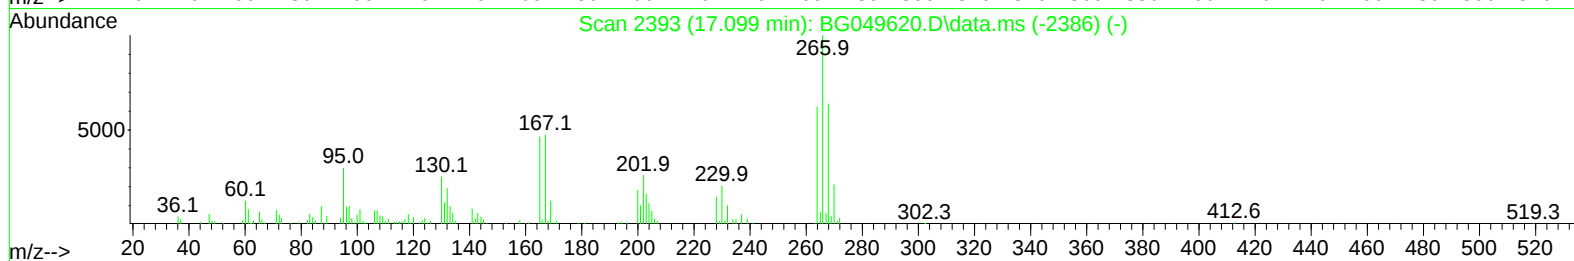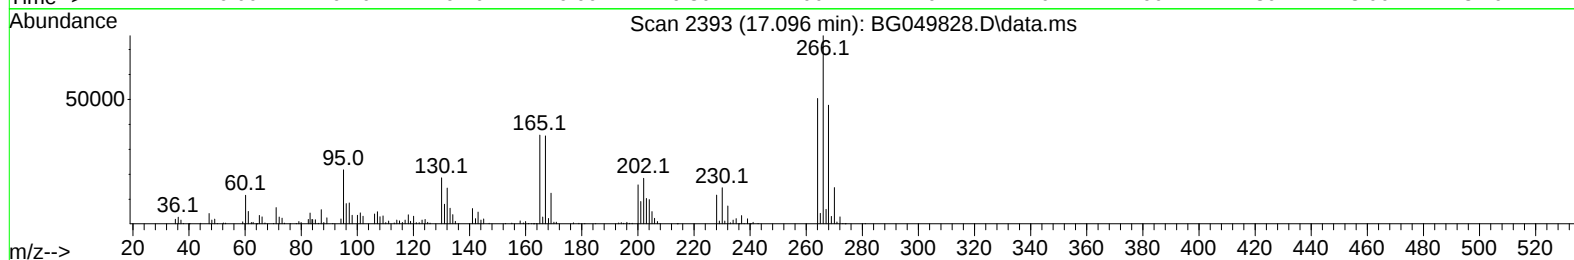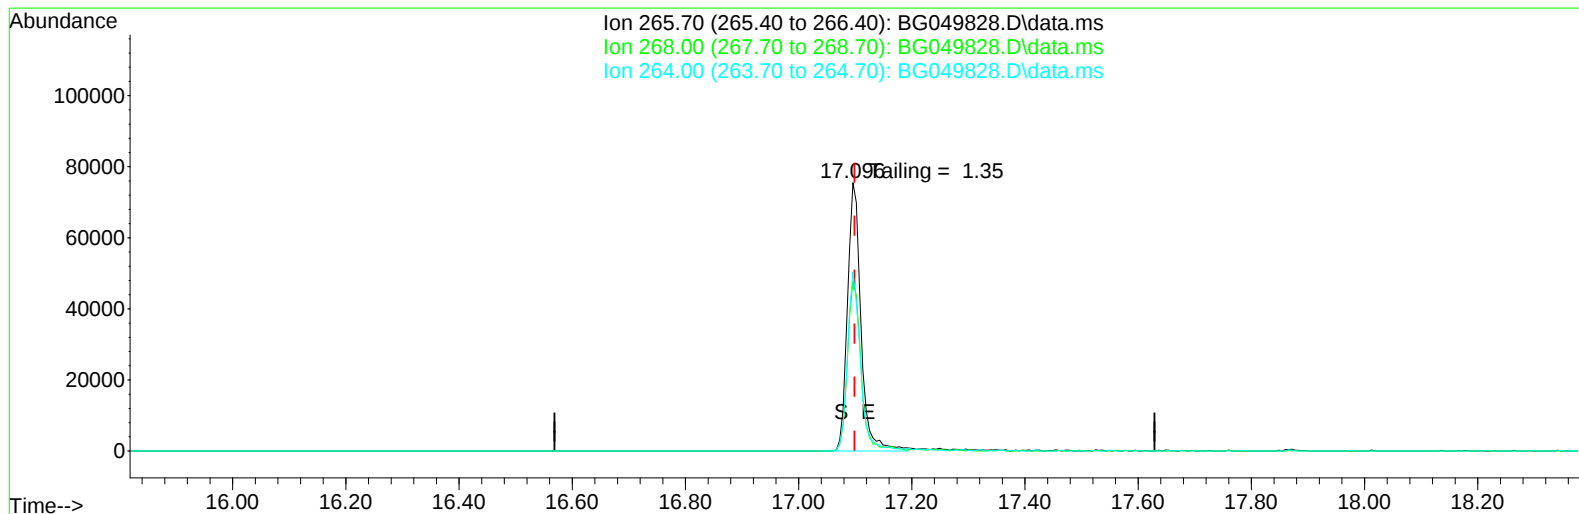

TIC: BG049828.D\data.ms

(70) Pentachlorophenol (C)

17.096min (-0.003) 143224.05 ng

response 126616

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.11
264.00	61.30	66.72
0.00	0.00	0.00