
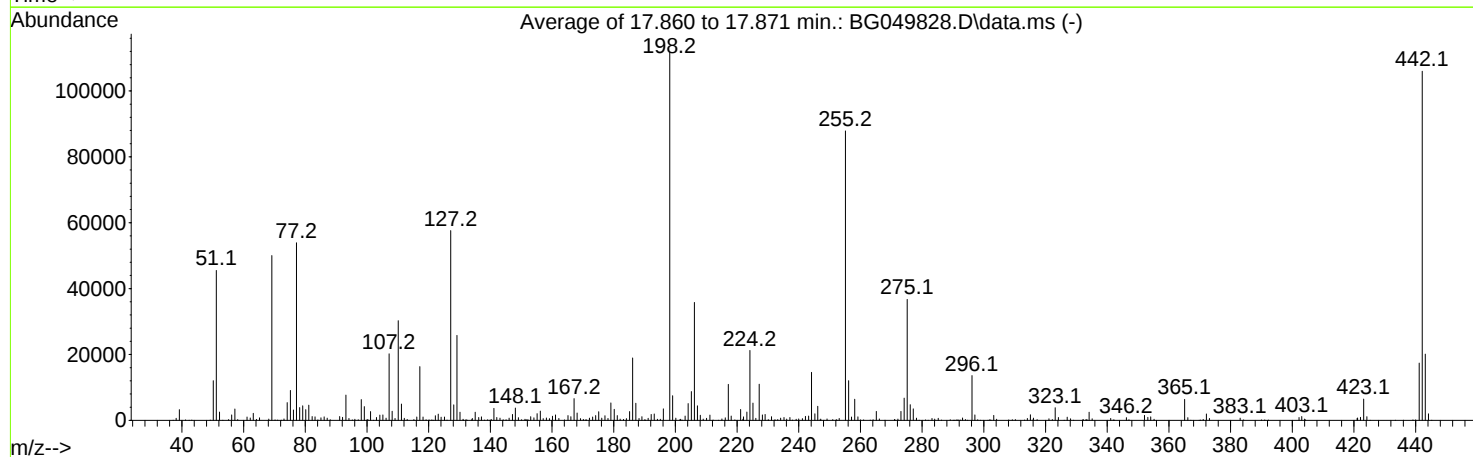


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG081321\  
 Data File : BG049828.D  
 Acq On : 13 Aug 2021 9:08  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG080321.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Aug 03 15:15:33 2021

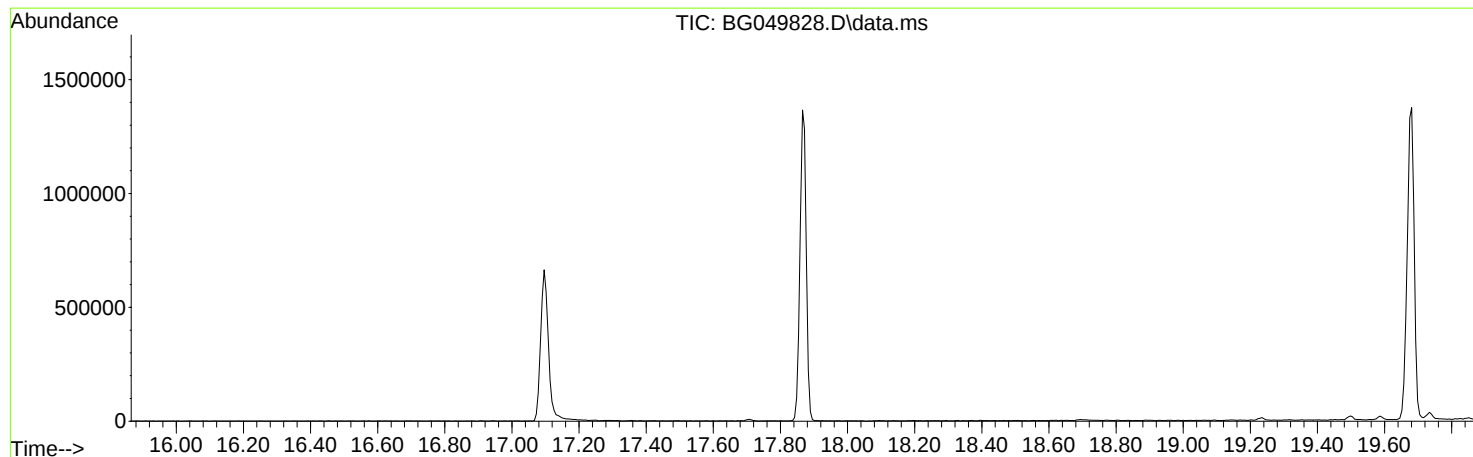

AutoFind: Scans 2523, 2524, 2525; Background Corrected with Scan 2516

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 40.8         | 45531      | PASS                |
| 68             | 69              | 0.00            | 2               | 0.8          | 393        | PASS                |
| 69             | 198             | 0.00            | 100             | 44.8         | 50059      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.3          | 144        | PASS                |
| 127            | 198             | 10              | 80              | 51.6         | 57635      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 111677     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 7474       | PASS                |
| 275            | 198             | 10              | 60              | 32.9         | 36741      | PASS                |
| 365            | 198             | 1               | 100             | 5.7          | 6375       | PASS                |
| 441            | 198             | 0.01            | 100             | 15.6         | 17405      | PASS                |
| 442            | 442             | 100             | 100             | 100.0        | 106013     | PASS                |
| 443            | 442             | 15              | 24              | 19.0         | 20126      | PASS                |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 8/13/2021     | BNA_G            | <u>BG049828.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 388122           | 20.9               |
| DDD           | 1859             | 20.46              |
| DDE           | 757              | 19.95              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 2616          | 390738           | 0.67               |
|               |                  |                    |

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG081321\  
Data File : BG049828.D  
Acq On : 13 Aug 2021 9:08  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Aug 13 10:53:42 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG080321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Aug 03 15:15:33 2021  
Response via : Initial Calibration

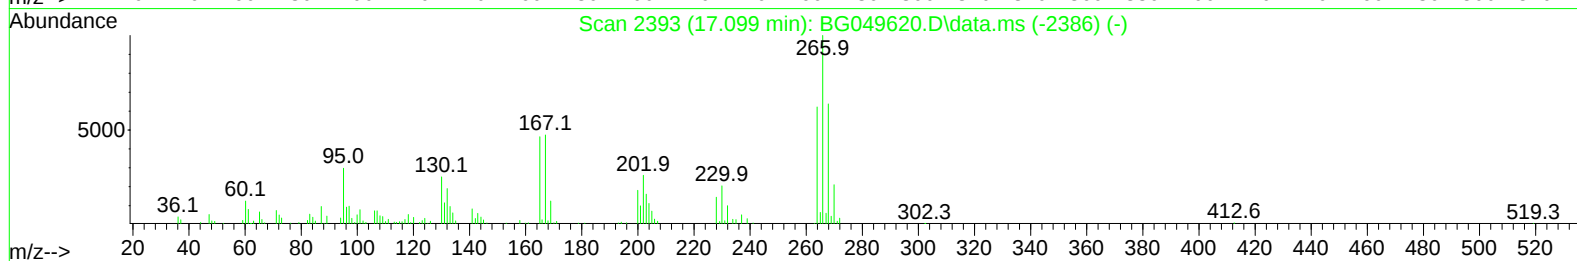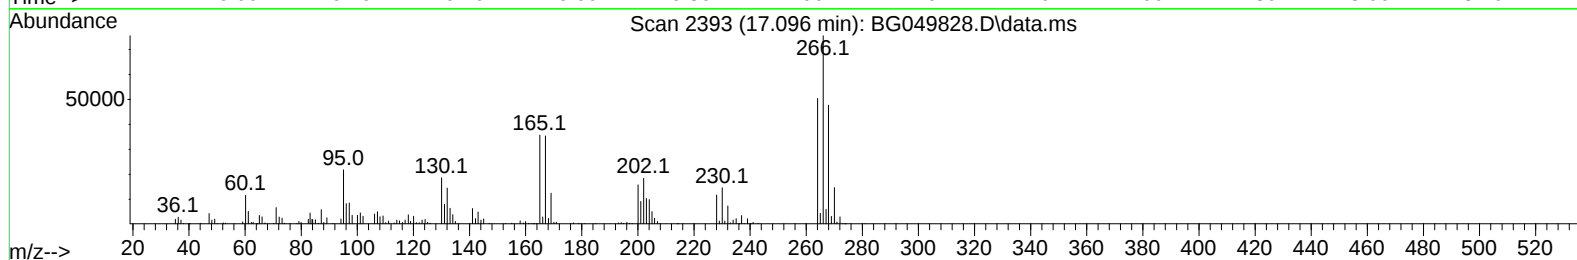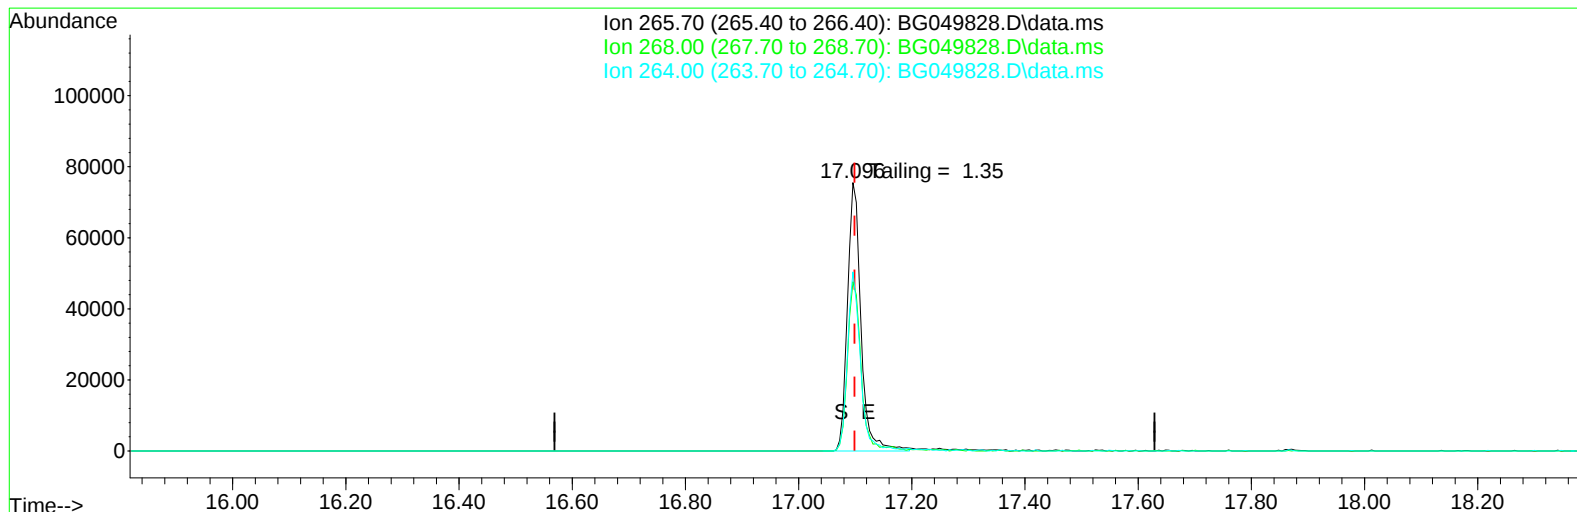

TIC: BG049828.D\data.ms

**(70) Pentachlorophenol (C)**

17.096min (-0.003) 143224.05 ng




response 126616

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.20  | 63.11  |
| 264.00 | 61.30  | 66.72  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG081321\  
Data File : BG049828.D  
Acq On : 13 Aug 2021 9:08  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Aug 13 10:53:42 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG080321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Aug 03 15:15:33 2021  
Response via : Initial Calibration

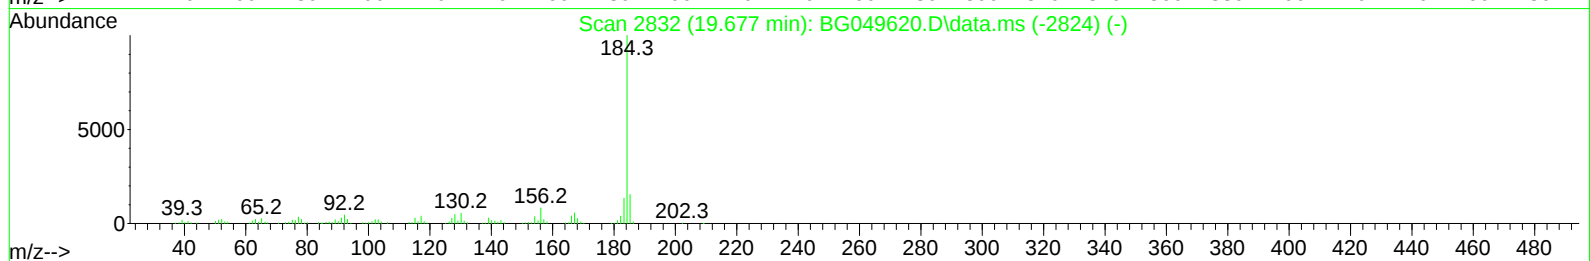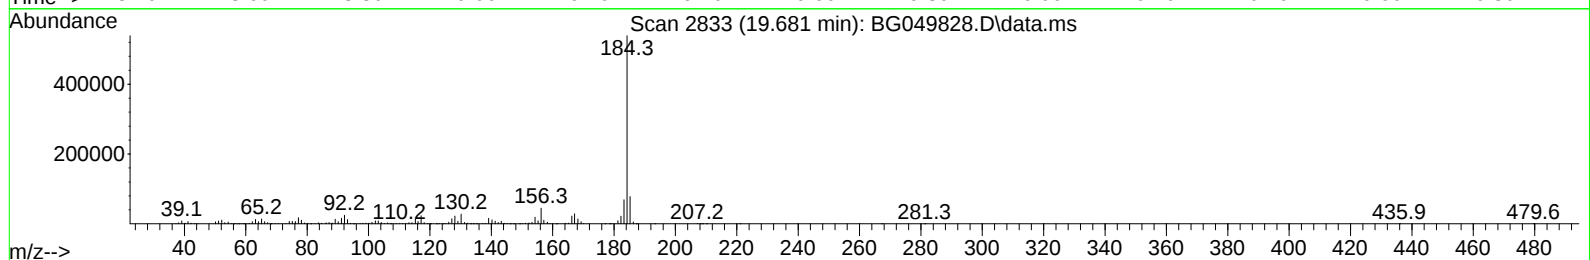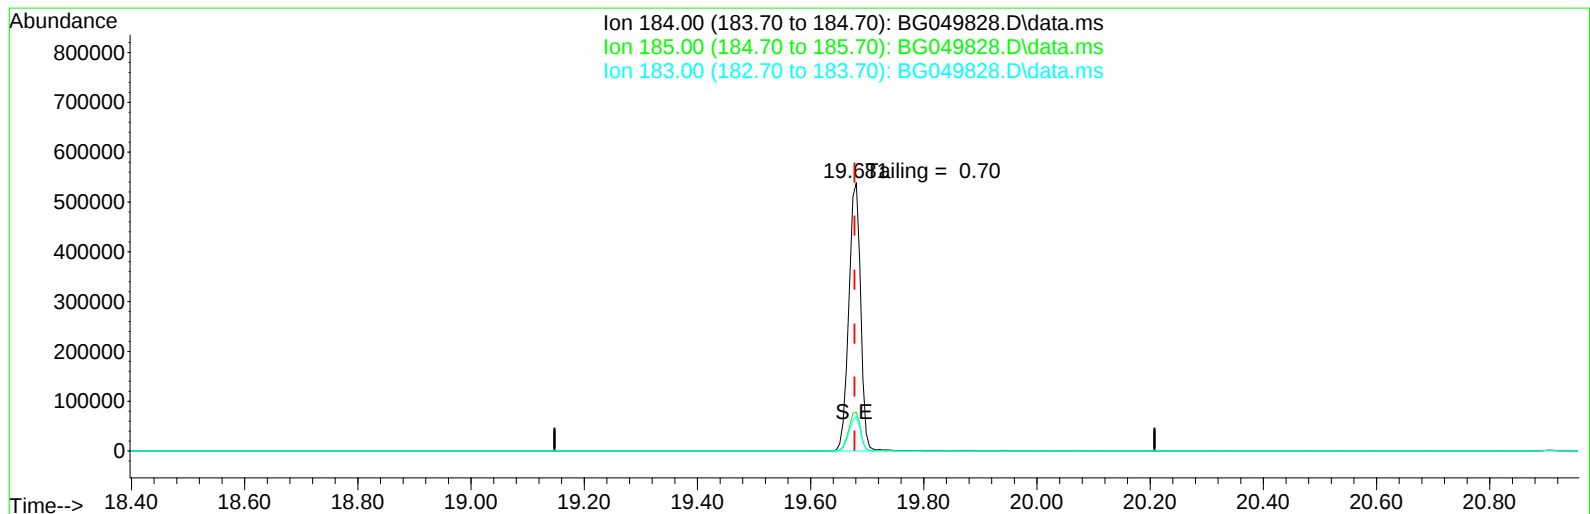

TIC: BG049828.D\data.ms

(77) Benzidine

19.681min (+ 0.003) 525703.44 ng

response 781239

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.40  | 14.53  |
| 183.00 | 11.70  | 12.81  |
| 0.00   | 0.00   | 0.00   |