


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081423\
Data File : BG058713.D
Acq On : 14 Aug 2023 8:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 28 22:29:07 2023

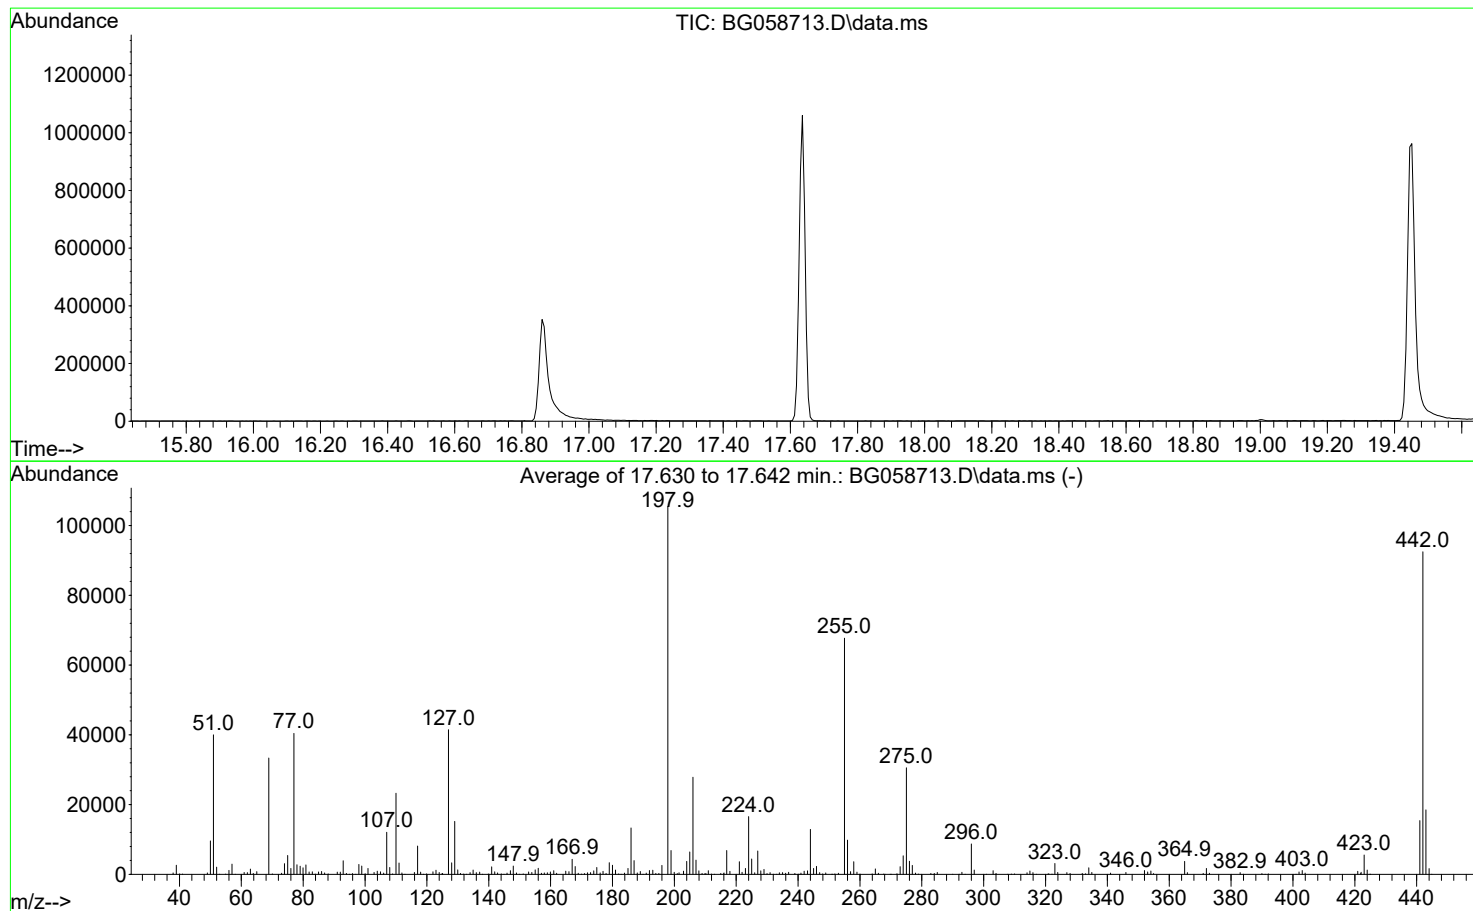




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	39997	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.6	33341	PASS
70	69	0.00	2	0.4	127	PASS
127	198	10	80	39.3	41483	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	105475	PASS
199	198	5	9	6.5	6825	PASS
275	198	10	60	29.0	30552	PASS
365	198	1	100	3.5	3739	PASS
441	198	0.01	100	14.6	15432	PASS
442	442	50	100	100.0	92496	PASS
443	442	15	24	20.0	18481	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081423\
Data File : BG058713.D
Acq On : 14 Aug 2023 8:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 14 11:35:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

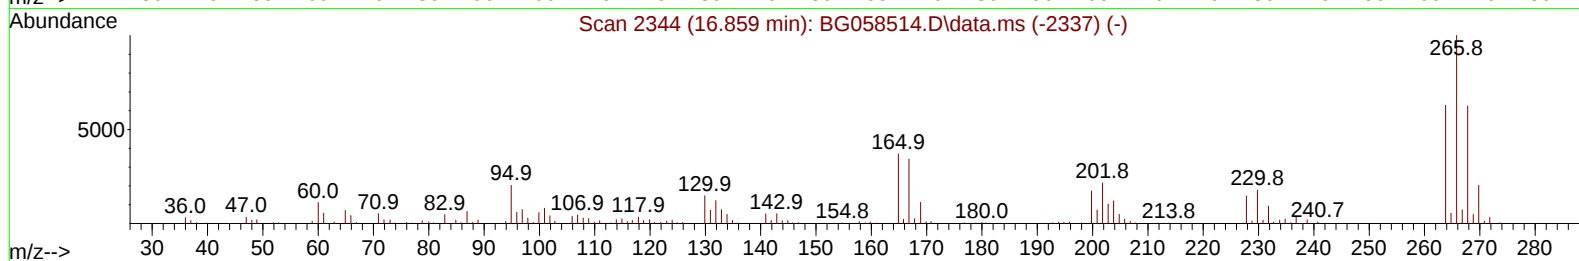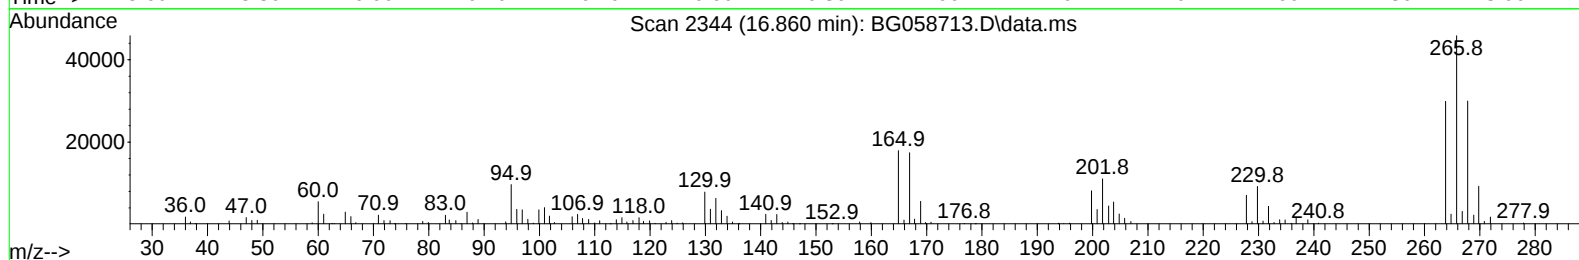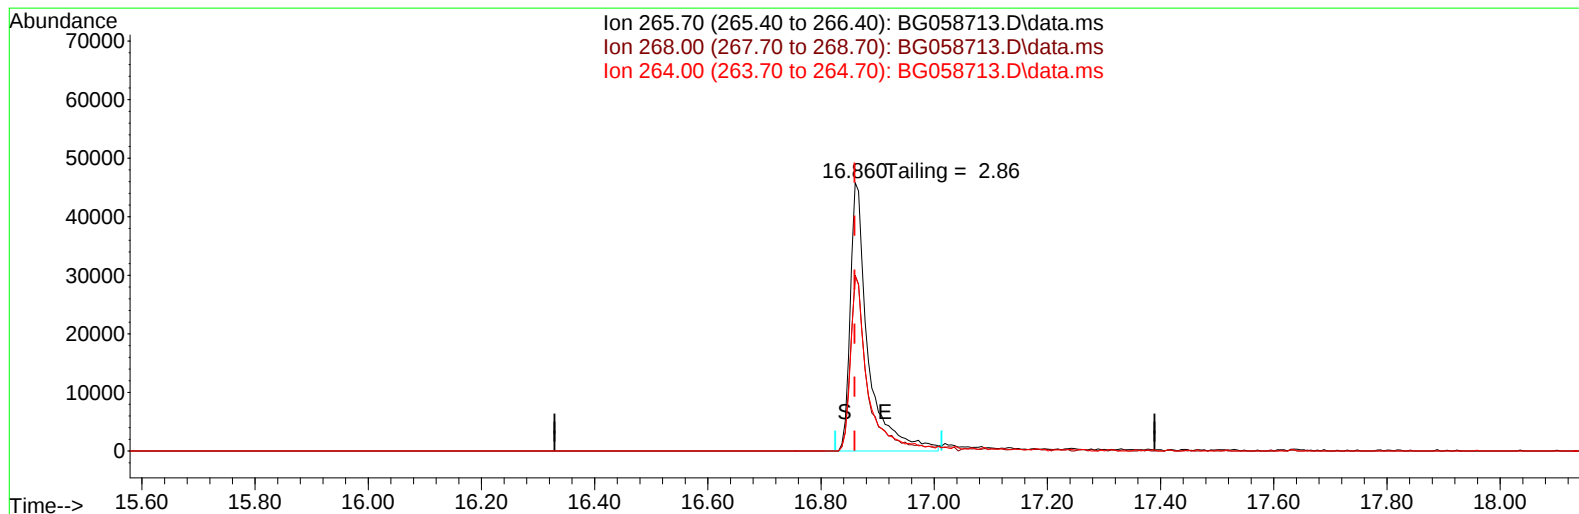

TIC: BG058713.D\data.ms

(70) Pentachlorophenol (C)

16.860min (+ 0.001) 22593.62 ng




response 100918

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	65.40
264.00	62.80	65.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081423\
Data File : BG058713.D
Acq On : 14 Aug 2023 8:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 14 11:35:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

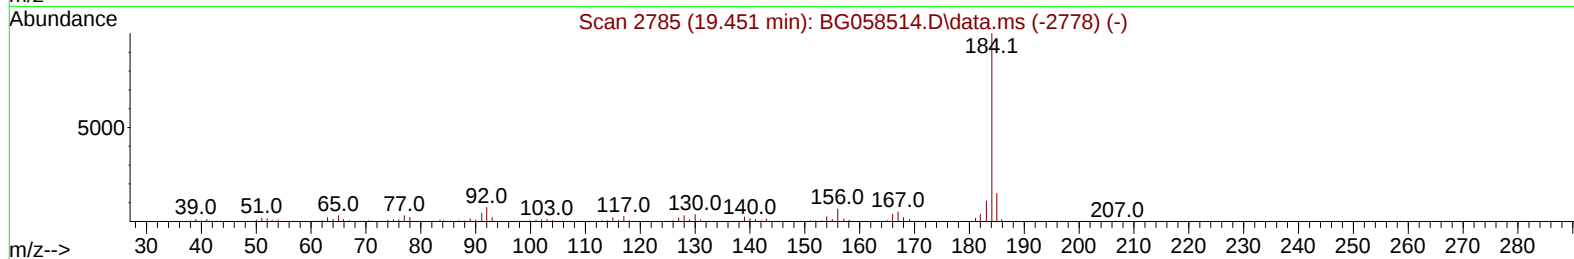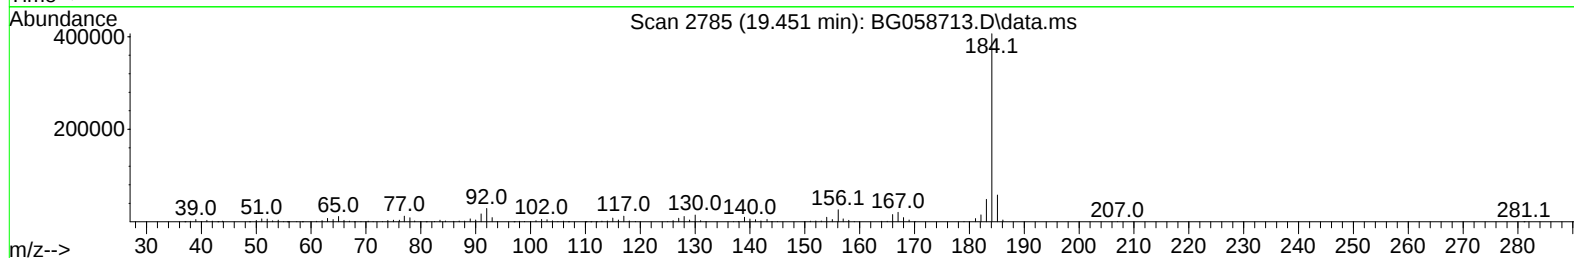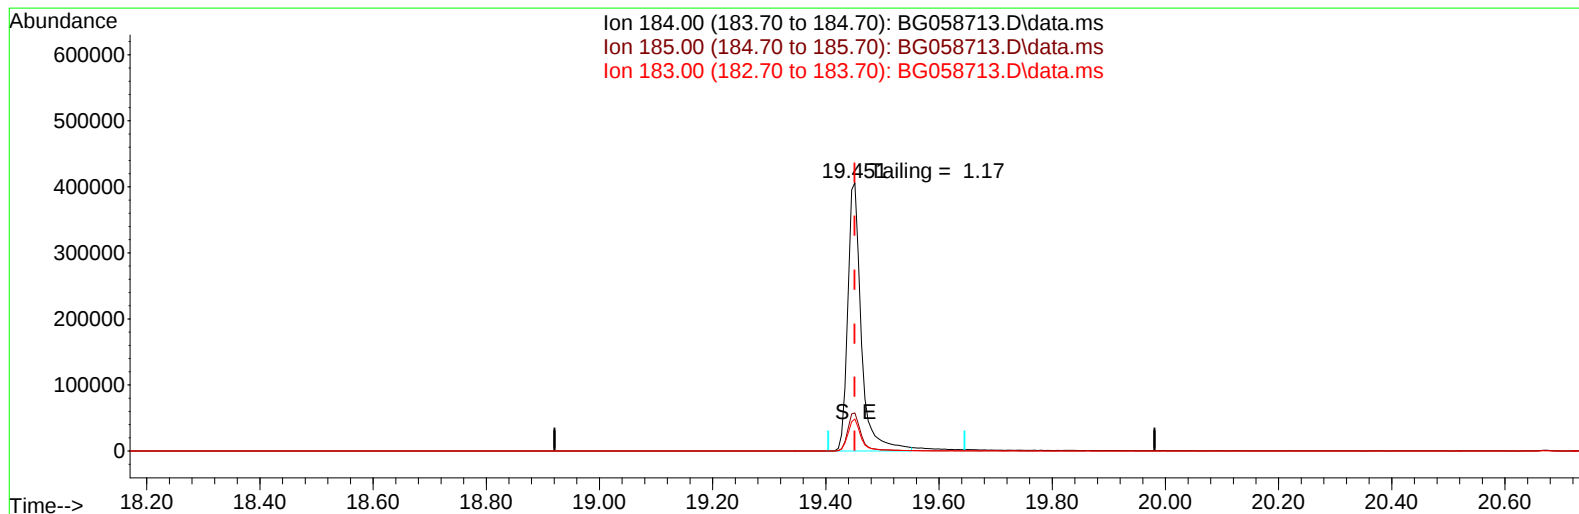

TIC: BG058713.D\data.ms

(77) Benzidine

19.451min (+ 0.001) 0.00 ng

response 695805

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.23
183.00	10.90	11.96
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/14/2023	BNA_G	BG058713.D
Compound Name	Response	Retention Time
DDT	339569	20.673
DDD	9069	20.239
DDE	1874	19.728
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10943	350512	3.12

Instrument :
BNA_G
ClientSampleId :
DFTPP