

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081519\
 Data File : BG042239.D
 Acq On : 15 Aug 2019 21:29
 Operator : HP/JU
 Sample : K4183-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AF3

Quant Time: Aug 16 16:12:12 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 14 10:42:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.02	152	71213	20.00	ng/ul	0.00
18) Naphthalene-d8	10.85	136	290249	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.69	164	195792	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.44	188	406969	20.00	ng/ul	0.00
77) Chrysene-d12	21.72	240	393146	20.00	ng/ul	0.00
85) Perylene-d12	24.99	264	458347	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.41	96	4136	2.54	ng/uL	0.00
5) Phenol-d5	7.18	99	91744	16.42	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.34	67	46218	14.79	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	85007	17.79	ng/ul	0.00
13) 4-Methylphenol-d8	8.74	113	78216	16.67	ng/ul	0.00
19) Nitrobenzene-d5	9.19	128	40995	18.76	ng/ul	0.00
22) 2-Nitrophenol-d4	9.92	143	49895	19.67	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.47	165	90522	17.68	ng/ul	0.00
29) 4-Chloroaniline-d4	10.98	131	101026	17.78	ng/ul	0.00
43) Dimethylphthalate-d6	14.08	166	270075	17.79	ng/ul	0.00
46) Acenaphthylene-d8	14.38	160	322813	18.61	ng/ul	0.00
51) 4-Nitrophenol-d4	14.89	143	30372	11.91	ng/ul	0.00
57) Fluorene-d10	15.68	176	238860	17.68	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.80	200	17929	6.87	ng/ul	0.00
70) Anthracene-d10	17.54	188	362986	18.59	ng/ul	0.00
78) Pyrene-d10	19.82	212	401489	18.30	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.77	264	437407	18.27	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.13	163	59838	3.969	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081519\
Data File : BG042239.D
Acq On : 15 Aug 2019 21:29
Operator : HP/JU
Sample : K4183-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF3

Quant Time: Aug 16 16:12:12 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 14 10:42:59 2019
Response via : Initial Calibration

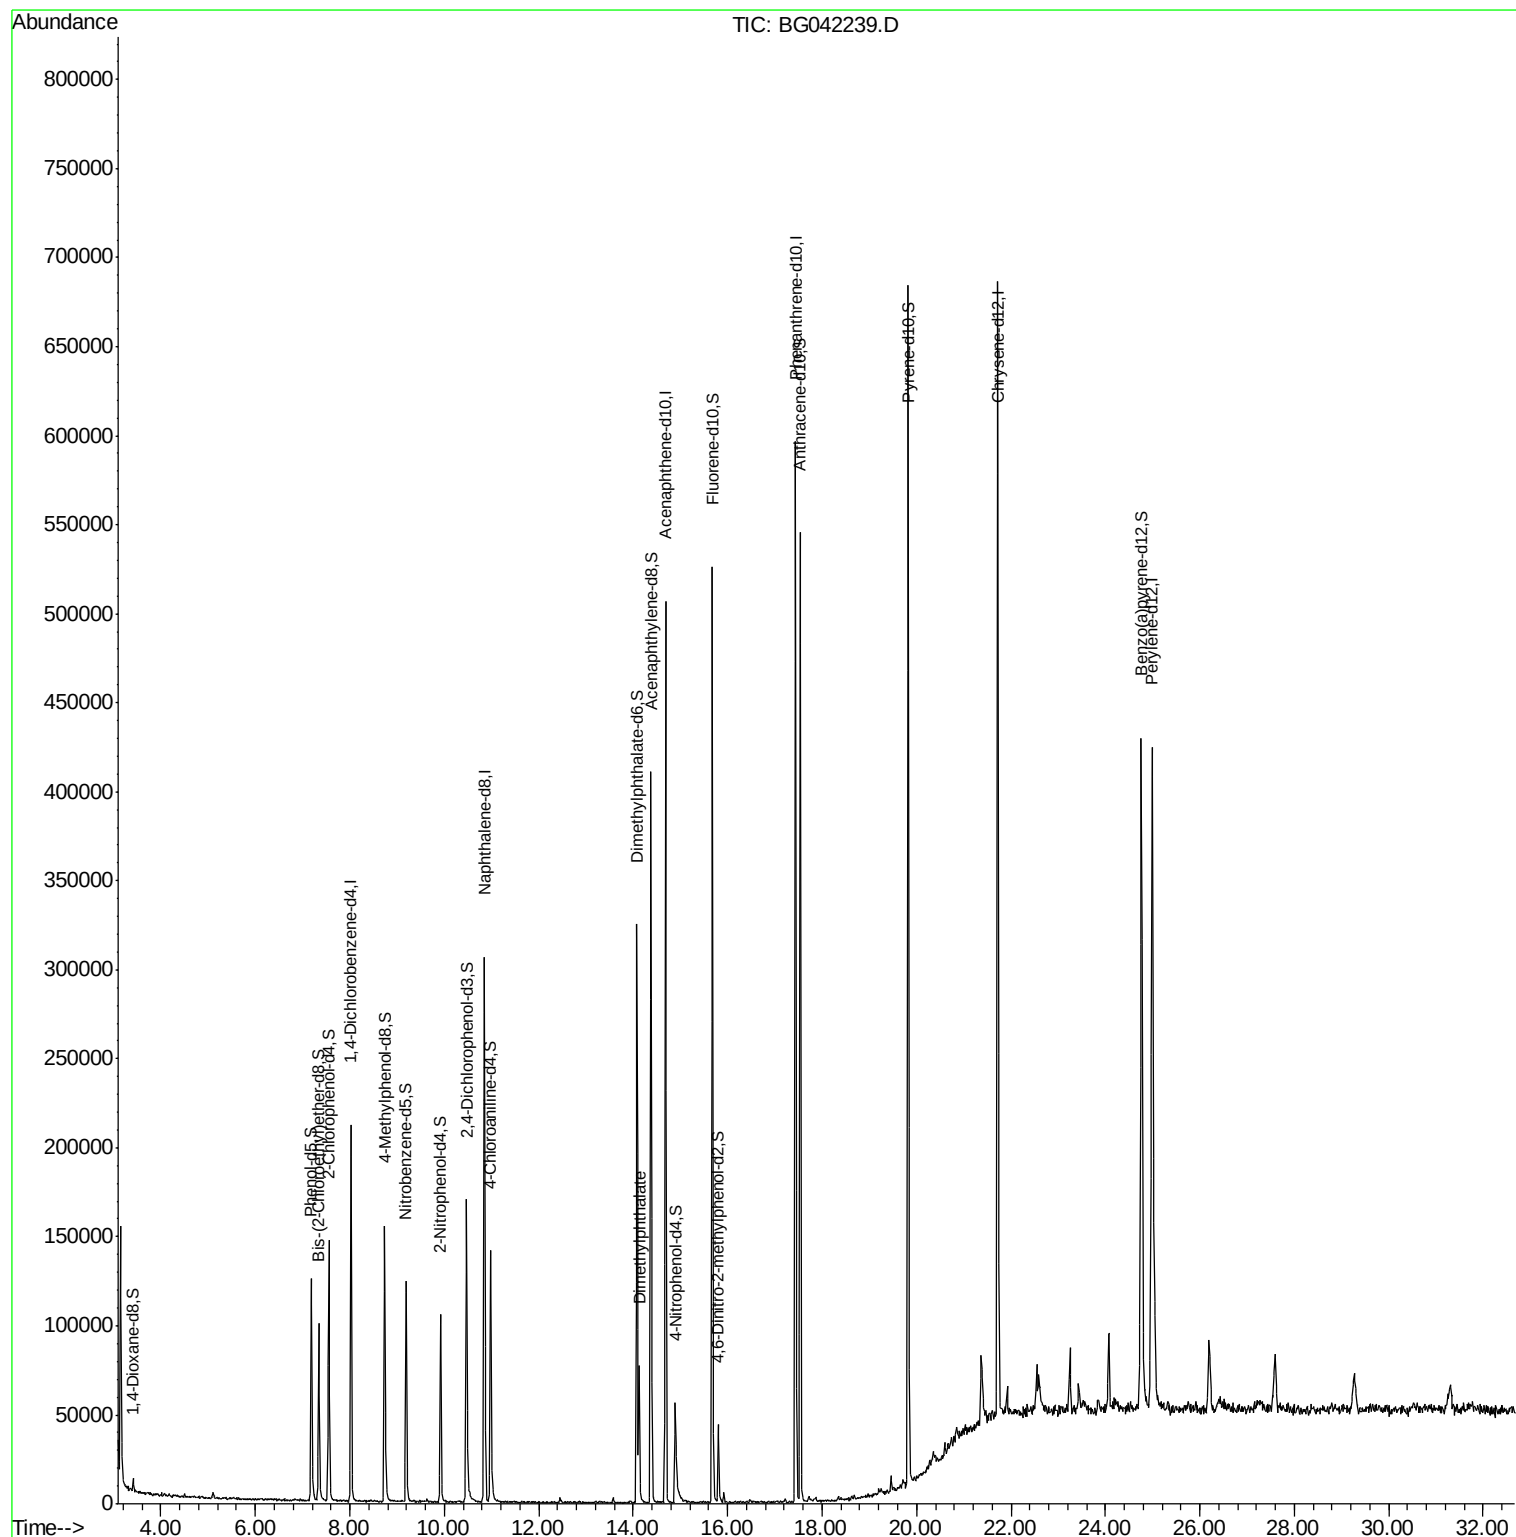

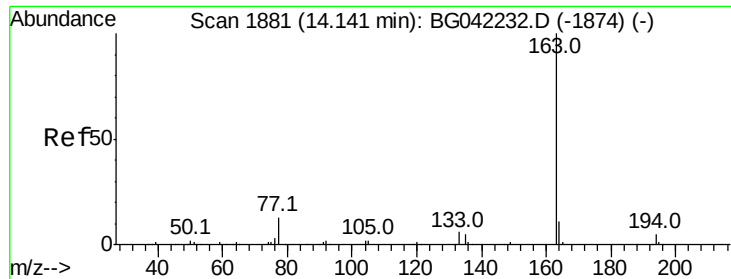

#44

Dimethylphthalate

Concen: 3.969 ng/ul

RT: 14.13 min Scan# 1879

Delta R.T. -0.00 min

Lab File: BG042239.D

Acq: 15 Aug 2019 21:29

Instrument :

BNA_G

ClientSampleId :

C0AF3

Tot Ion:163 Resp: 59838

Ion Ratio Lower Upper

163 100

194 4.9 4.2 6.2

164 10.2 7.8 11.8

