
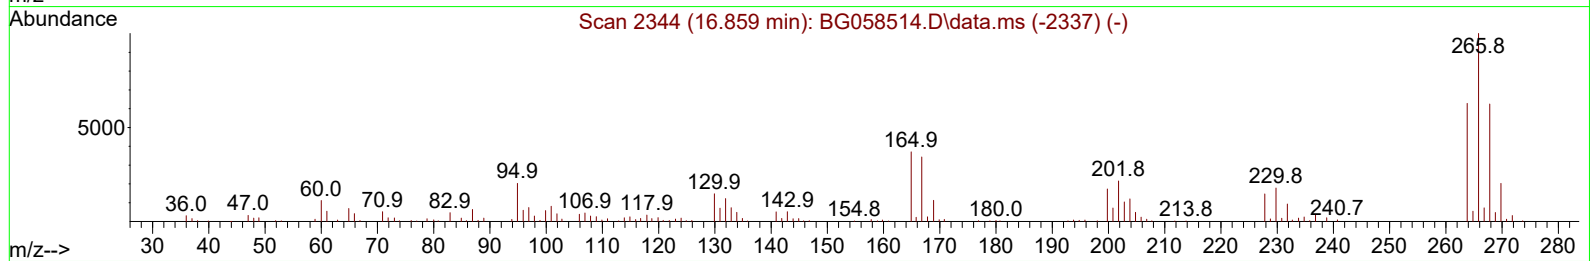
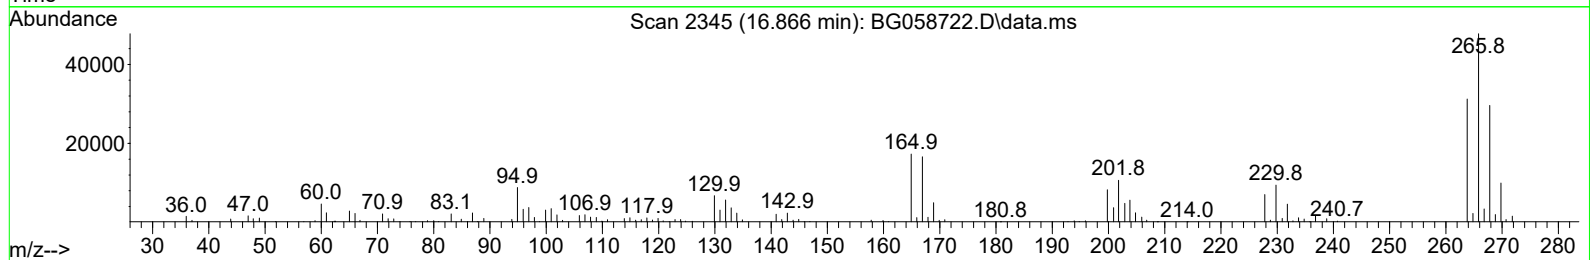


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081523\
Data File : BG058722.D
Acq On : 15 Aug 2023 7:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 15 18:45:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

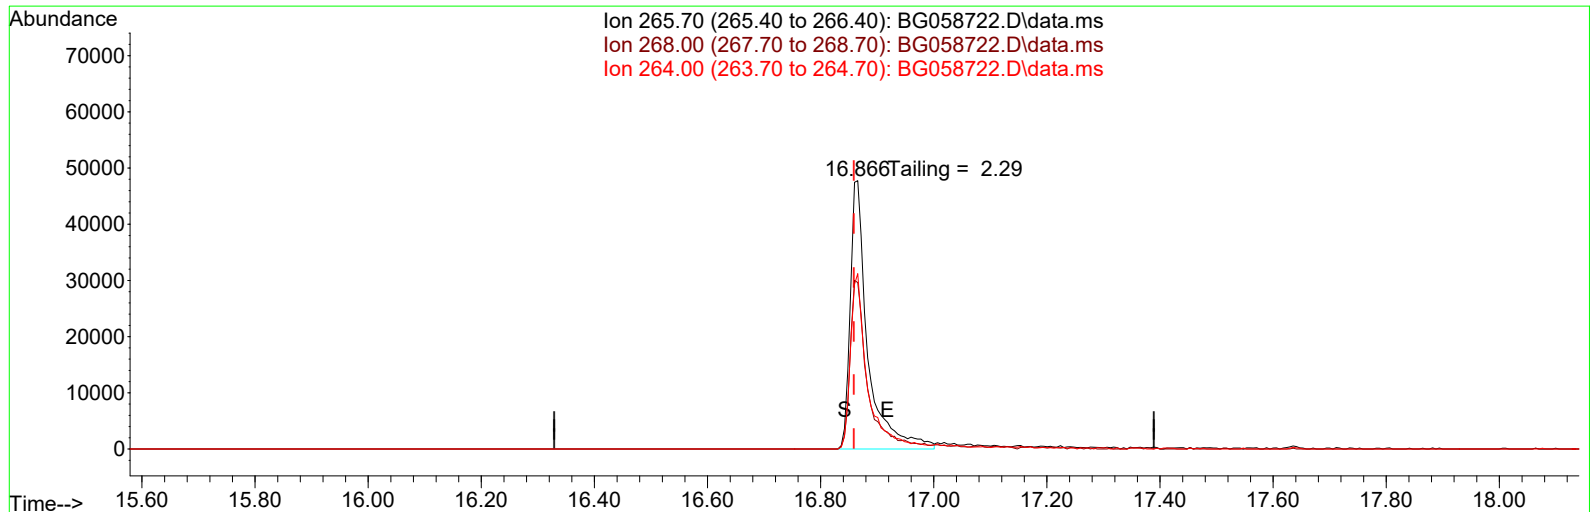

TIC: BG058722.D\data.ms

(70) Pentachlorophenol (C)




16.866min (+ 0.007) 23096.44 ng

response 103836

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	62.03
264.00	62.80	65.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081523\
Data File : BG058722.D
Acq On : 15 Aug 2023 7:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 15 18:45:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

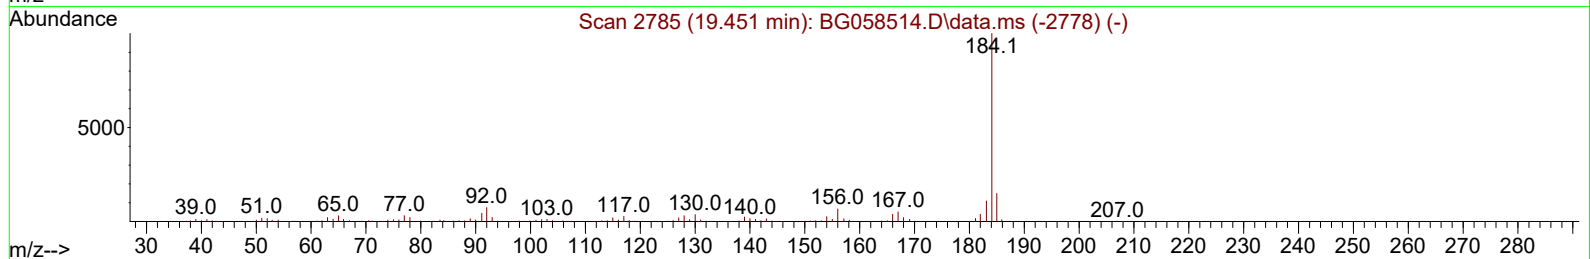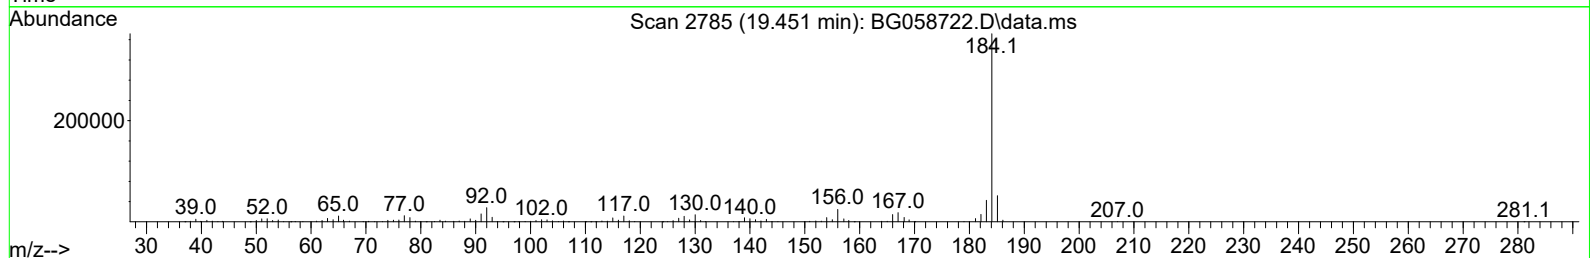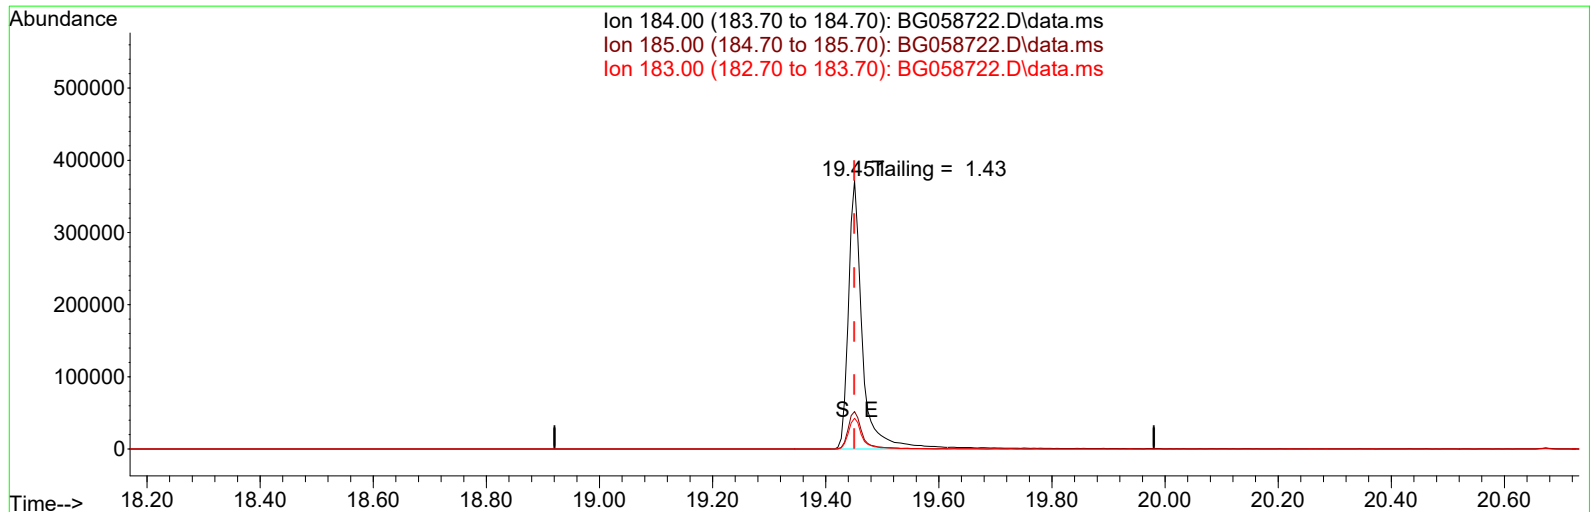

TIC: BG058722.D\data.ms

(77) Benzidine**19.451min (+ 0.000) 180280.37 ng****response 634237**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.95
183.00	10.90	11.44
0.00	0.00	0.00