

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081523\
 Data File : BG058732.D
 Acq On : 15 Aug 2023 14:59
 Operator : MA/JU
 Sample : 04016-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 B-PP15A

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG058732.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	384	391	405	rVB	427564	685274	44.44%	7.707%
2	6.983	655	663	675	rBV	428780	752097	48.77%	8.458%
3	7.811	796	804	812	rBV	152082	258743	16.78%	2.910%
4	8.974	993	1002	1022	rBV	242255	453529	29.41%	5.101%
5	10.608	1272	1280	1296	rBV	207910	397821	25.80%	4.474%
6	13.076	1693	1700	1721	rBV	676013	1056809	68.53%	11.885%
7	14.456	1927	1935	1950	rBV	355478	564871	36.63%	6.353%
8	15.949	2183	2189	2213	rBV	495877	843930	54.72%	9.491%
9	17.206	2396	2403	2415	rBV	417012	677446	43.93%	7.619%
10	18.093	2550	2554	2563	rBV3	17418	34645	2.25%	0.390%
11	19.821	2842	2848	2861	rBV	1188047	1542139	100.00%	17.344%
12	20.614	2978	2983	2987	rBV	13566	16228	1.05%	0.183%
13	21.101	3061	3066	3069	rBV	26001	39695	2.57%	0.446%
14	21.448	3118	3125	3141	rVB2	411560	697920	45.26%	7.849%
15	21.618	3149	3154	3163	rVB4	12765	22687	1.47%	0.255%
16	22.194	3247	3252	3257	rBV2	11325	17570	1.14%	0.198%
17	22.846	3357	3363	3373	rVB5	12350	27816	1.80%	0.313%
18	23.023	3387	3393	3399	rBV3	9976	19412	1.26%	0.218%
19	23.599	3487	3491	3498	rVB4	10325	21274	1.38%	0.239%
20	24.521	3636	3648	3662	rBV	242474	761723	49.39%	8.567%




Sum of corrected areas: 8891629

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081523\
Data File : BG058732.D
Acq On : 15 Aug 2023 14:59
Operator : MA/JU
Sample : 04016-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
B-PP15A

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

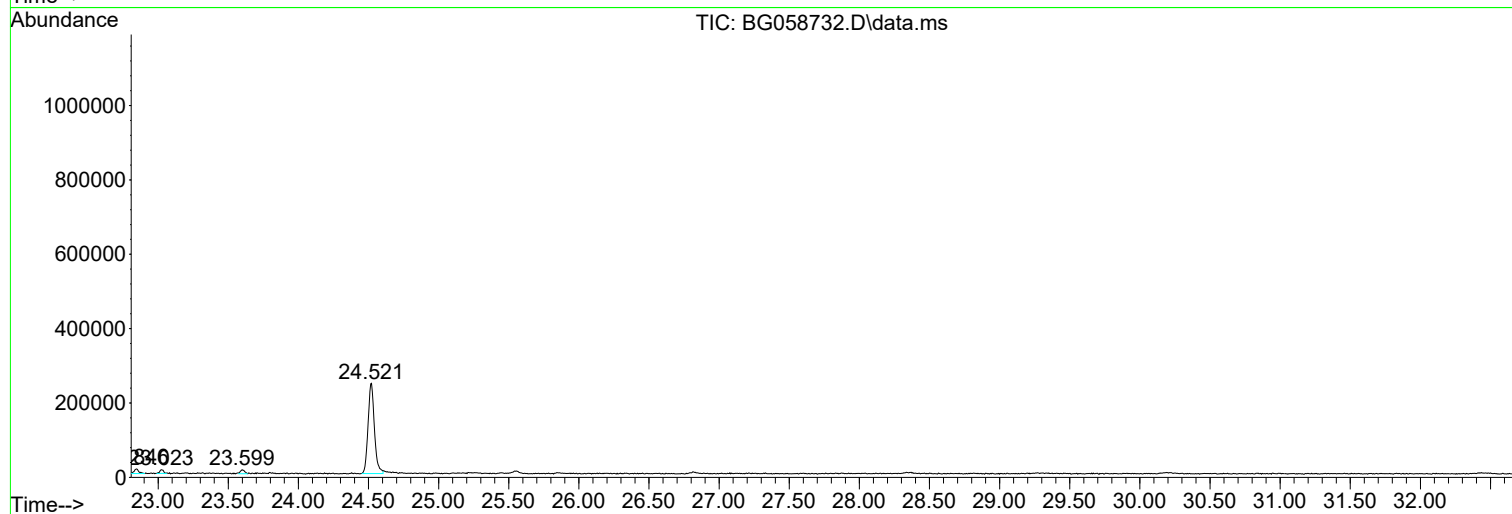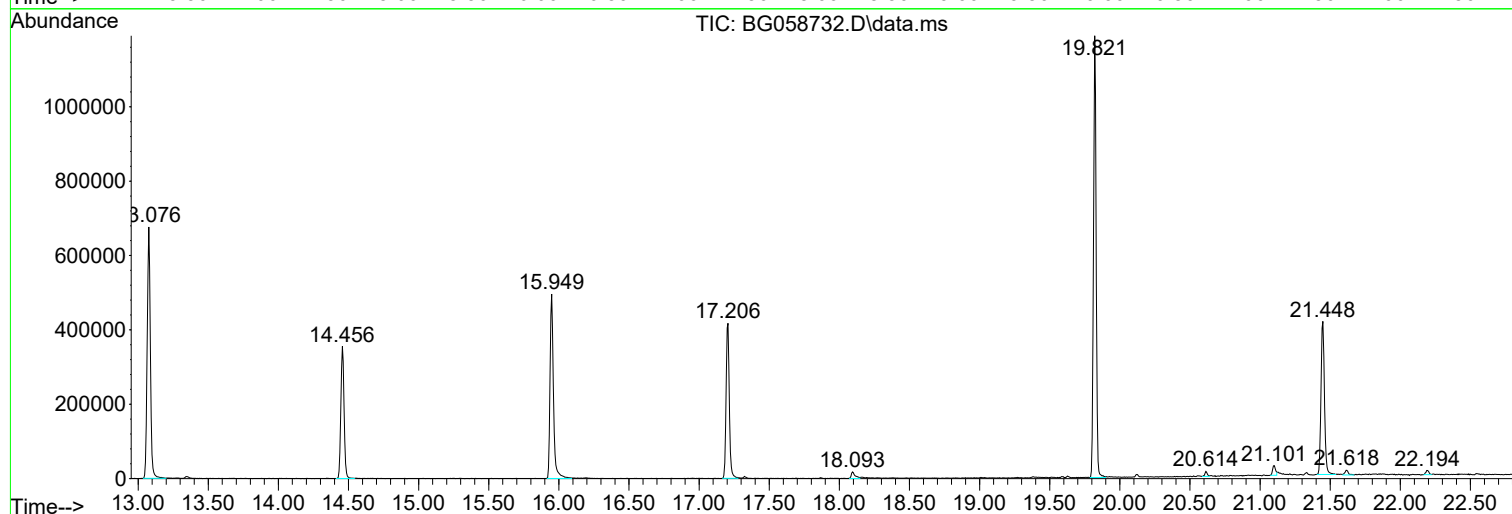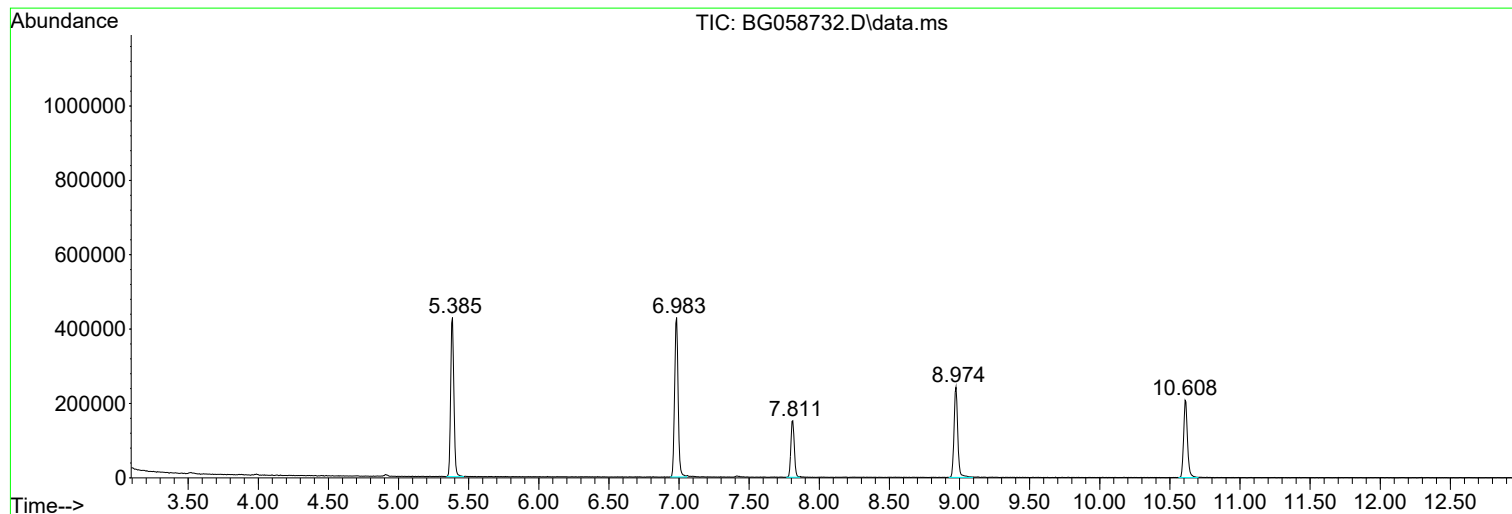

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081523\
Data File : BG058732.D
Acq On : 15 Aug 2023 14:59
Operator : MA/JU
Sample : 04016-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
B-PP15A

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081523\
Data File : BG058732.D
Acq On : 15 Aug 2023 14:59
Operator : MA/JU
Sample : 04016-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
B-PP15A

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------