


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081523\
Data File : BG058722.D
Acq On : 15 Aug 2023 7:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 28 22:29:07 2023

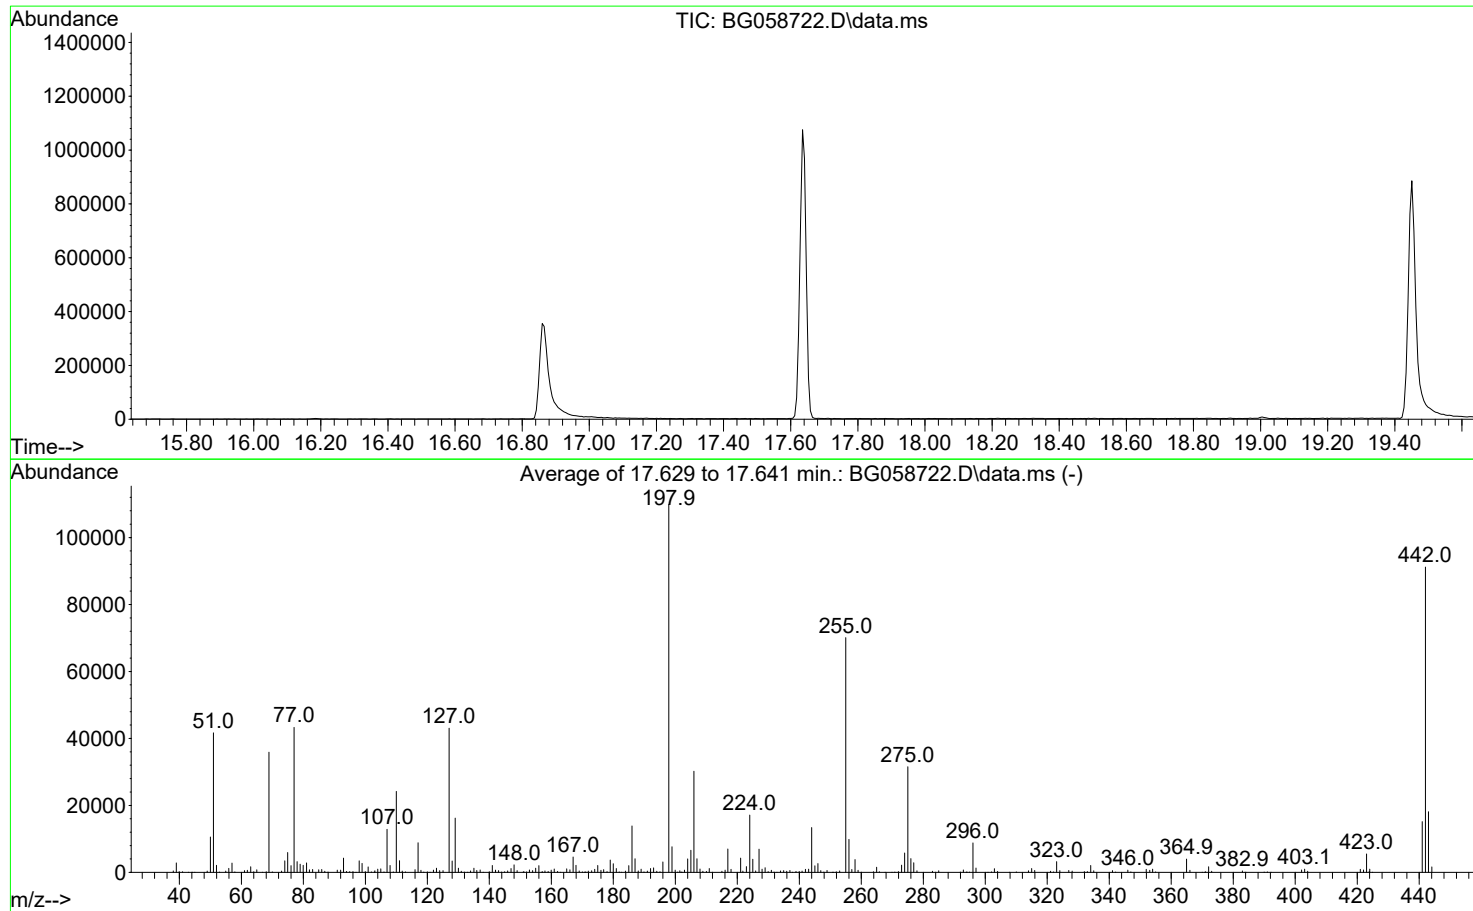




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	41685	PASS
68	69	0.00	2	0.6	217	PASS
69	198	0.00	100	32.7	35881	PASS
70	69	0.00	2	0.4	156	PASS
127	198	10	80	39.2	43043	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	109872	PASS
199	198	5	9	7.0	7661	PASS
275	198	10	60	28.7	31555	PASS
365	198	1	100	3.6	3988	PASS
441	198	0.01	100	13.8	15151	PASS
442	442	50	100	100.0	91192	PASS
443	442	15	24	19.9	18133	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081523\
Data File : BG058722.D
Acq On : 15 Aug 2023 7:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 15 18:45:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

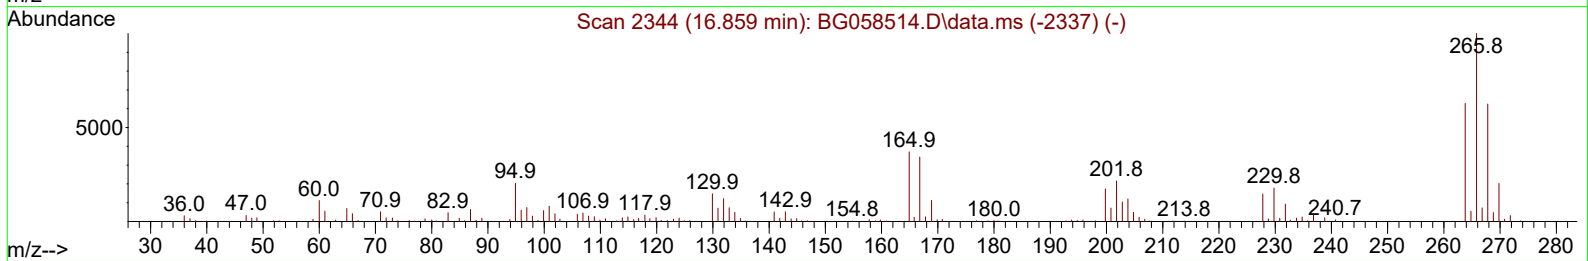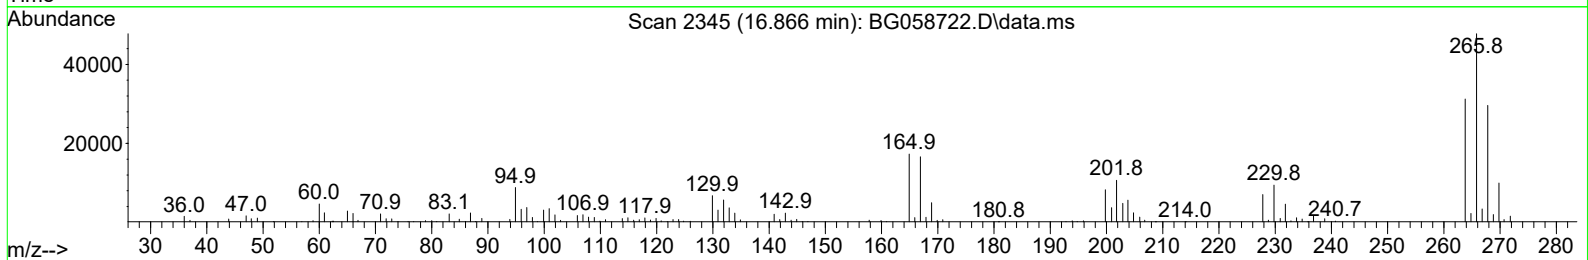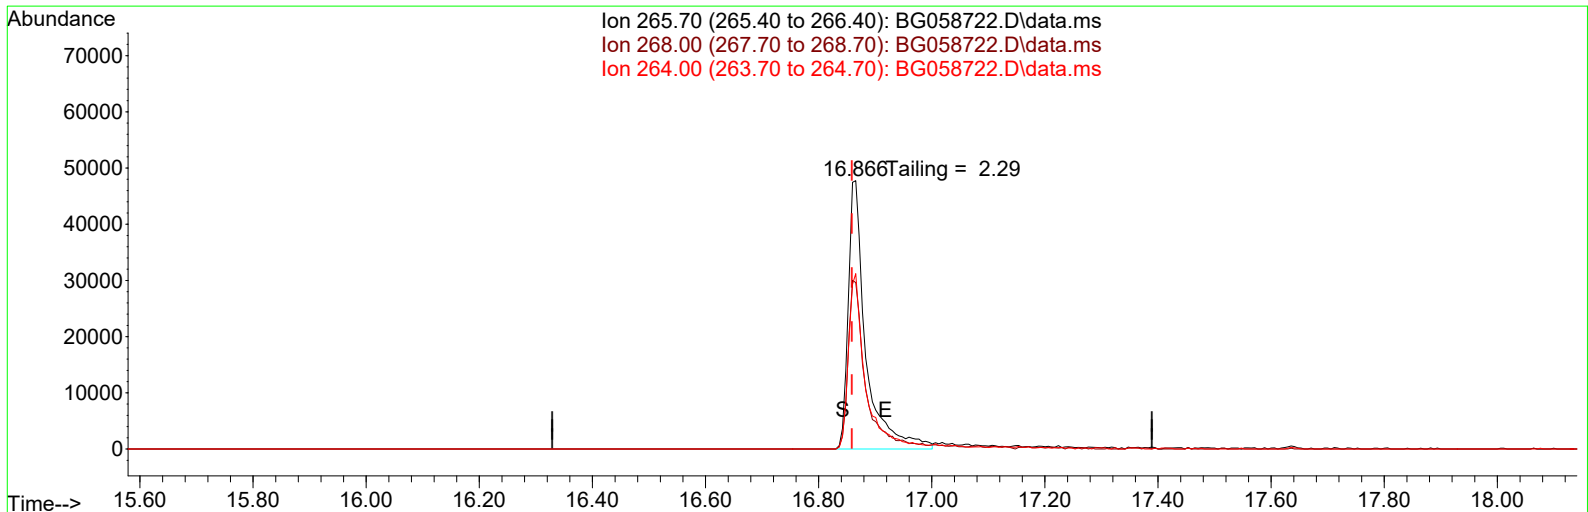

TIC: BG058722.D\data.ms

(70) Pentachlorophenol (C)

16.866min (+ 0.007) 23096.44 ng




response 103836

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	62.03
264.00	62.80	65.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081523\
Data File : BG058722.D
Acq On : 15 Aug 2023 7:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 15 18:45:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

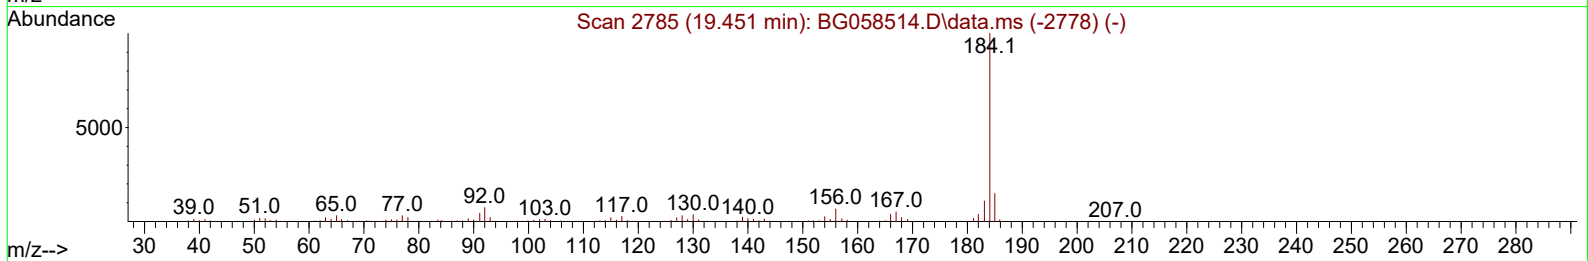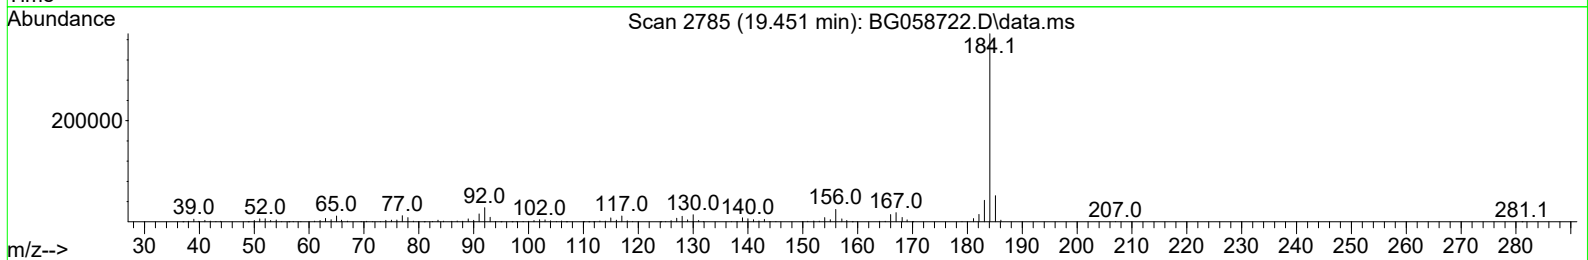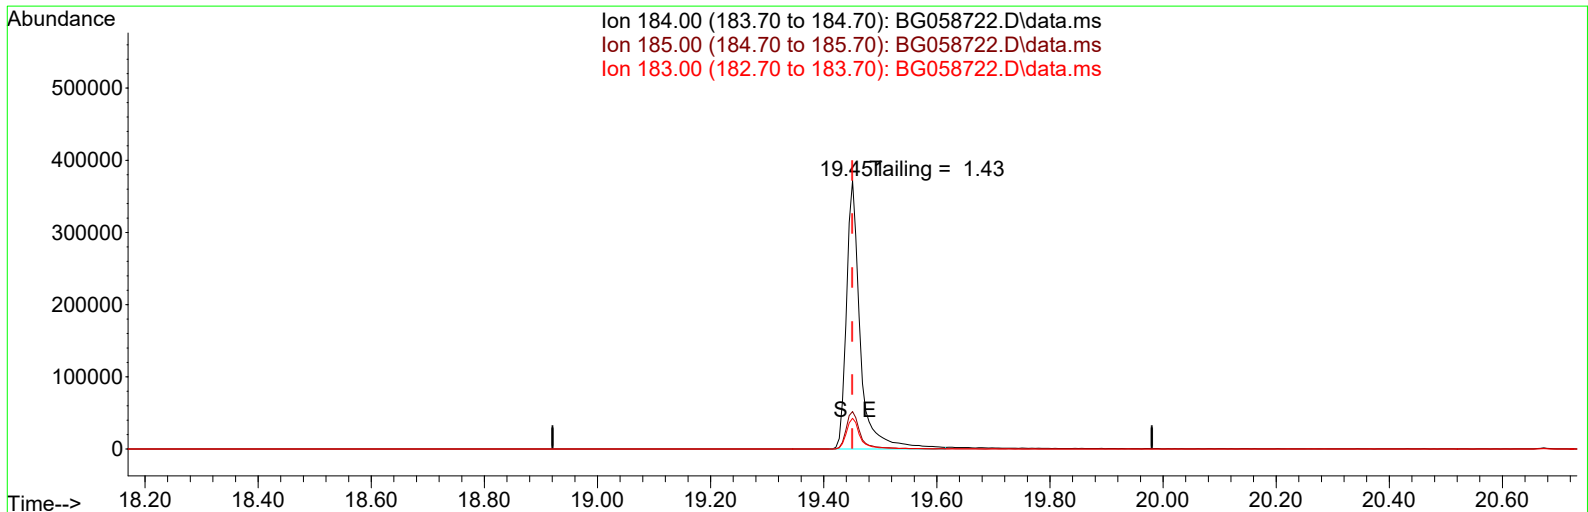

TIC: BG058722.D\data.ms

(77) Benzidine

19.451min (+ 0.000) 180280.37 ng

response 634237

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.95
183.00	10.90	11.44
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/15/2023	BNA_G	BG058722.D
Compound Name	Response	Retention Time
DDT	359279	20.673
DDD	13070	20.238
DDE	1426	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14496	373775	3.88

Instrument :
BNA_G
ClientSampleId :
DFTPP