
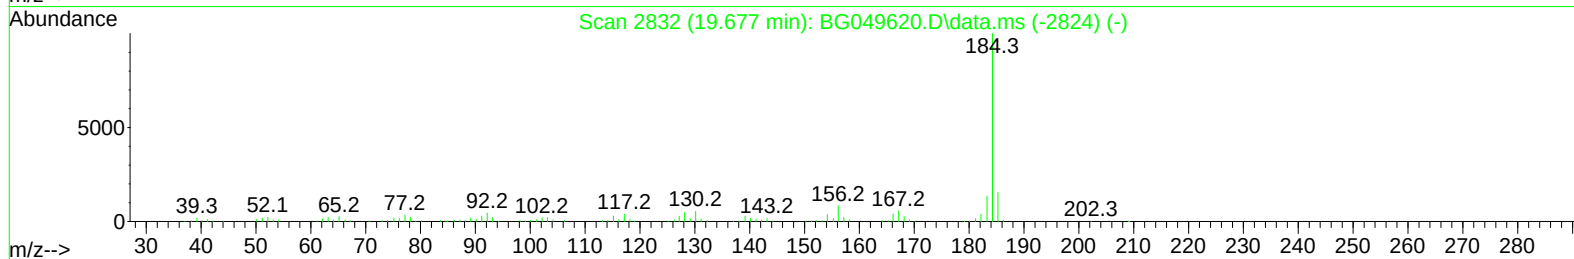
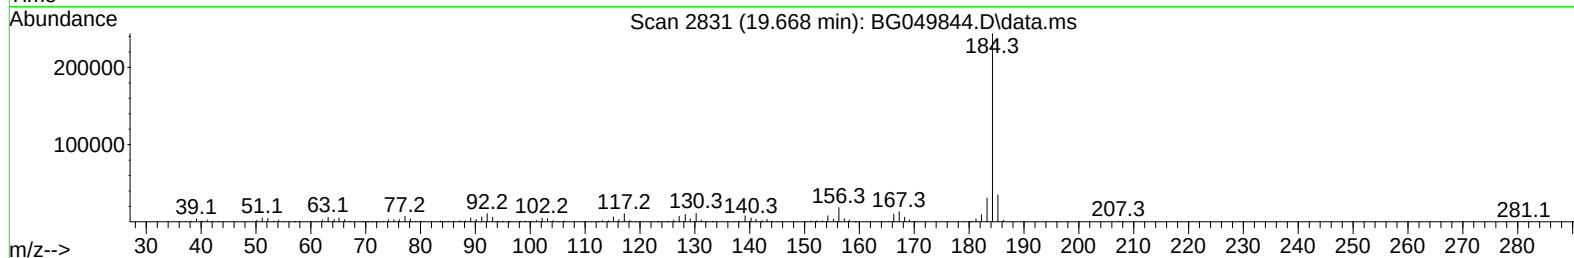


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081621\
Data File : BG049844.D
Acq On : 16 Aug 2021 9:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 13:00:03 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 15:15:33 2021
Response via : Initial Calibration

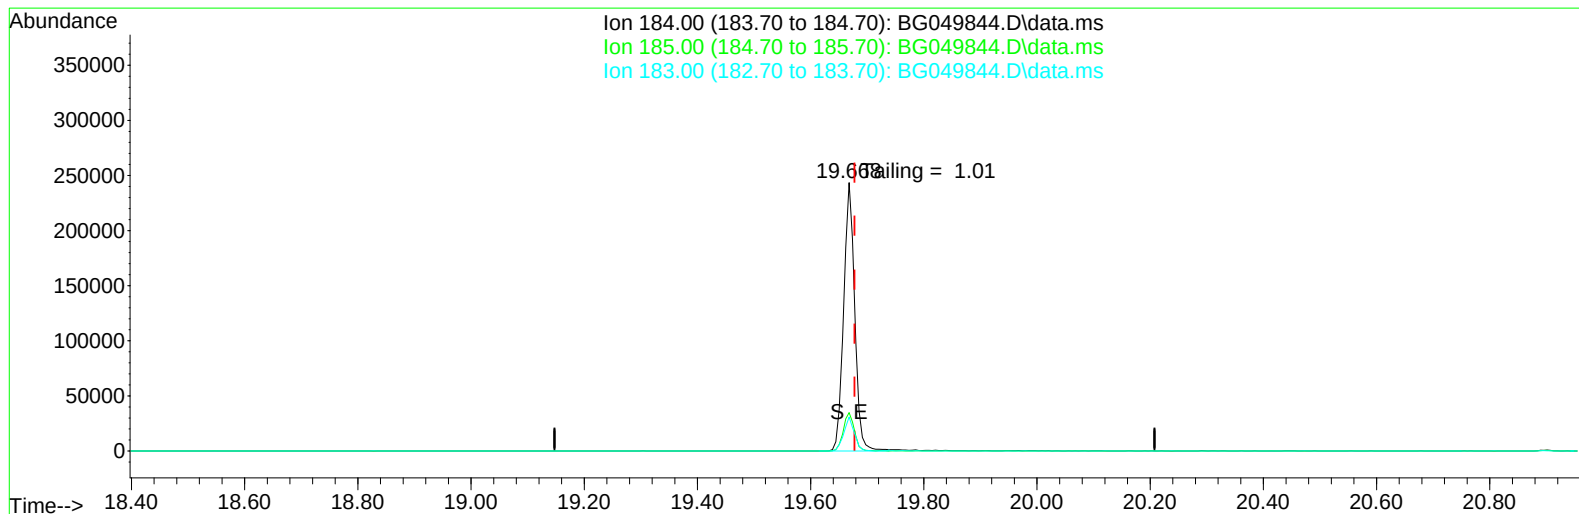




TIC: BG049844.D\data.ms

(77) Benzidine**19.668min (-0.009) 240369.54 ng****response 332574**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.31
183.00	11.70	12.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081621\
Data File : BG049844.D
Acq On : 16 Aug 2021 9:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 13:00:03 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 15:15:33 2021
Response via : Initial Calibration

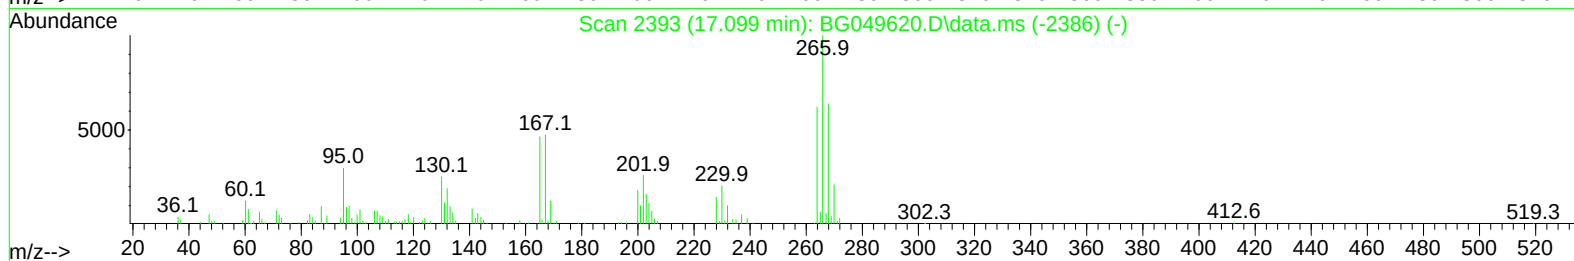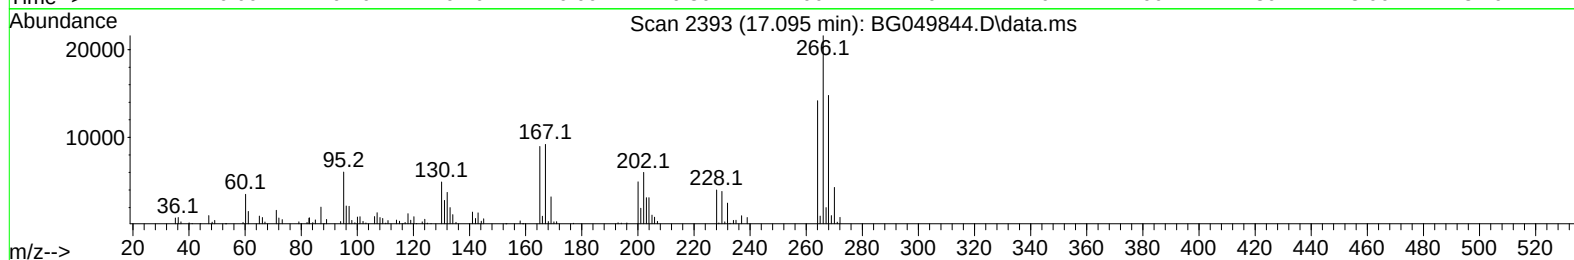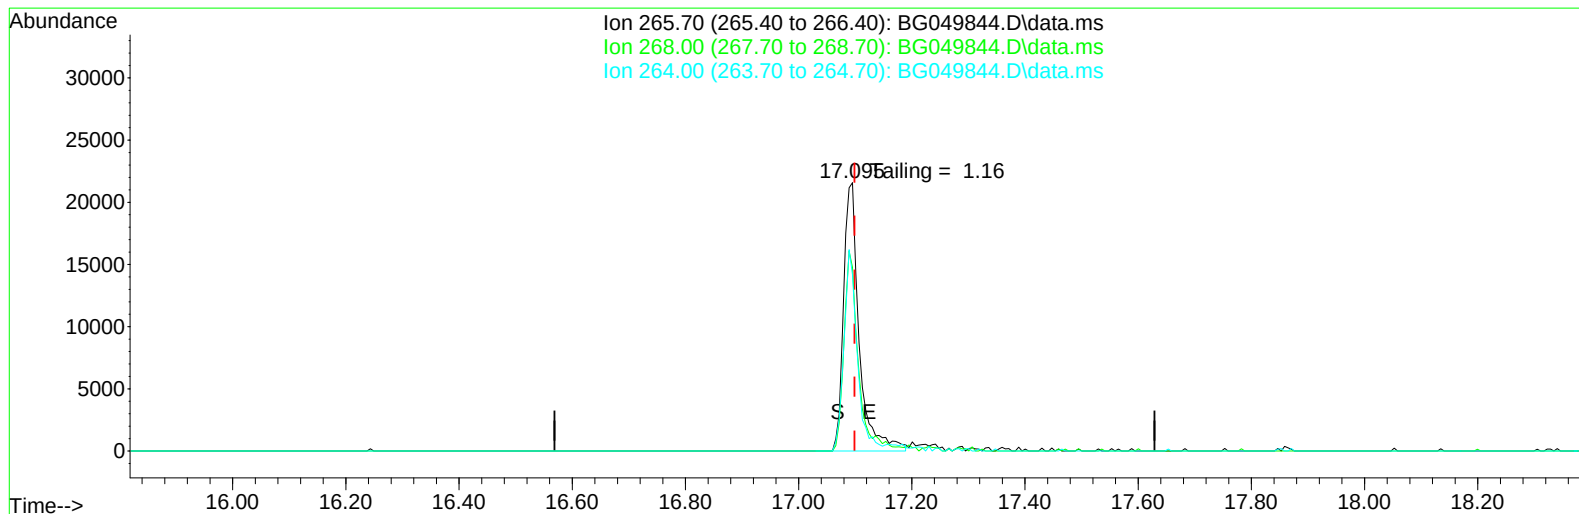

TIC: BG049844.D\data.ms

(70) Pentachlorophenol (C)

17.095min (-0.004) 18928.89 ng

response 41702

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	68.45
264.00	61.30	65.68
0.00	0.00	0.00