
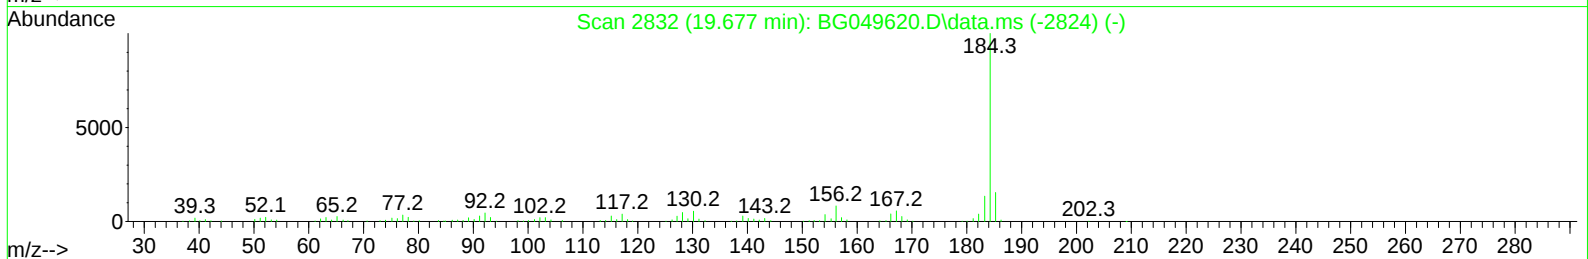
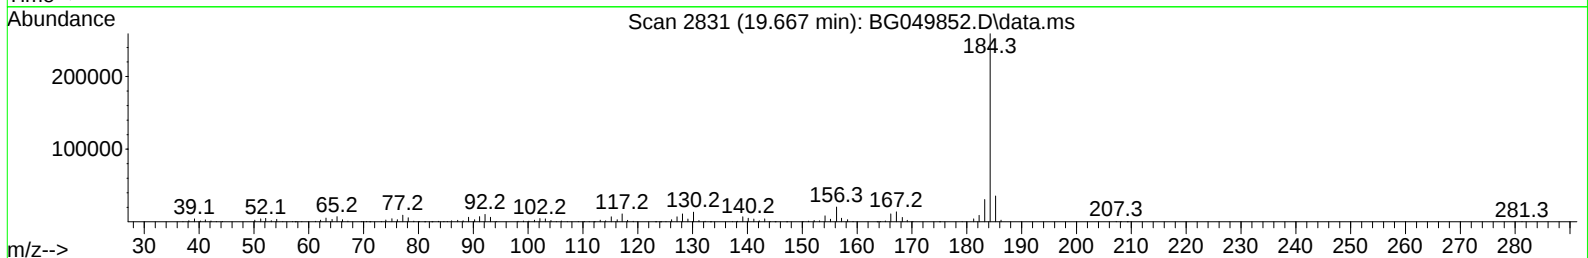


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081621\
Data File : BG049852.D
Acq On : 16 Aug 2021 16:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 17:08:15 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 15:15:33 2021
Response via : Initial Calibration

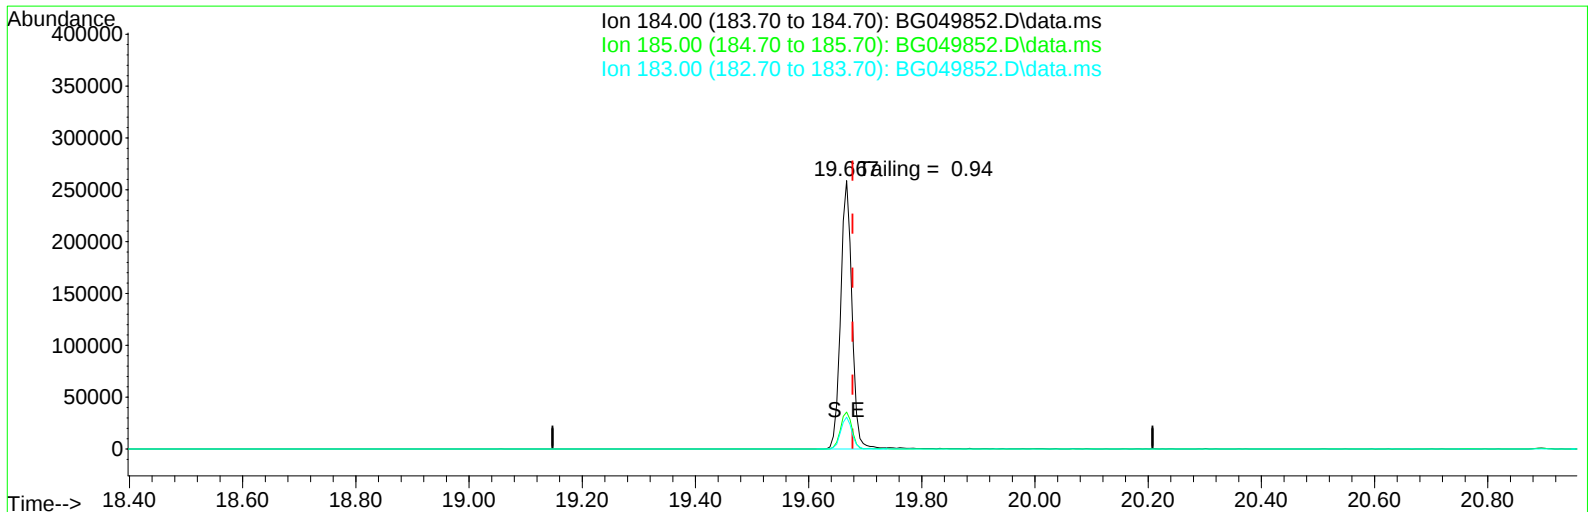

TIC: BG049852.D\data.ms

(77) Benzidine




19.667min (-0.010) 5342.17 ng m

response 357114

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.76
183.00	11.70	11.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081621\
Data File : BG049852.D
Acq On : 16 Aug 2021 16:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 17:08:15 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 15:15:33 2021
Response via : Initial Calibration

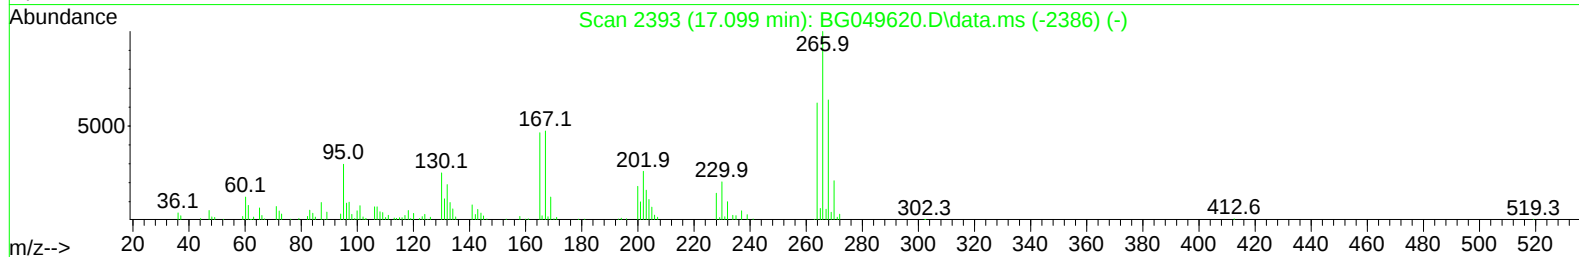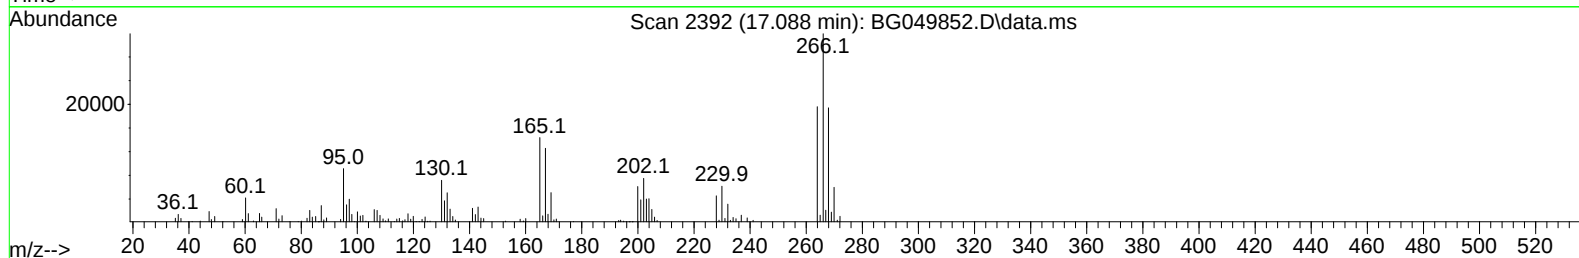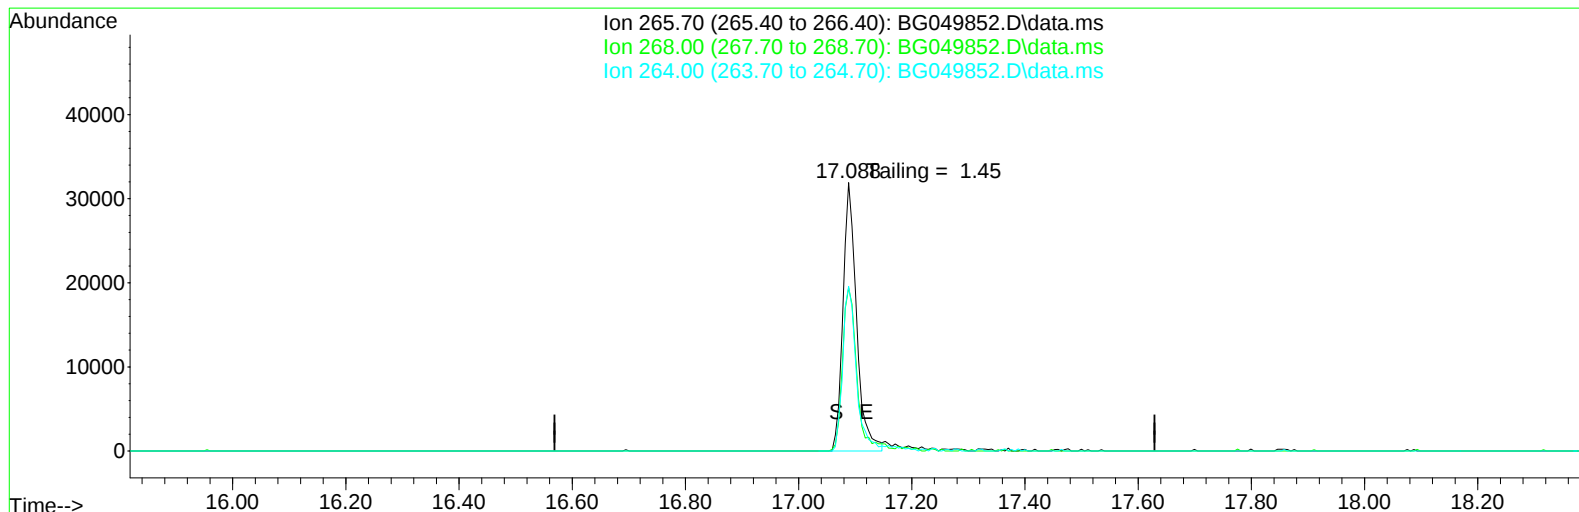

TIC: BG049852.D\data.ms

(70) Pentachlorophenol (C)

17.088min (-0.010) 123587.48 ng m

response 52894

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	60.79
264.00	61.30	61.34
0.00	0.00	0.00