


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081621\
 Data File : BG049844.D
 Acq On : 16 Aug 2021 9:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 16 18:23:02 2021

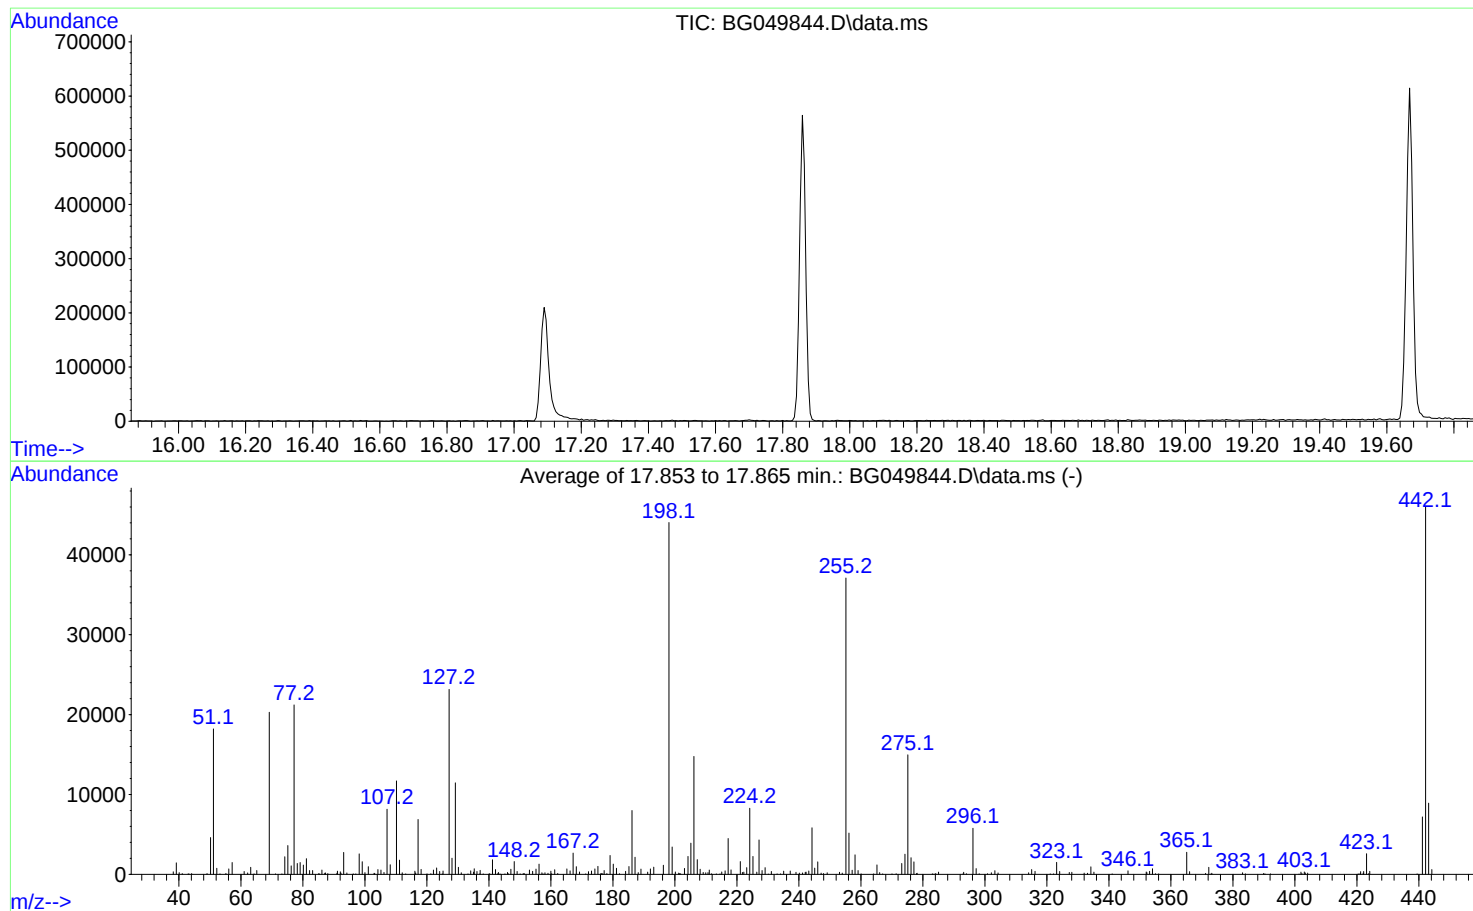




AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.3	18202	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.1	20301	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.6	23157	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	44045	PASS
199	198	5	9	7.8	3424	PASS
275	198	10	60	34.0	14973	PASS
365	198	1	100	6.3	2769	PASS
441	198	0.01	100	16.3	7197	PASS
442	442	100	100	100.0	46051	PASS
443	442	15	24	19.3	8909	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081621\
Data File : BG049844.D
Acq On : 16 Aug 2021 9:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 16 13:00:03 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 15:15:33 2021
Response via : Initial Calibration

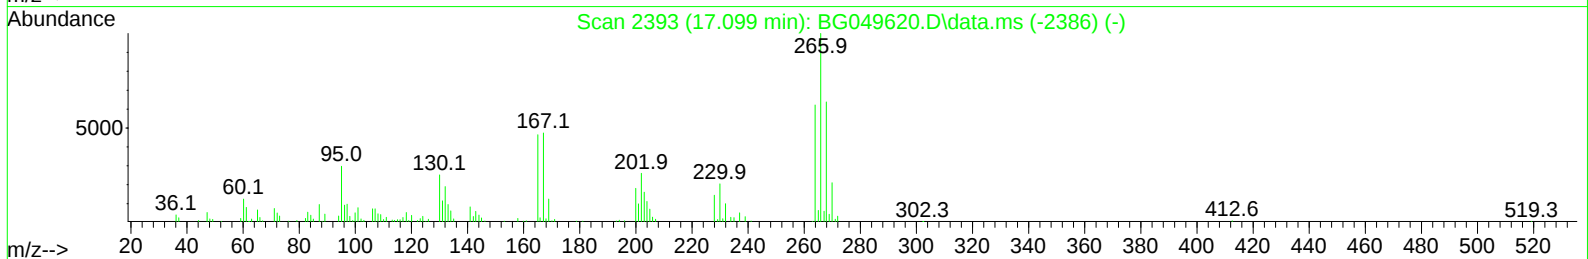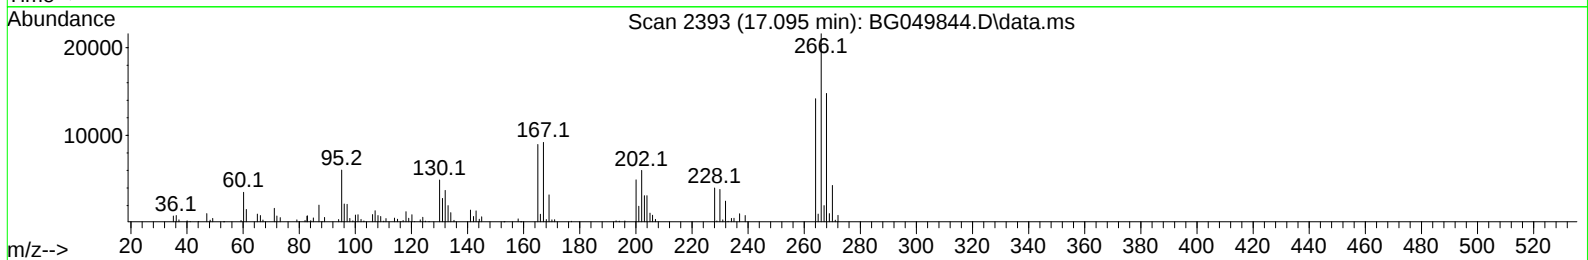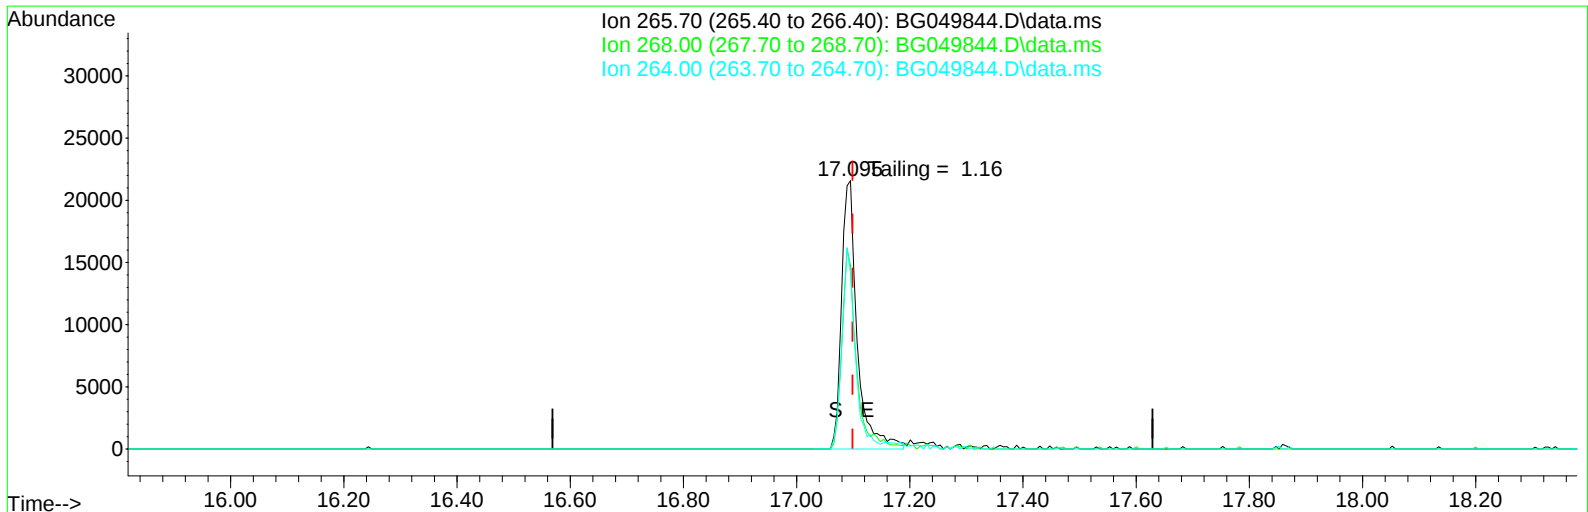

TIC: BG049844.D\data.ms

(70) Pentachlorophenol (C)

17.095min (-0.004) 18928.89 ng

response 41702

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	68.45
264.00	61.30	65.68
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/16/2021	BNA_G	BG049844.D
Compound Name	Response	Retention Time
DDT	166146	20.9
DDD	763	20.46
DDE	739	19.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1502	167648	0.90