


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081621\
 Data File : BG049852.D
 Acq On : 16 Aug 2021 16:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 16 18:23:02 2021

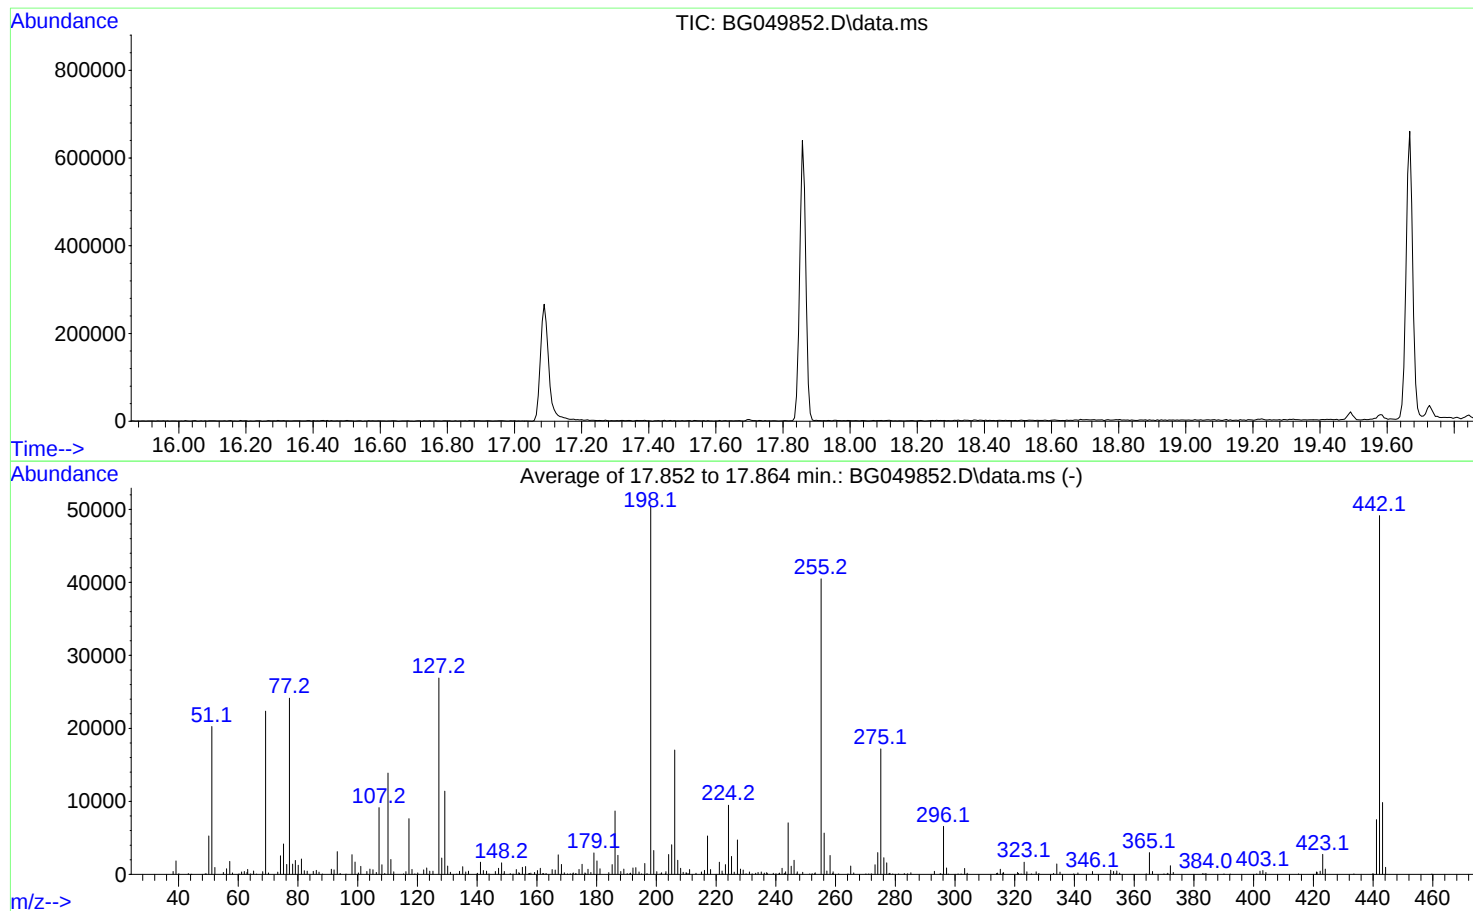




AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	20263	PASS
68	69	0.00	2	1.6	365	PASS
69	198	0.00	100	44.4	22360	PASS
70	69	0.00	2	0.8	190	PASS
127	198	10	80	53.4	26904	PASS
197	198	0.00	2	0.2	107	PASS
198	198	100	100	100.0	50397	PASS
199	198	5	9	6.5	3263	PASS
275	198	10	60	34.1	17181	PASS
365	198	1	100	5.9	2989	PASS
441	198	0.01	100	14.9	7495	PASS
442	442	100	100	100.0	49157	PASS
443	442	15	24	20.0	9849	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081621\
Data File : BG049852.D
Acq On : 16 Aug 2021 16:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 16 17:08:15 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 15:15:33 2021
Response via : Initial Calibration

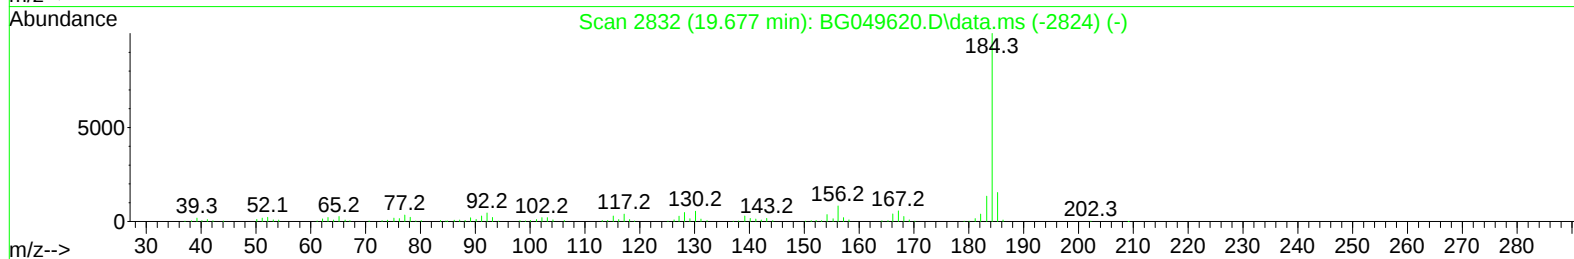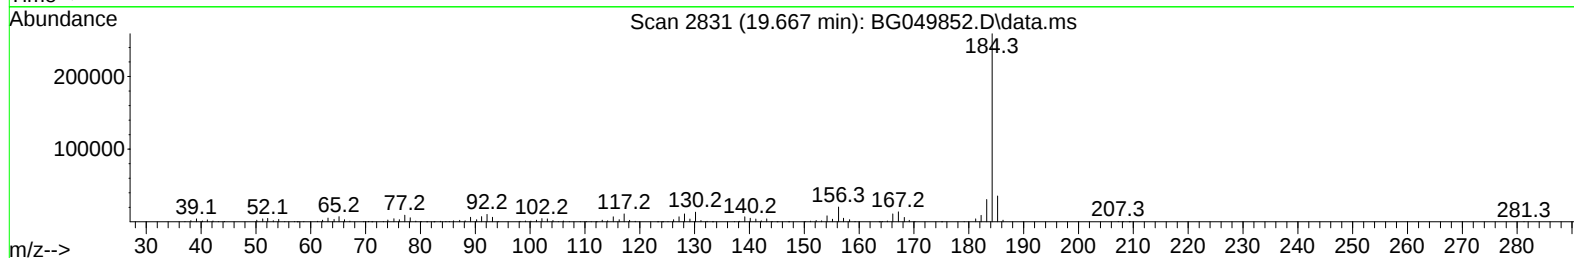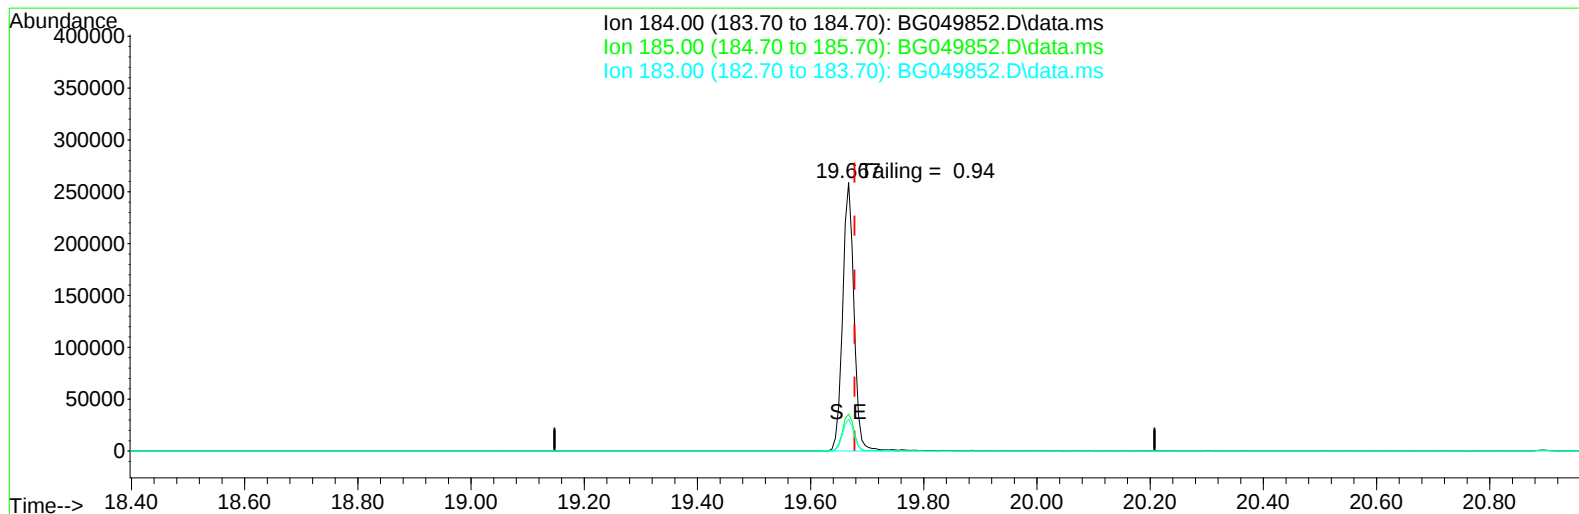

TIC: BG049852.D\data.ms

(77) Benzidine

19.667min (-0.010) 5342.17 ng m




response 357114

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.76
183.00	11.70	11.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081621\
Data File : BG049852.D
Acq On : 16 Aug 2021 16:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 16 17:08:15 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 15:15:33 2021
Response via : Initial Calibration

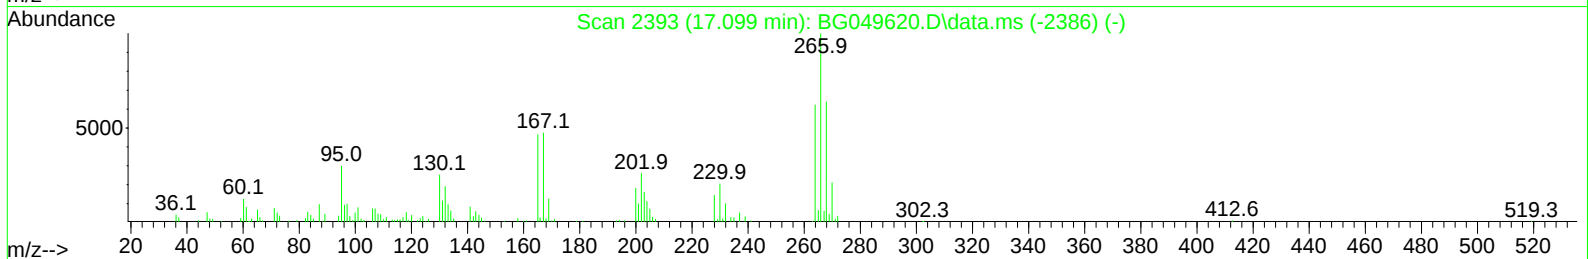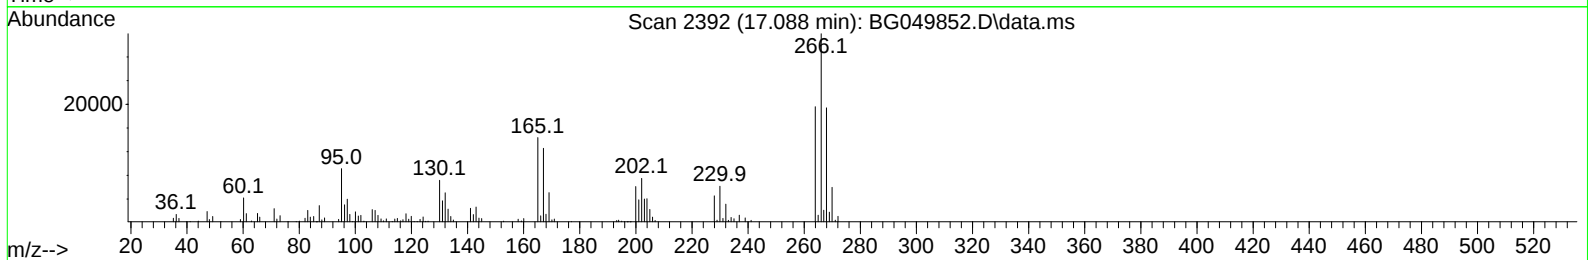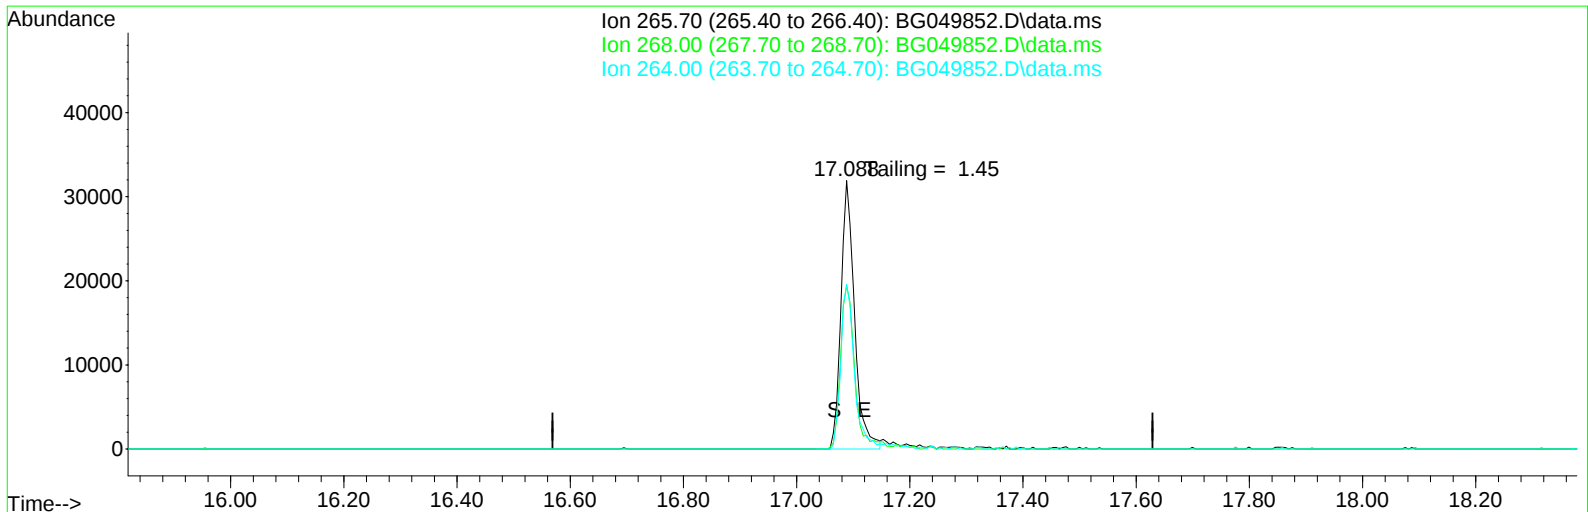

TIC: BG049852.D\data.ms

(70) Pentachlorophenol (C)

17.088min (-0.010) 123587.48 ng m

response 52894

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	60.79
264.00	61.30	61.34
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/16/2021	BNA_G	<u>BG049852.D</u>
Compound Name	Response	Retention Time
DDT	202894	20.89
DDD	1355	20.46
DDE	416	19.94
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1771	204665	0.87

Instrument :
BNA_G
ClientSampleId :
DFTPP