
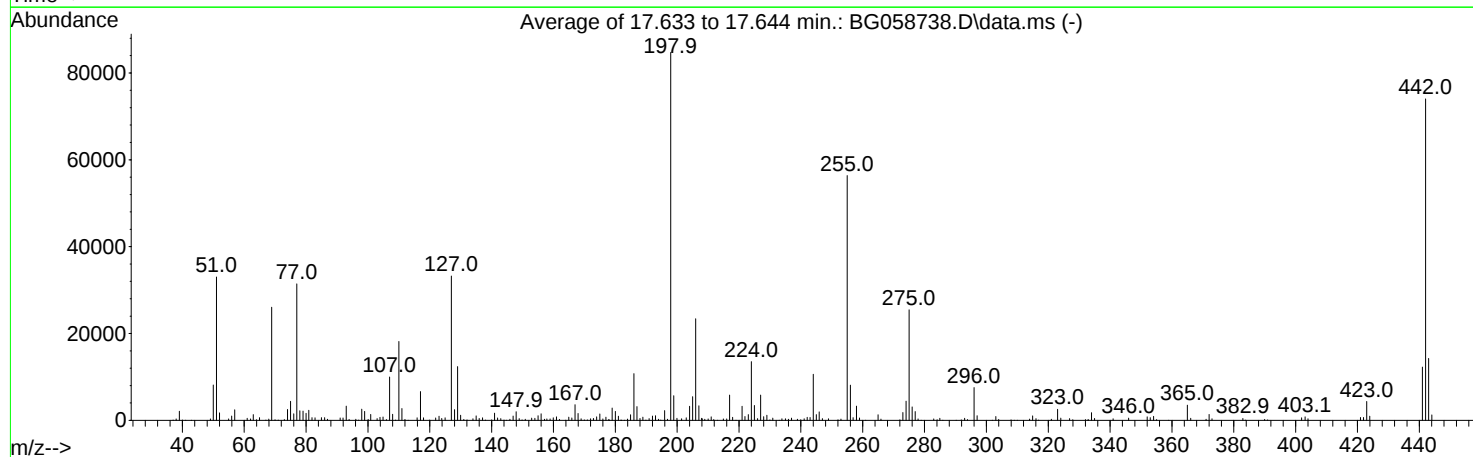


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081623\
 Data File : BG058738.D
 Acq On : 16 Aug 2023 7:05
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 28 22:29:07 2023

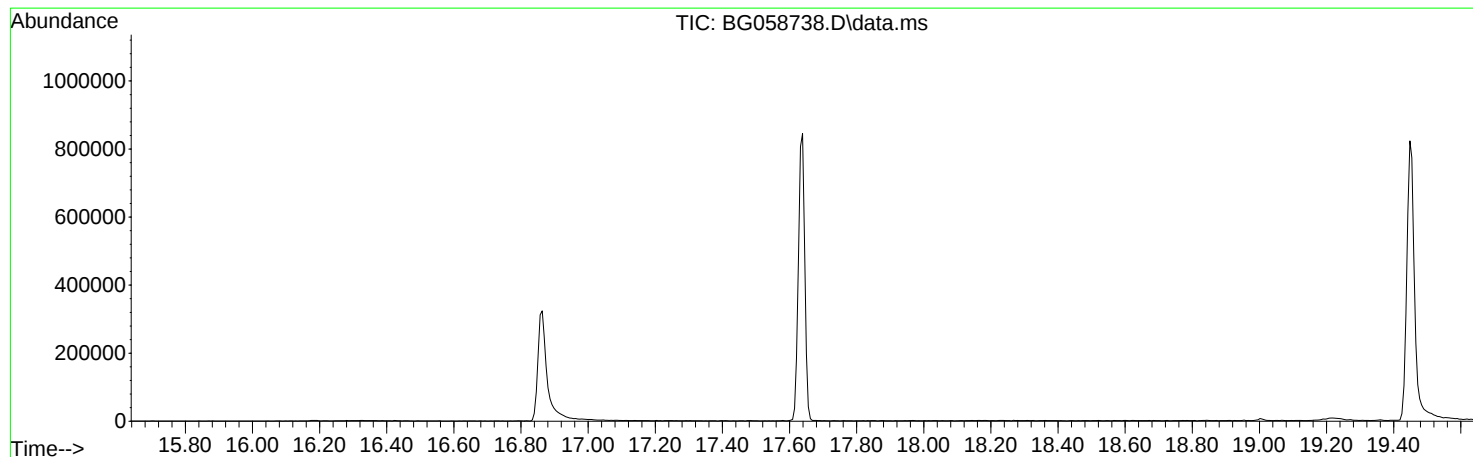




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	33000	PASS
68	69	0.00	2	1.1	285	PASS
69	198	0.00	100	30.7	26036	PASS
70	69	0.00	2	0.5	139	PASS
127	198	10	80	39.2	33243	PASS
197	198	0.00	2	0.3	244	PASS
198	198	100	100	100.0	84707	PASS
199	198	5	9	6.7	5672	PASS
275	198	10	60	30.0	25451	PASS
365	198	1	100	4.1	3486	PASS
441	198	0.01	100	14.5	12271	PASS
442	442	50	100	100.0	74021	PASS
443	442	15	24	19.3	14272	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081623\
Data File : BG058738.D
Acq On : 16 Aug 2023 7:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 16 18:28:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

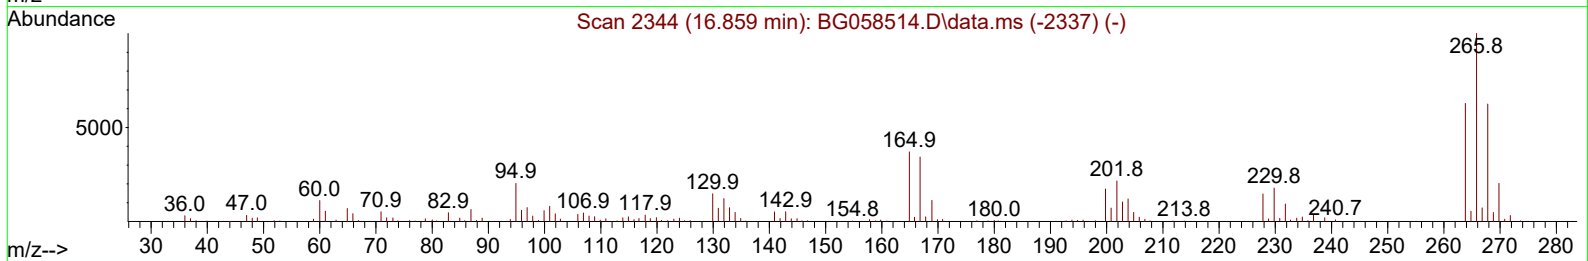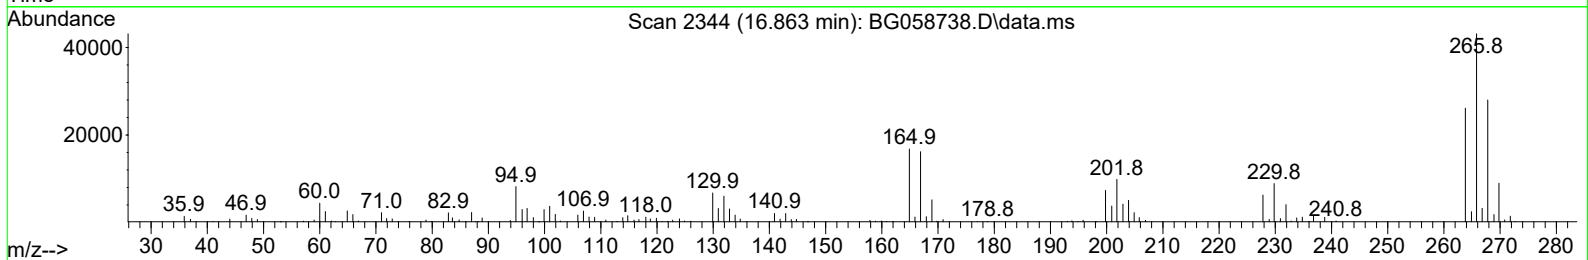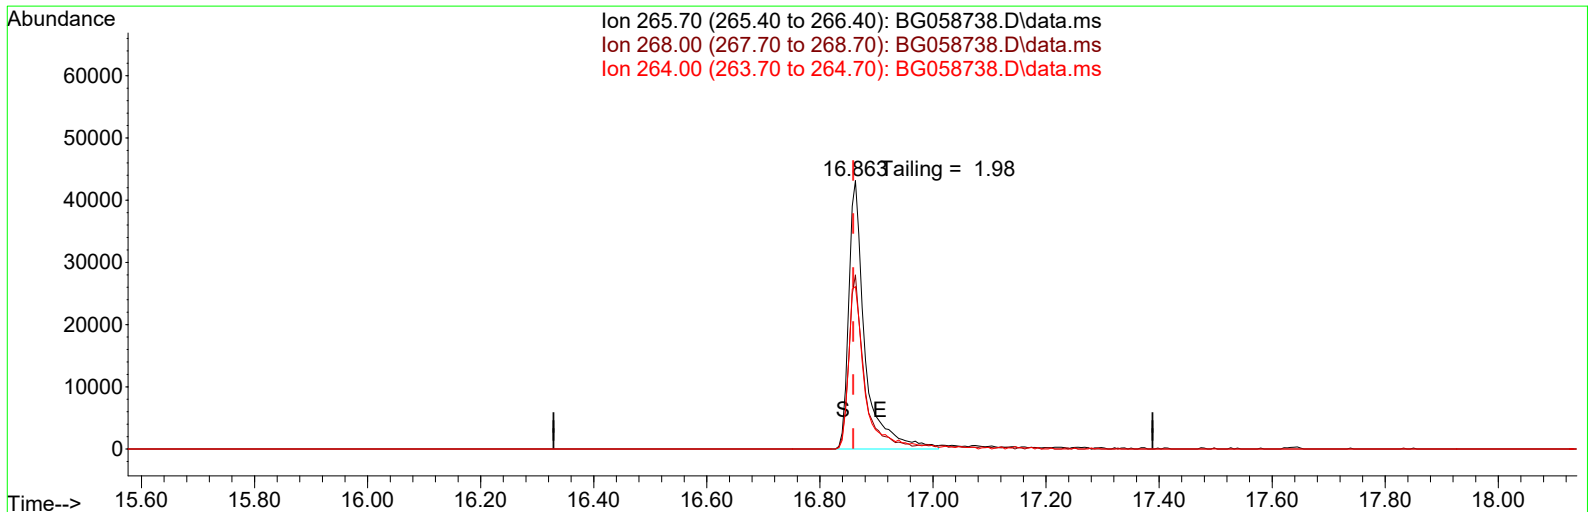

TIC: BG058738.D\data.ms

(70) Pentachlorophenol (C)

16.863min (+ 0.004) 22089.62 ng




response 86454

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	64.90
264.00	62.80	60.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081623\
Data File : BG058738.D
Acq On : 16 Aug 2023 7:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 16 18:28:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

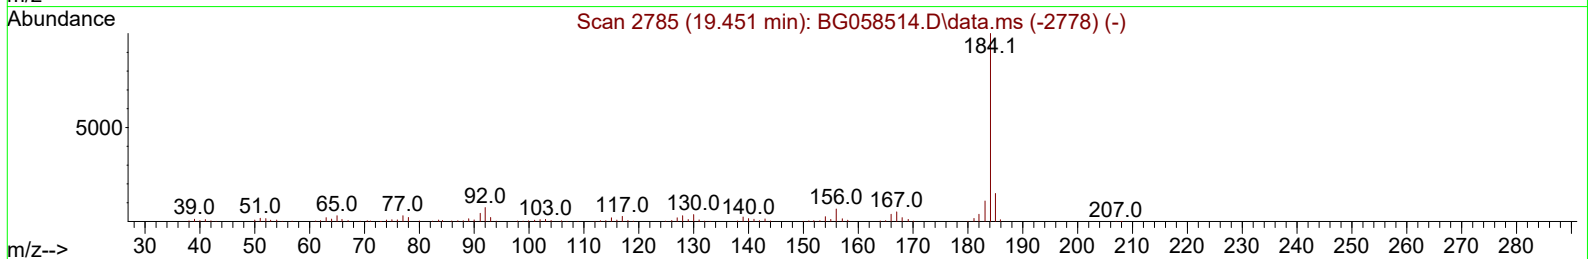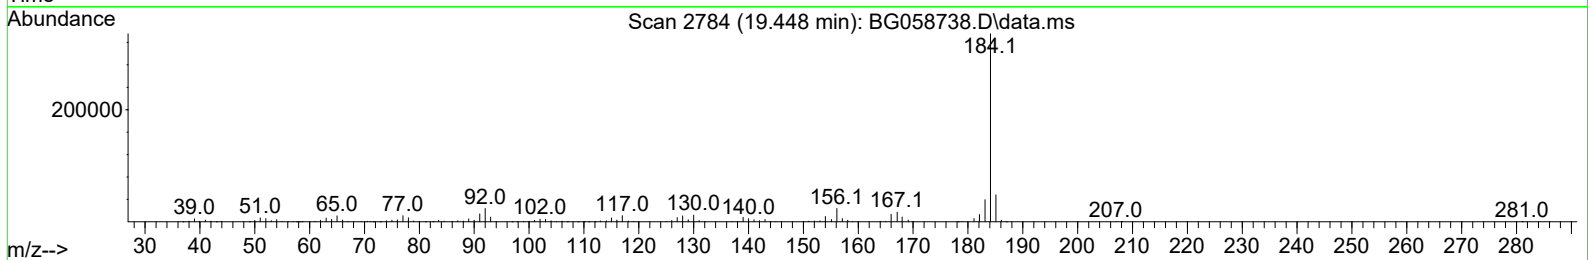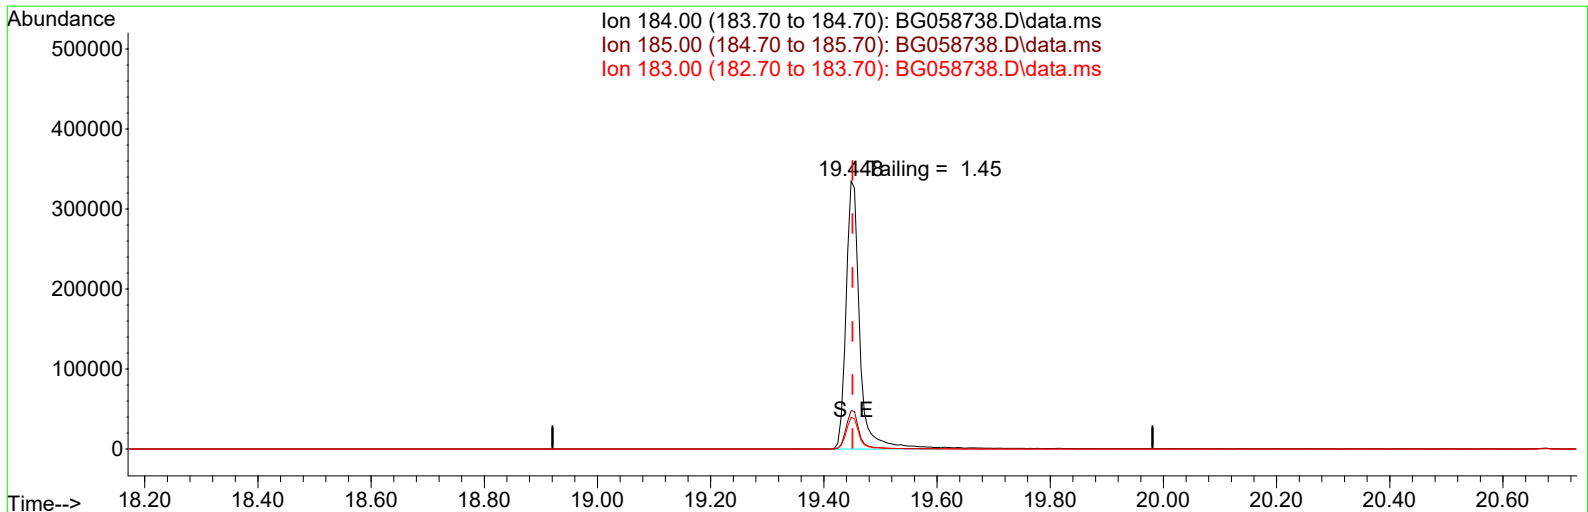

TIC: BG058738.D\data.ms

(77) Benzidine

19.448min (-0.002) 662813.01 ng

response 562852

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.32
183.00	10.90	11.80
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/16/2023	BNA_G	<u>BG058738.D</u>
Compound Name	Response	Retention Time
DDT	288060	20.67
DDD	8205	20.235
DDE	750	19.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8955	297015	3.01

Instrument :
BNA_G
ClientSampleId :
DFTPP