
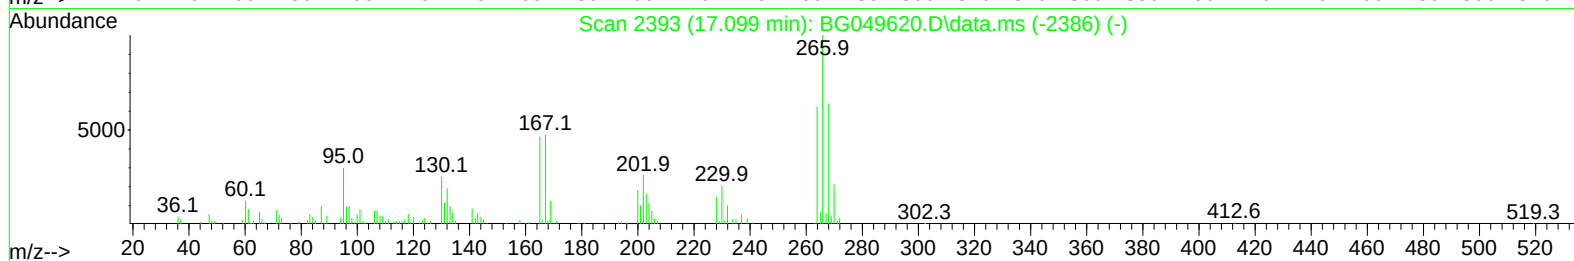
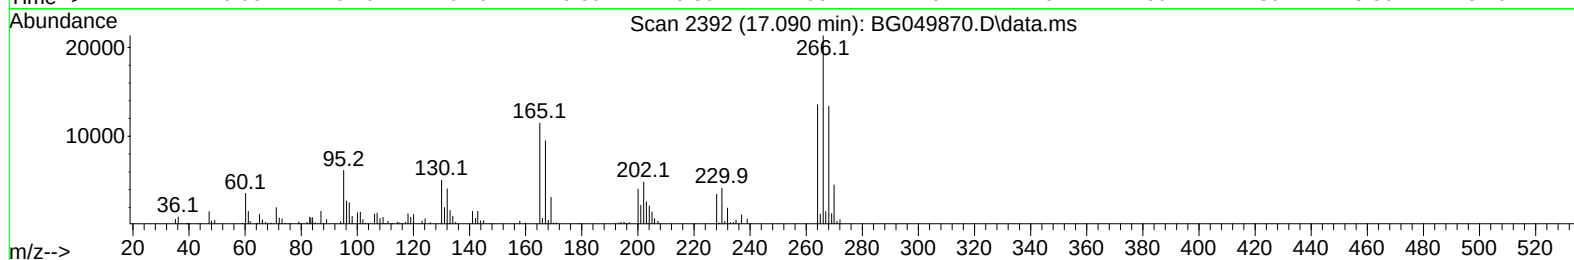


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081721\
Data File : BG049870.D
Acq On : 17 Aug 2021 9:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 11:54:19 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 16 18:23:02 2021
Response via : Initial Calibration

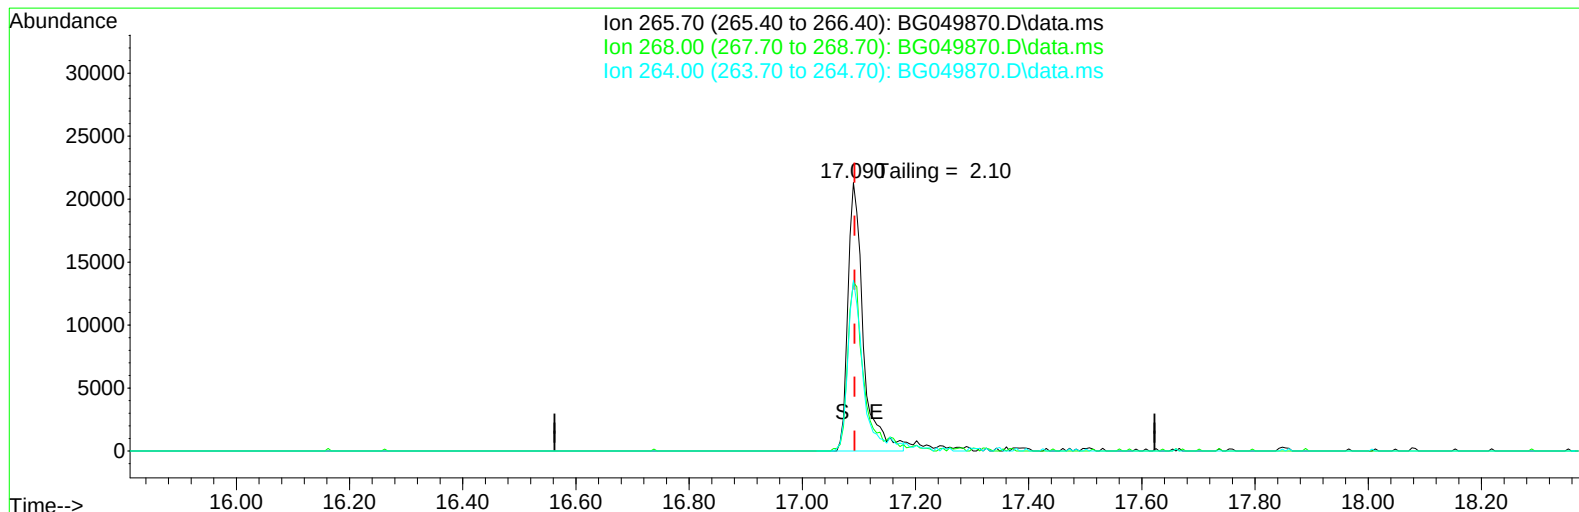

TIC: BG049870.D\data.ms

(70) Pentachlorophenol (C)




17.090min (-0.002) 99258.98 ng

response 39696

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	62.83
264.00	61.30	63.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081721\
Data File : BG049870.D
Acq On : 17 Aug 2021 9:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 11:54:19 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 16 18:23:02 2021
Response via : Initial Calibration

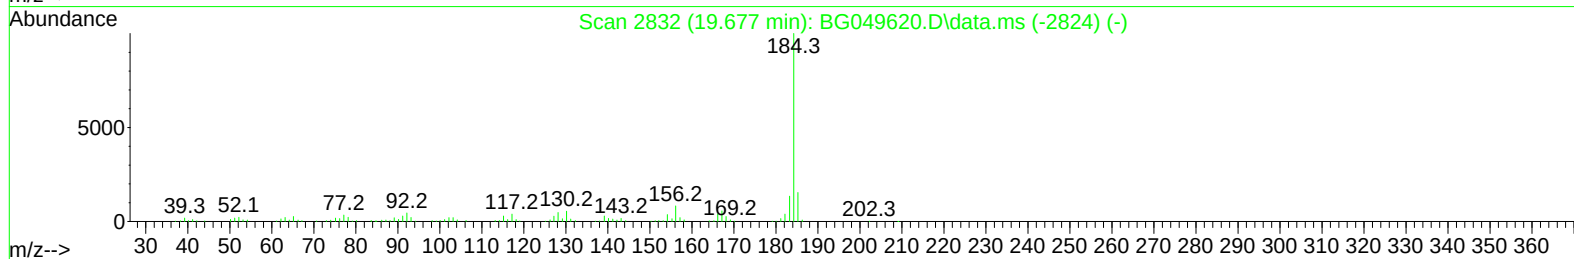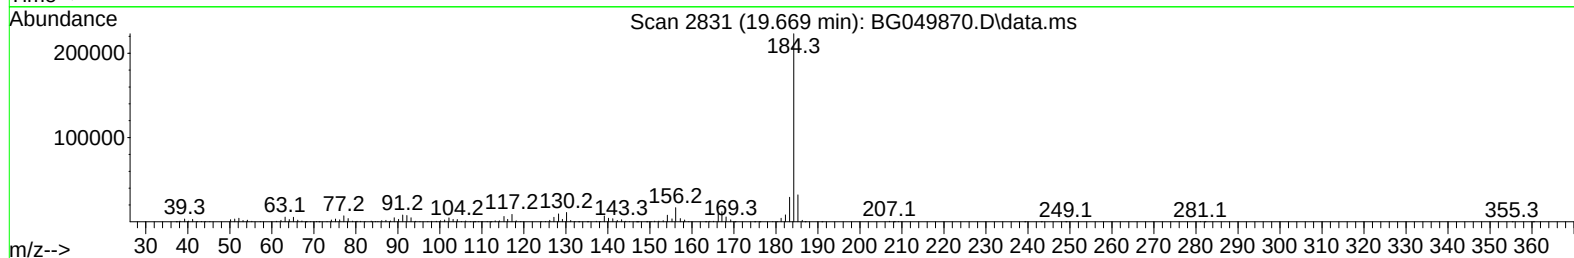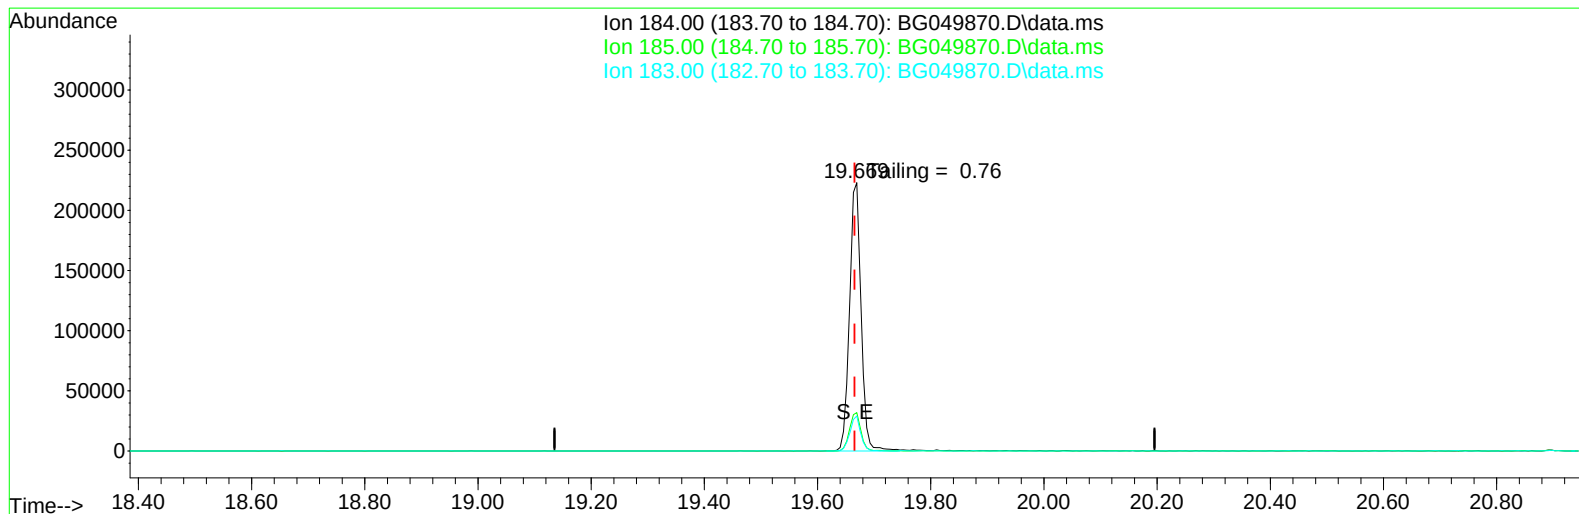

TIC: BG049870.D\data.ms

(77) Benzidine

19.669min (+ 0.004) 176687.71 ng

response 316898

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.33
183.00	11.70	13.08
0.00	0.00	0.00