
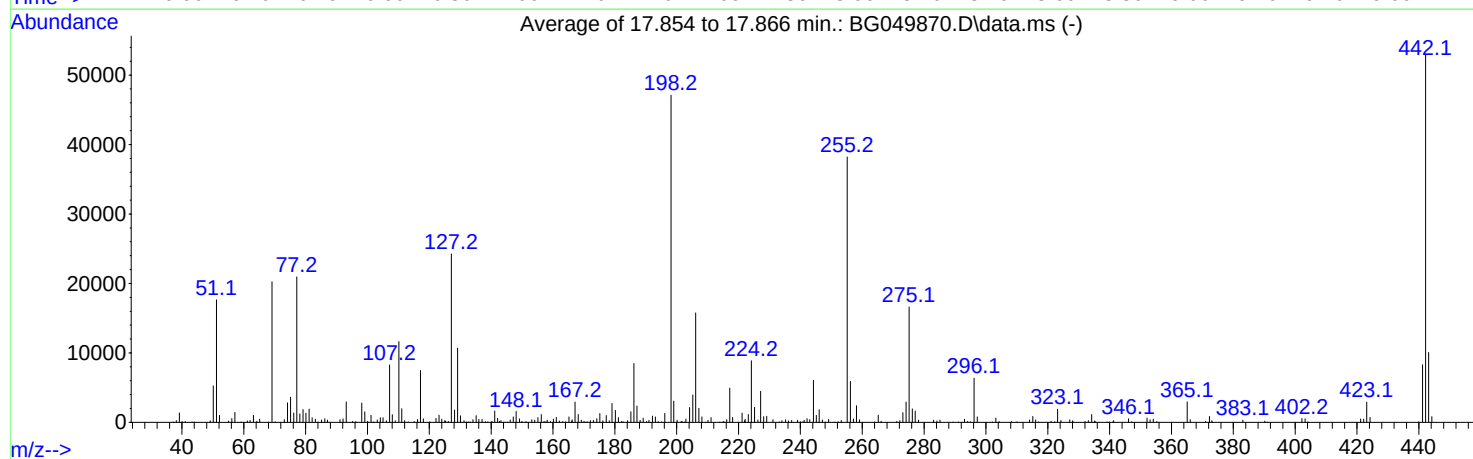


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG081721\  
 Data File : BG049870.D  
 Acq On : 17 Aug 2021 9:30  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG080321.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Aug 16 18:23:02 2021

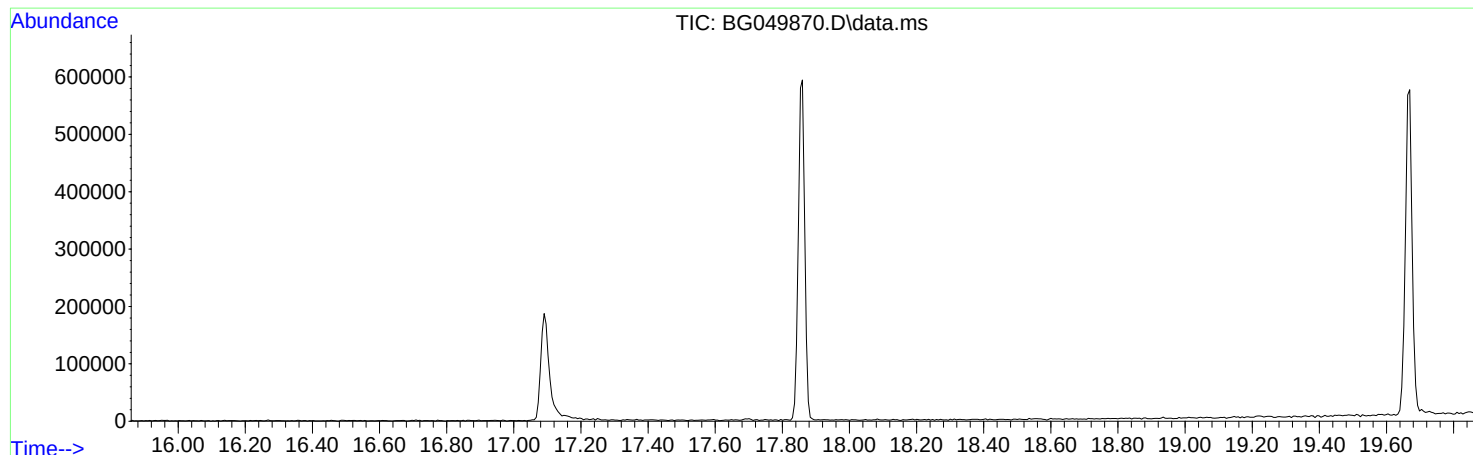




AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2515

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 37.5         | 17651      | PASS                |
| 68             | 69              | 0.00            | 2               | 0.3          | 53         | PASS                |
| 69             | 198             | 0.00            | 100             | 43.0         | 20244      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 96         | PASS                |
| 127            | 198             | 10              | 80              | 51.5         | 24266      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 47109      | PASS                |
| 199            | 198             | 5               | 9               | 6.5          | 3065       | PASS                |
| 275            | 198             | 10              | 60              | 35.2         | 16601      | PASS                |
| 365            | 198             | 1               | 100             | 6.3          | 2946       | PASS                |
| 441            | 198             | 0.01            | 100             | 17.6         | 8297       | PASS                |
| 442            | 442             | 100             | 100             | 100.0        | 52965      | PASS                |
| 443            | 442             | 15              | 24              | 19.0         | 10059      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG081721\  
Data File : BG049870.D  
Acq On : 17 Aug 2021 9:30  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Aug 17 11:54:19 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG080321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 16 18:23:02 2021  
Response via : Initial Calibration

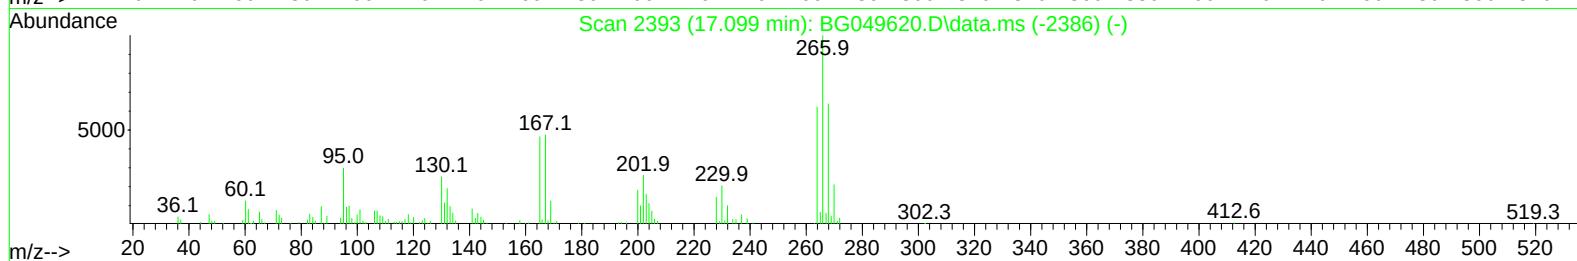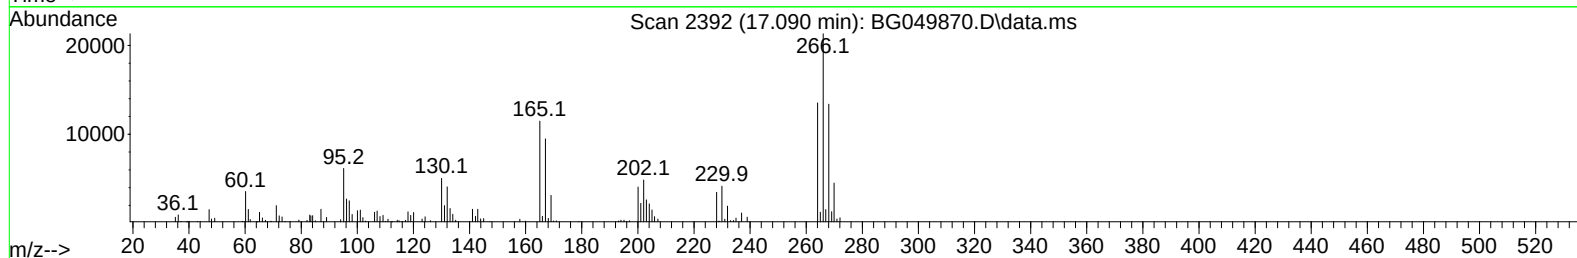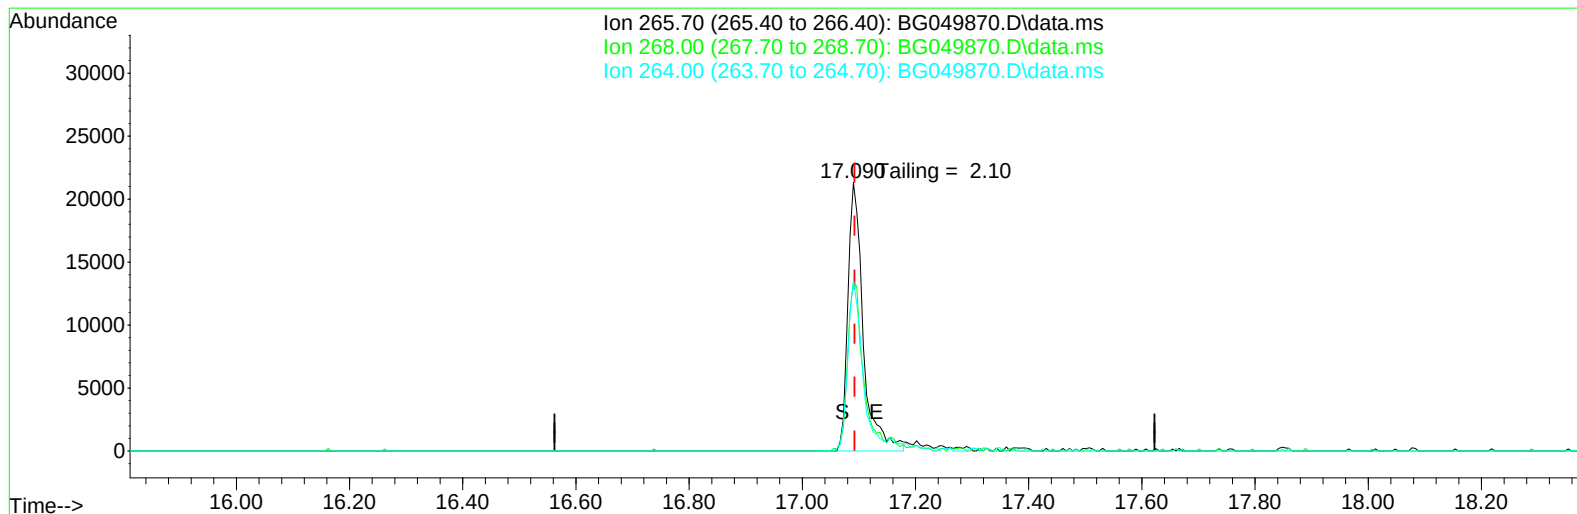

TIC: BG049870.D\data.ms

**(70) Pentachlorophenol (C)**

17.090min (-0.002) 99258.98 ng




response 39696

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.20  | 62.83  |
| 264.00 | 61.30  | 63.54  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG081721\  
Data File : BG049870.D  
Acq On : 17 Aug 2021 9:30  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Aug 17 11:54:19 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG080321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 16 18:23:02 2021  
Response via : Initial Calibration

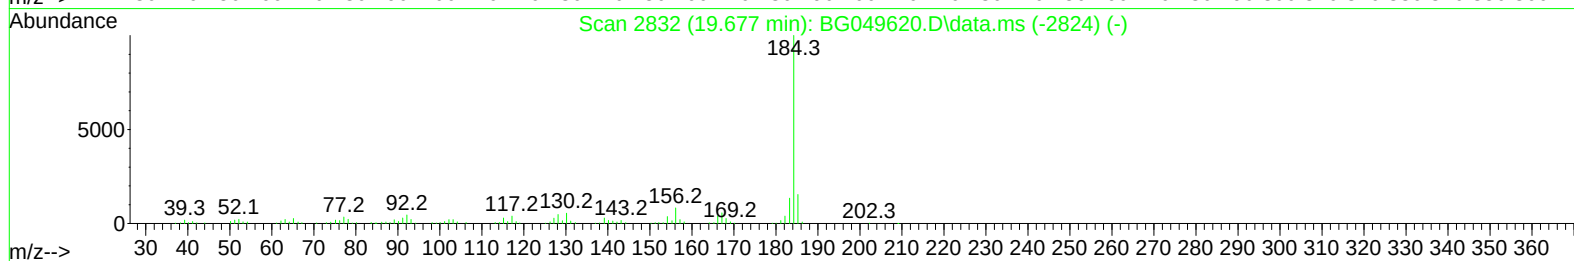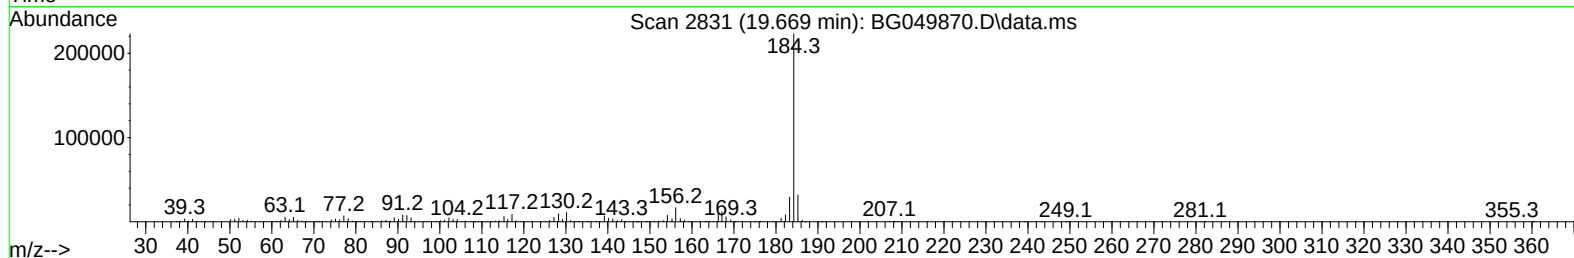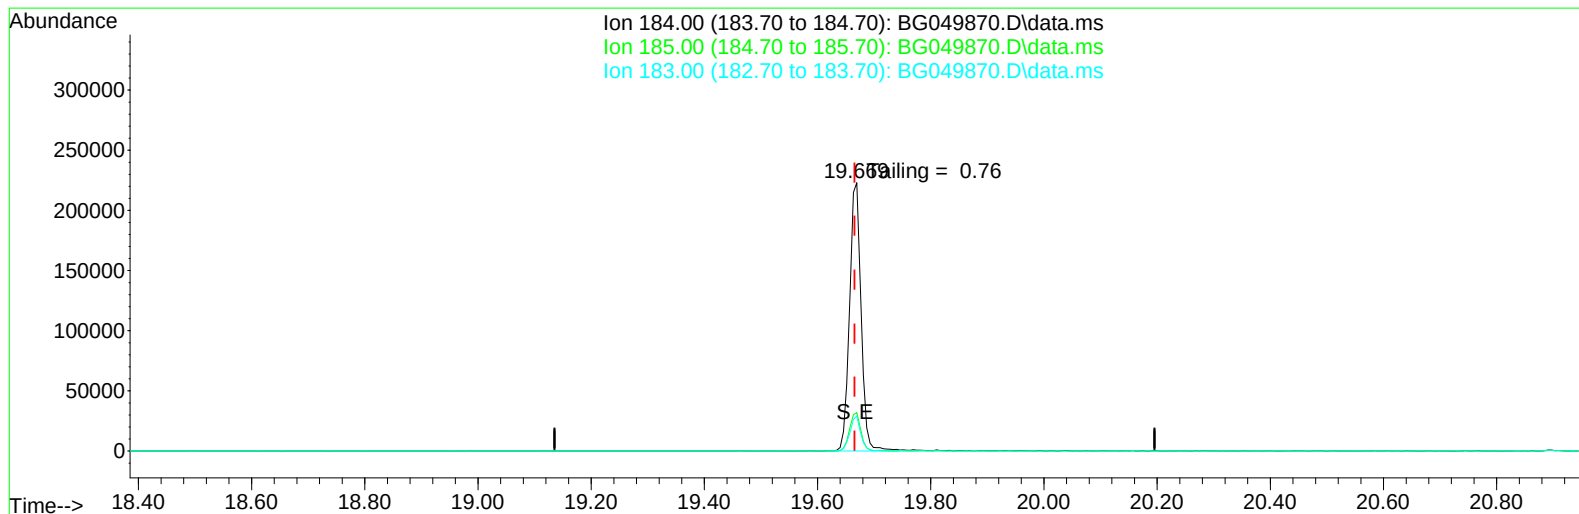

TIC: BG049870.D\data.ms

(77) Benzidine

19.669min (+ 0.004) 176687.71 ng

response 316898

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.40  | 14.33  |
| 183.00 | 11.70  | 13.08  |
| 0.00   | 0.00   | 0.00   |

DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 8/17/2021     | BNA_G            | BG049870.D         |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 148986           | 20.89              |
| DDD           | 1758             | 20.45              |
| DDE           | 757              | 19.95              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 2515          | 151501           | 1.66               |
|               |                  |                    |