


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081723\
Data File : BG058753.D
Acq On : 17 Aug 2023 7:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 28 22:29:07 2023

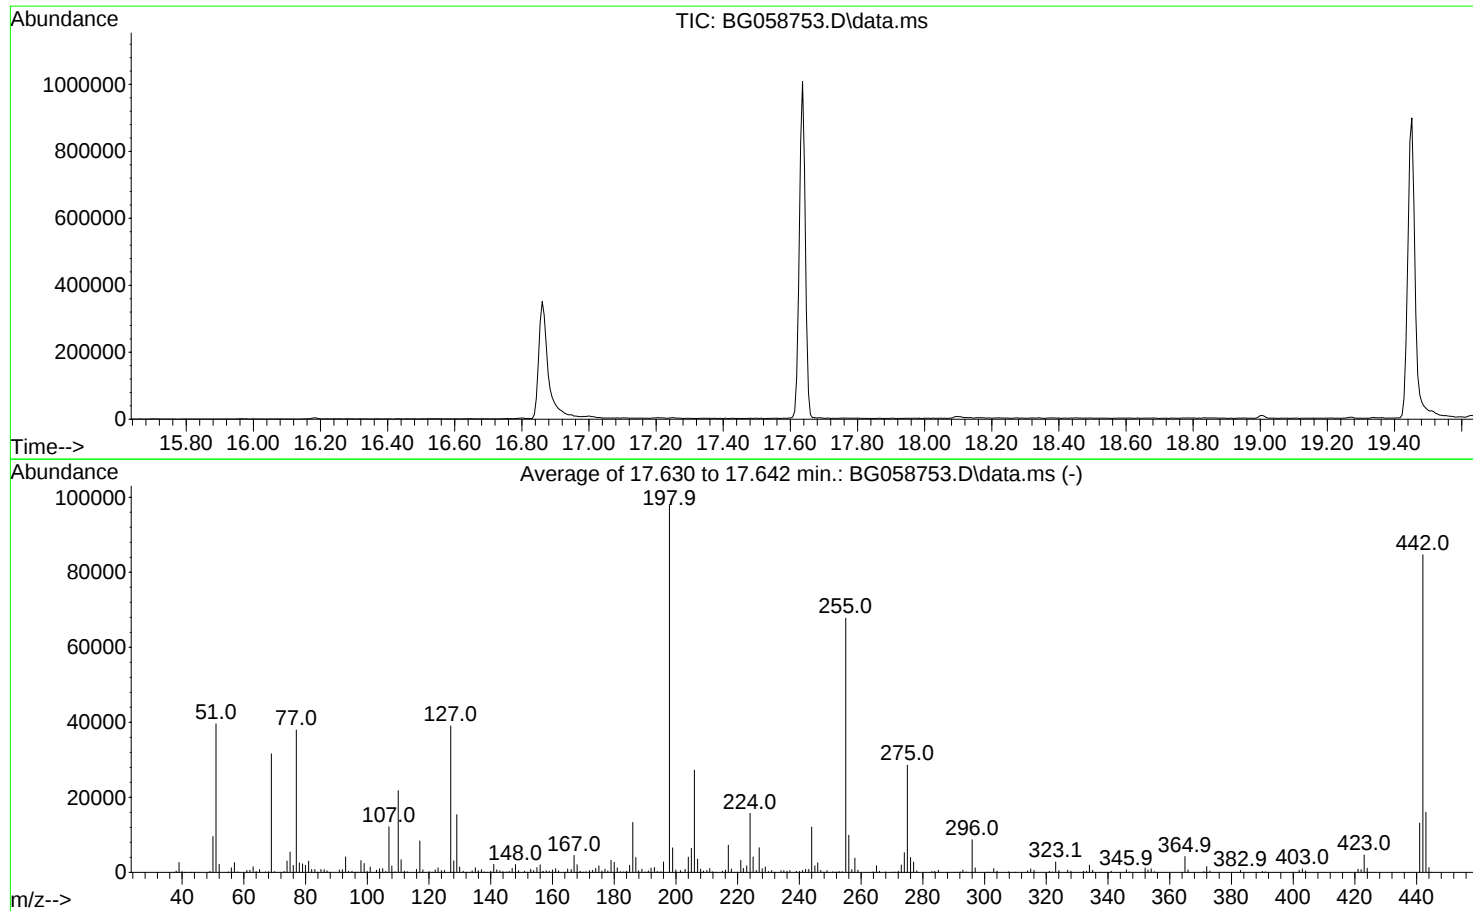




Spectrum Information: Average of 17.630 to 17.642 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	39573	PASS
68	69	0.00	2	0.6	181	PASS
69	198	0.00	100	32.2	31611	PASS
70	69	0.00	2	0.7	212	PASS
127	198	10	80	39.8	39019	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	98061	PASS
199	198	5	9	6.6	6521	PASS
275	198	10	60	29.1	28571	PASS
365	198	1	100	4.3	4245	PASS
441	198	0.01	100	13.4	13134	PASS
442	442	50	100	100.0	84656	PASS
443	442	15	24	18.9	16021	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081723\
Data File : BG058753.D
Acq On : 17 Aug 2023 7:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 17 09:22:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

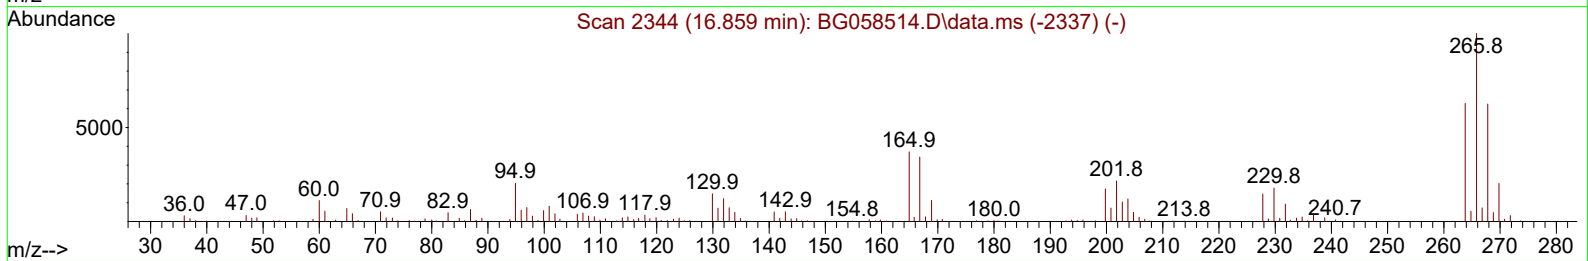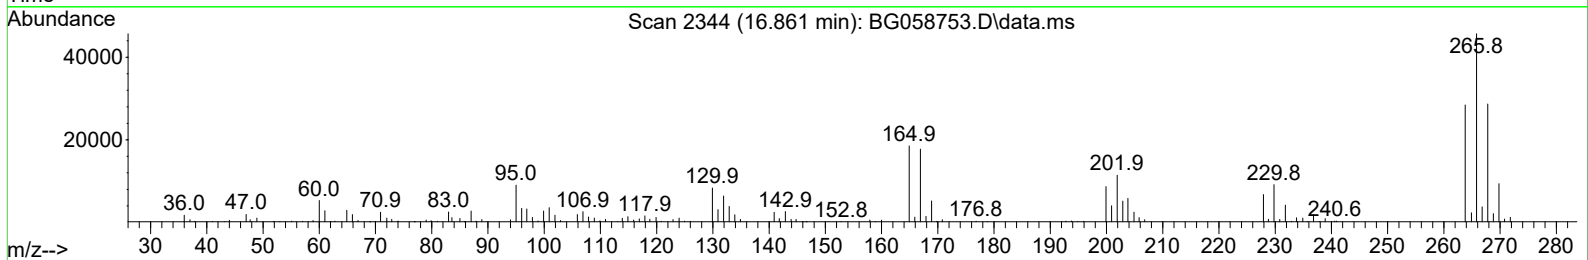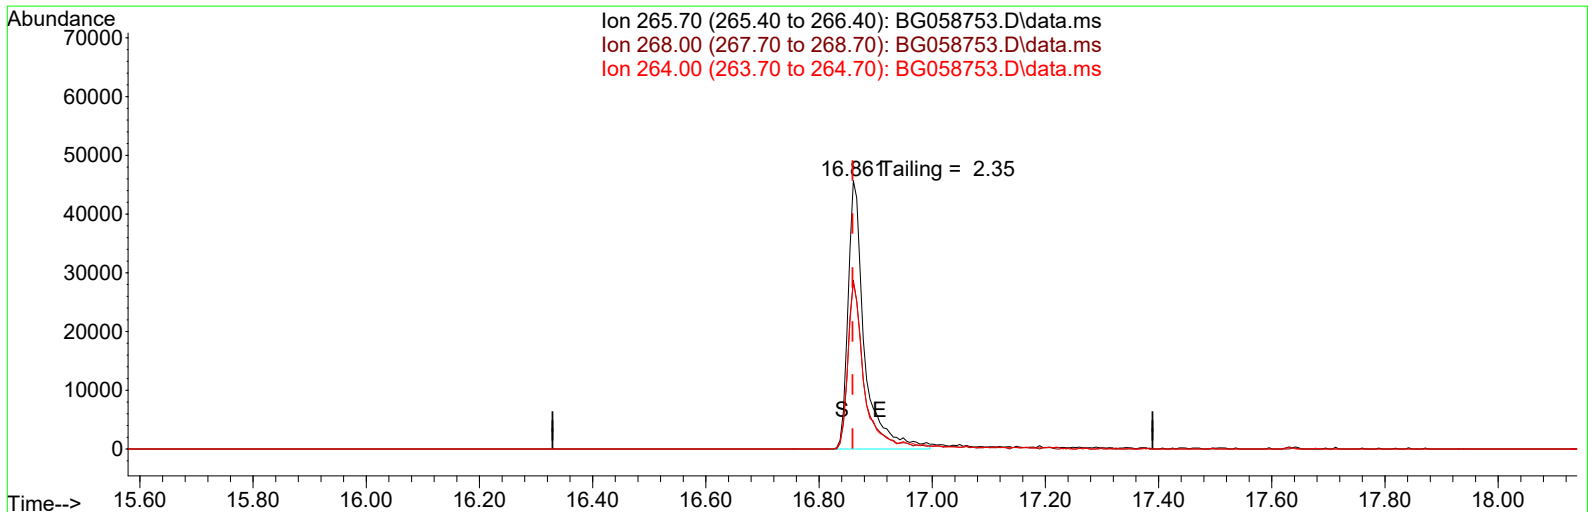

TIC: BG058753.D\data.ms

(70) Pentachlorophenol (C)

16.861min (+ 0.002) 8720.45 ng




response 91859

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	62.80
264.00	62.80	62.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081723\
Data File : BG058753.D
Acq On : 17 Aug 2023 7:41
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 17 09:22:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

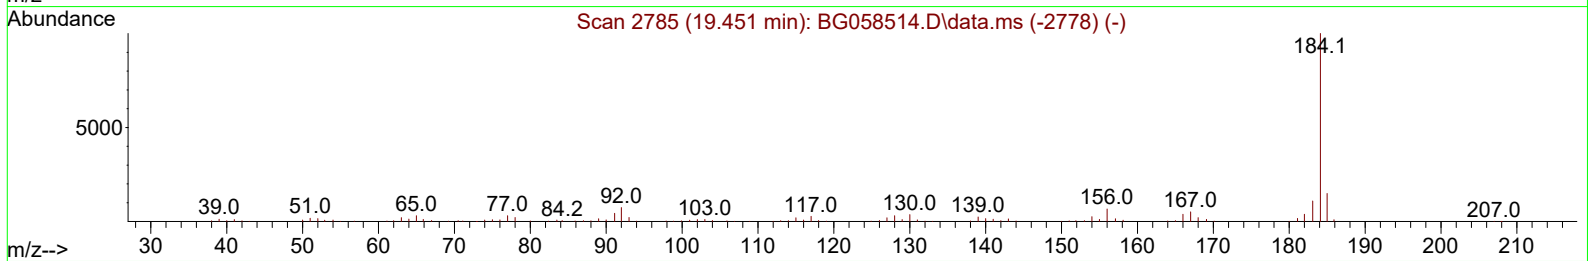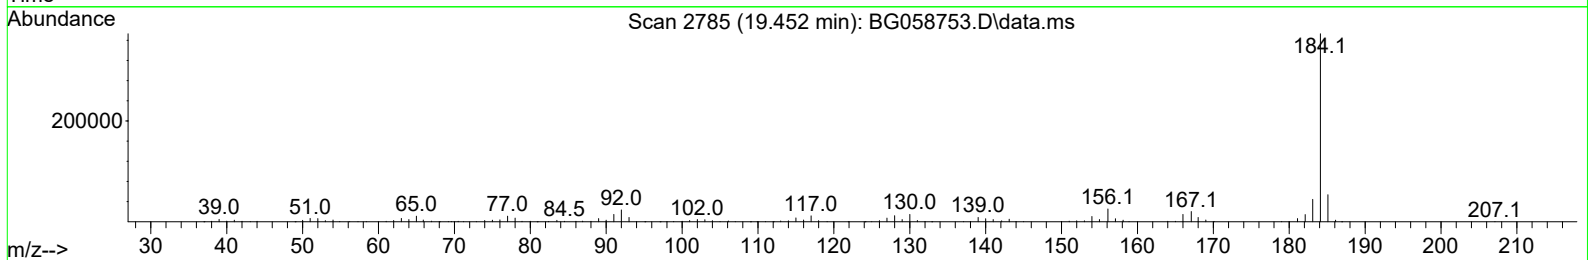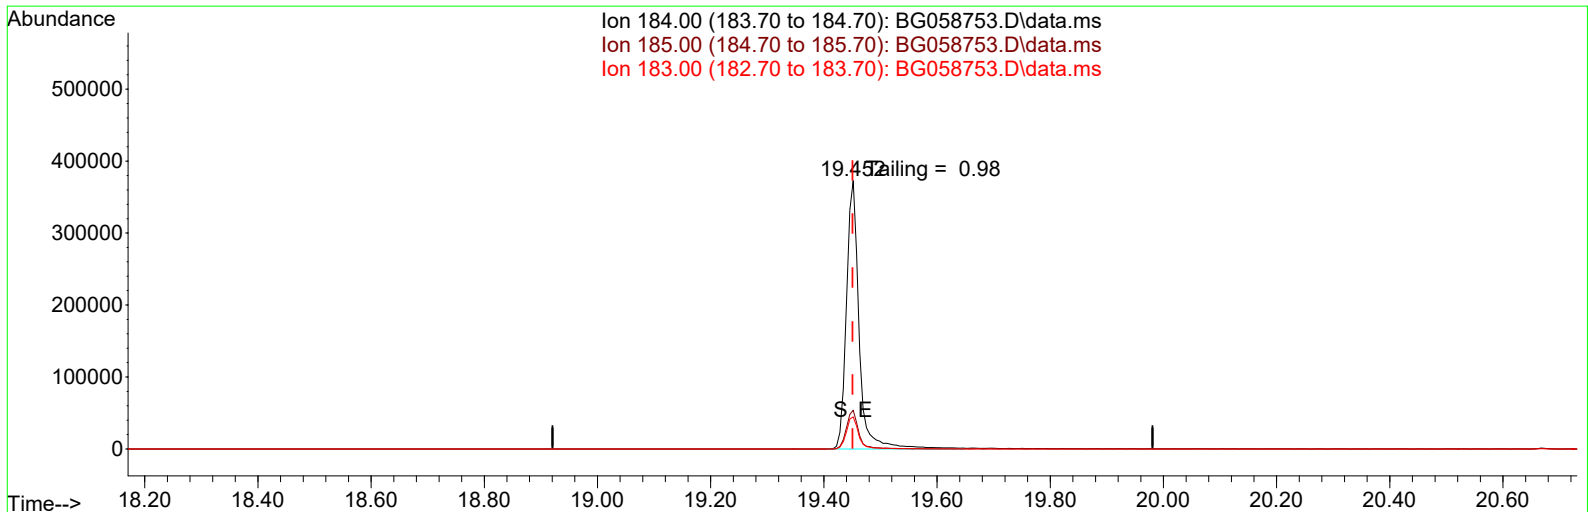

TIC: BG058753.D\data.ms

(77) Benzidine

19.452min (+ 0.001) 27495.39 ng

response 583301

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.42
183.00	10.90	11.98
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/17/2023	BNA_G	<u>BG058753.D</u>
Compound Name	Response	Retention Time
DDT	301112	20.674
DDD	9780	20.239
DDE	6768	19.728
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16548	317660	5.21

Instrument :
BNA_G
ClientSampleId :
DFTPP