
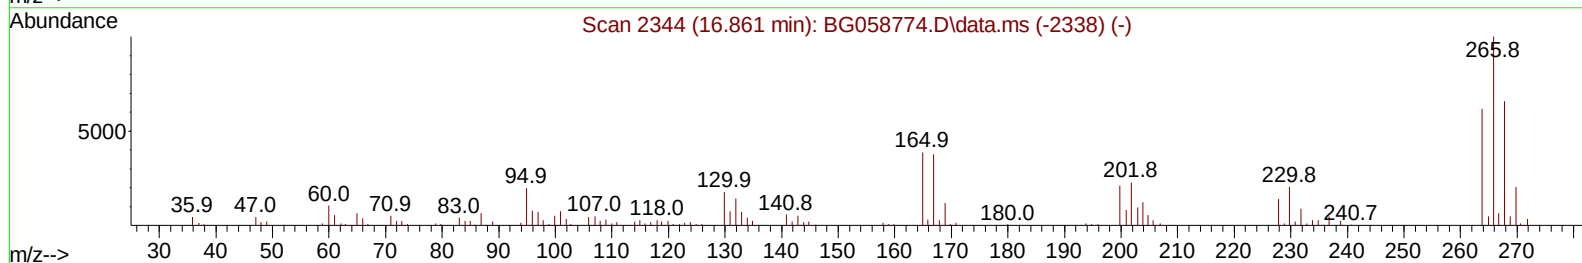
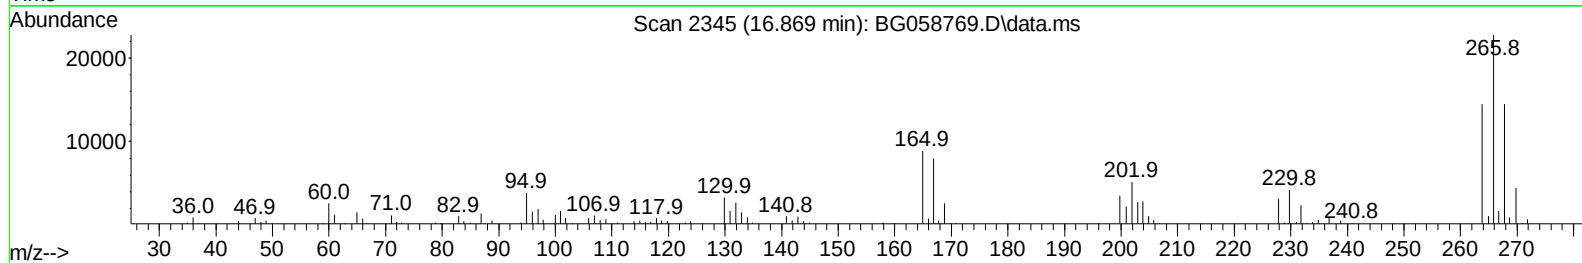


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081823\
 Data File : BG058769.D
 Acq On : 18 Aug 2023 9:58
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 18 16:32:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 18 16:13:55 2023
 Response via : Initial Calibration

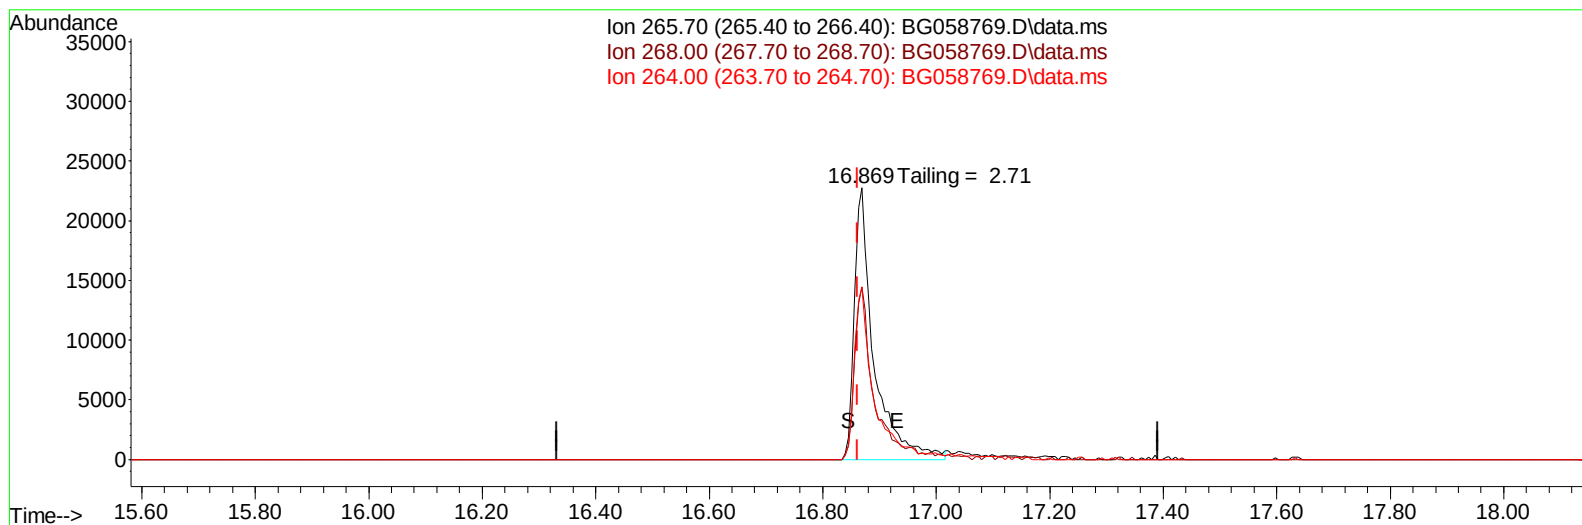




TIC: BG058769.D\data.ms

(70) Pentachlorophenol (C)**16.869min (+ 0.008) 19741.51 ng****response 54336**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.90	67.55
264.00	61.90	63.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081823\
Data File : BG058769.D
Acq On : 18 Aug 2023 9:58
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 18 16:32:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 18 16:13:55 2023
Response via : Initial Calibration

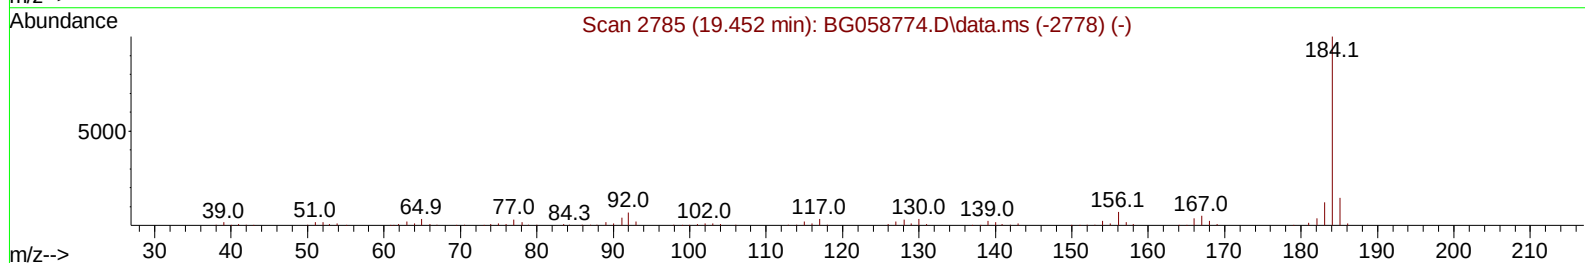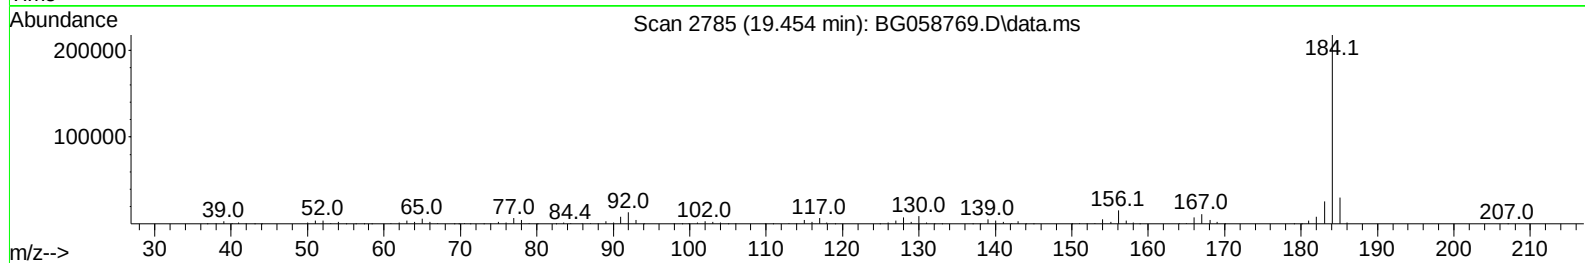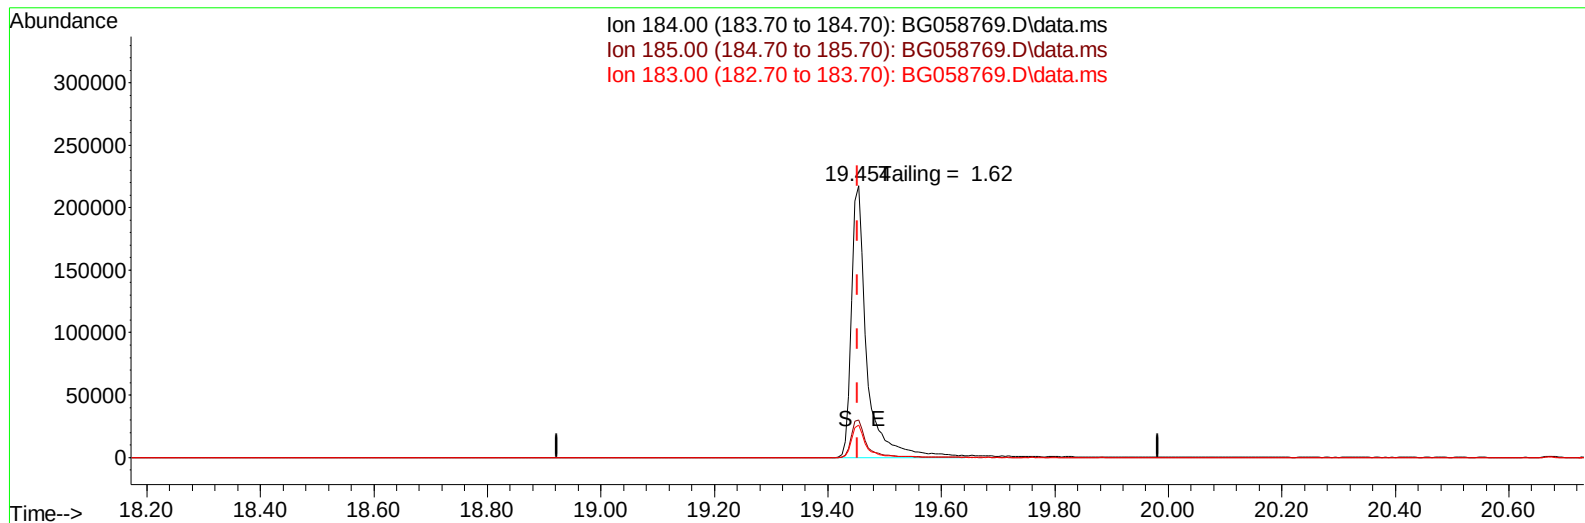

TIC: BG058769.D\data.ms

(77) Benzidine**19.454min (+ 0.002) 299332.90 ng****response 411060**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.81
183.00	12.50	11.87
0.00	0.00	0.00