


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081823\
Data File : BG058769.D
Acq On : 18 Aug 2023 9:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 21 01:40:57 2023

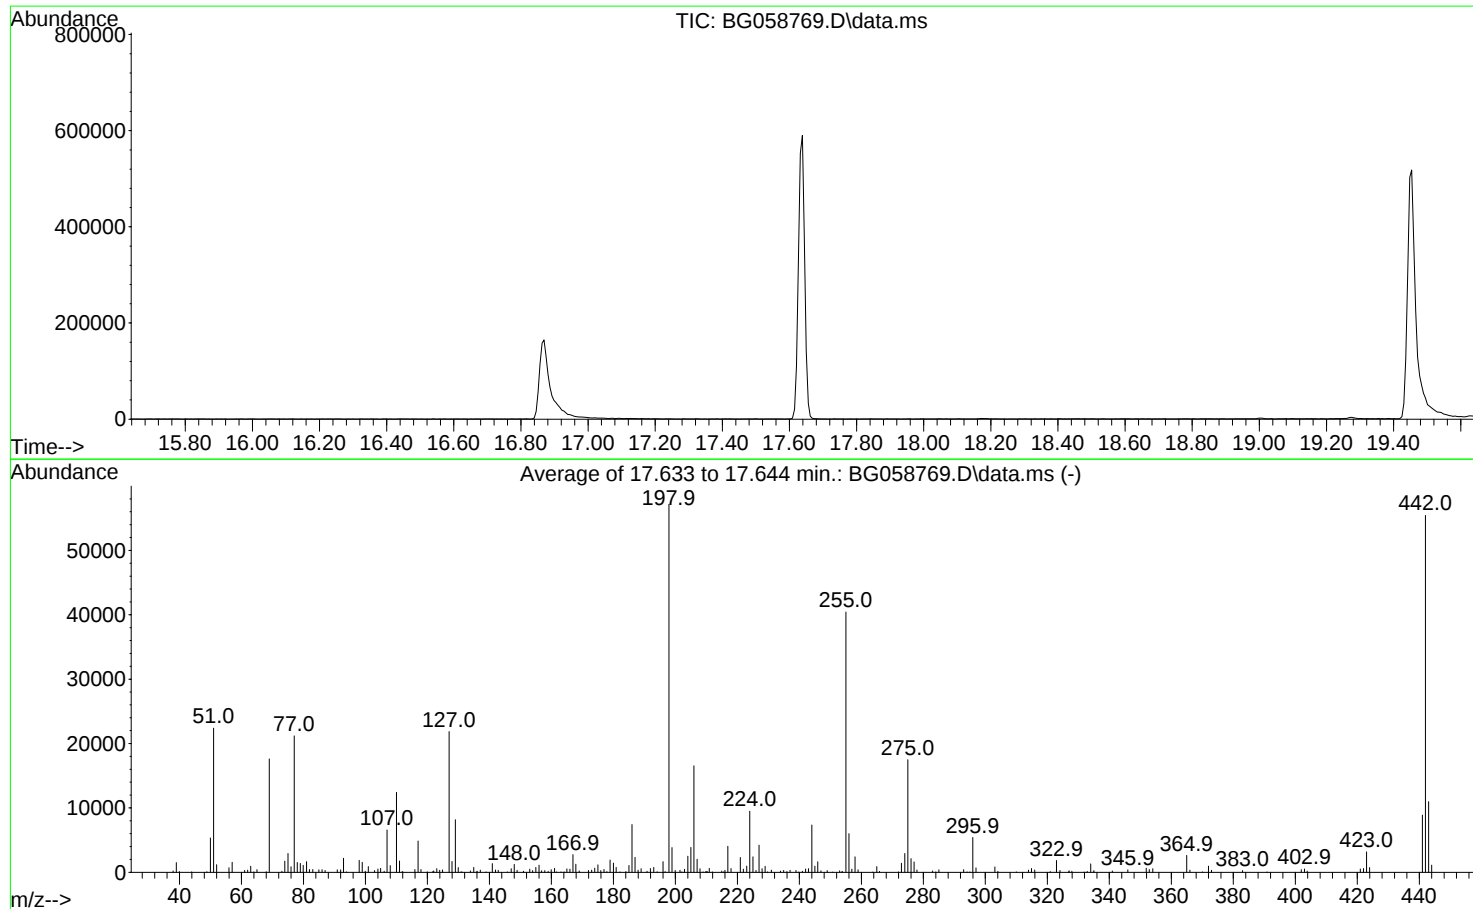




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	22395	PASS
68	69	0.00	2	0.5	85	PASS
69	198	0.00	100	30.8	17621	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.3	21862	PASS
197	198	0.00	2	0.2	122	PASS
198	198	100	100	100.0	57144	PASS
199	198	5	9	6.7	3836	PASS
275	198	10	60	30.6	17474	PASS
365	198	1	100	4.6	2618	PASS
441	198	0.01	100	15.6	8886	PASS
442	442	50	100	100.0	55453	PASS
443	442	15	24	19.8	10979	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081823\
 Data File : BG058769.D
 Acq On : 18 Aug 2023 9:58
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Aug 18 16:32:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 18 16:13:55 2023
 Response via : Initial Calibration

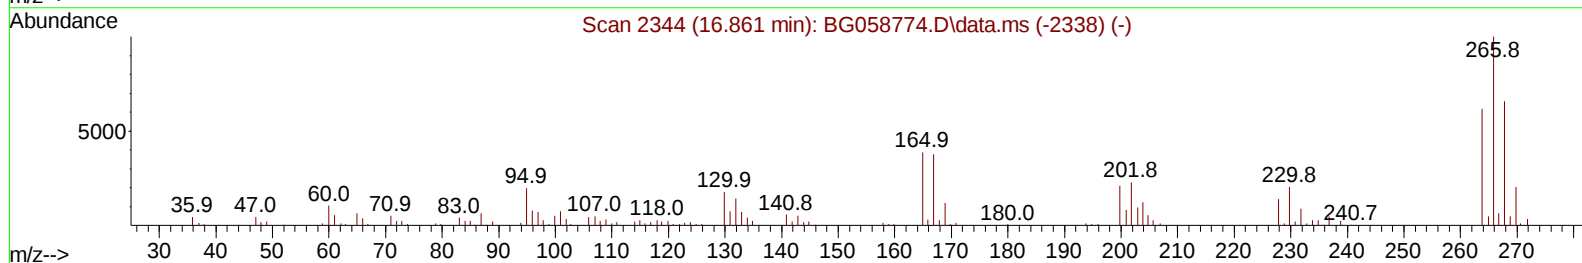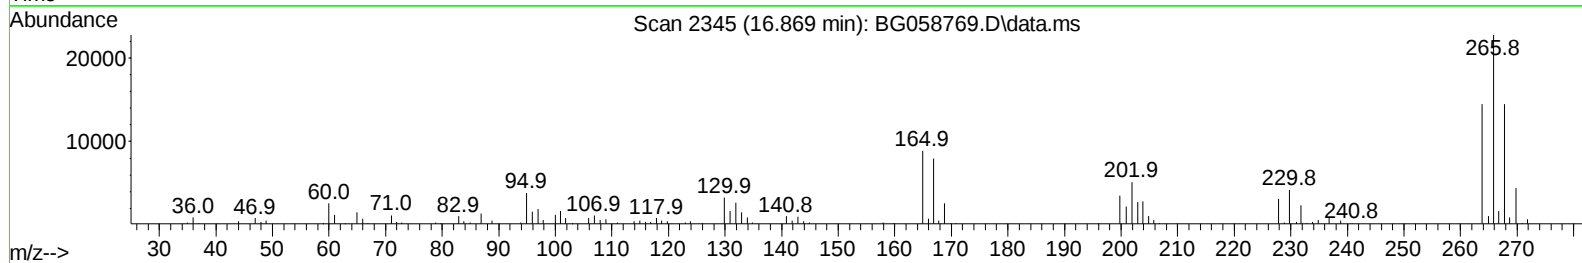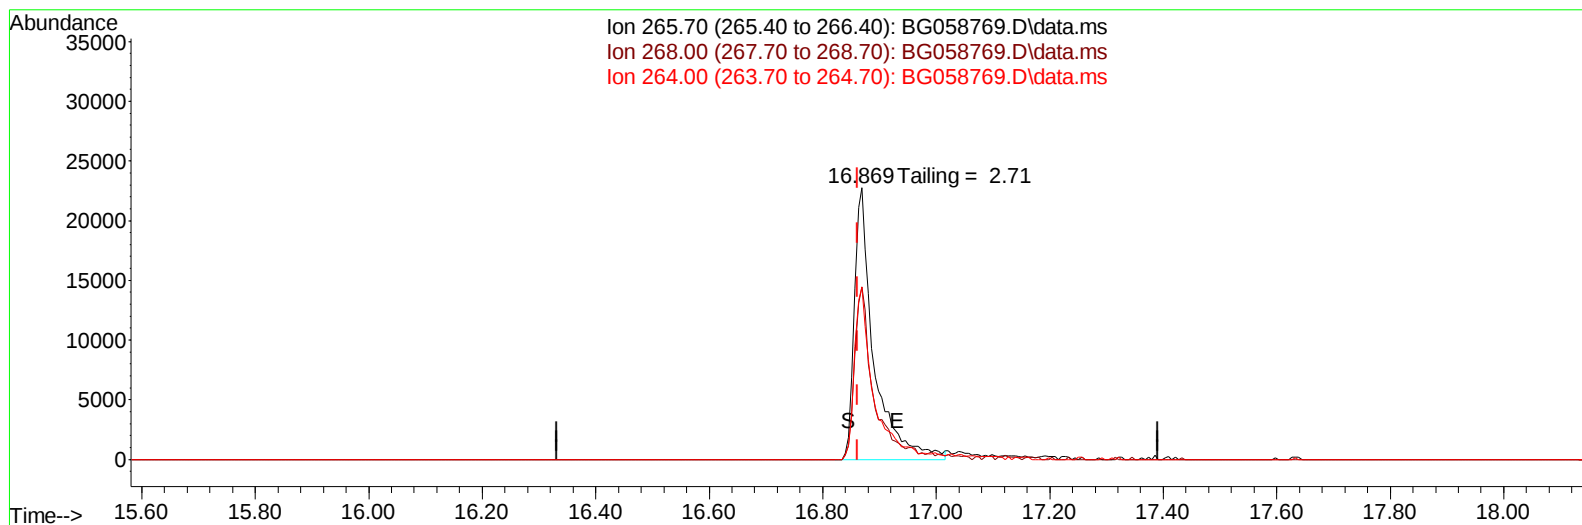

TIC: BG058769.D\data.ms




(70) Pentachlorophenol (C)**16.869min (+ 0.008) 19741.51 ng****response 54336**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.90	67.55
264.00	61.90	63.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081823\
Data File : BG058769.D
Acq On : 18 Aug 2023 9:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 18 16:32:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG081823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 18 16:13:55 2023
Response via : Initial Calibration

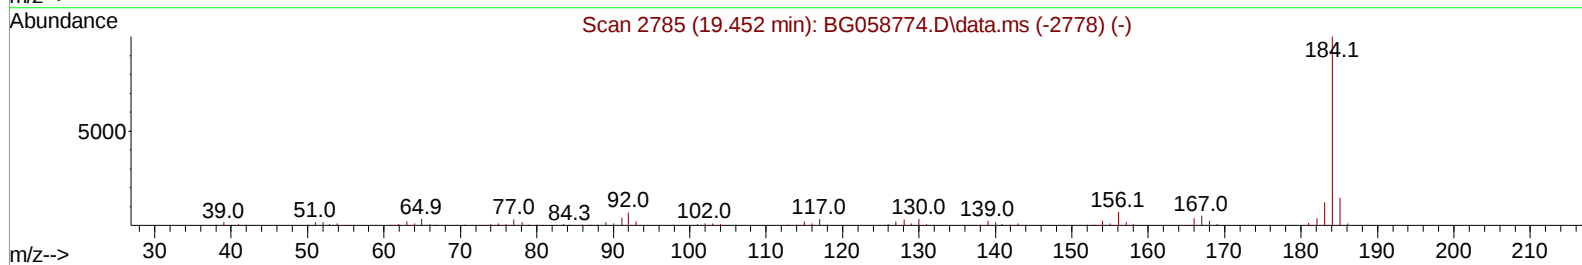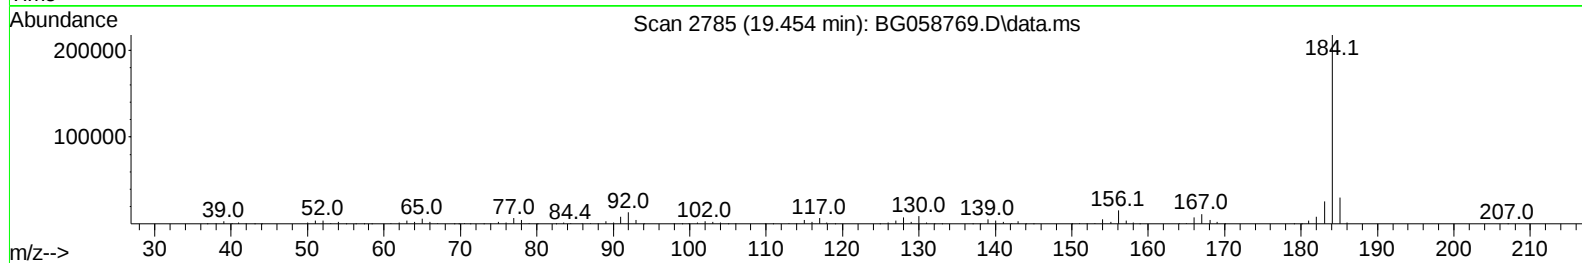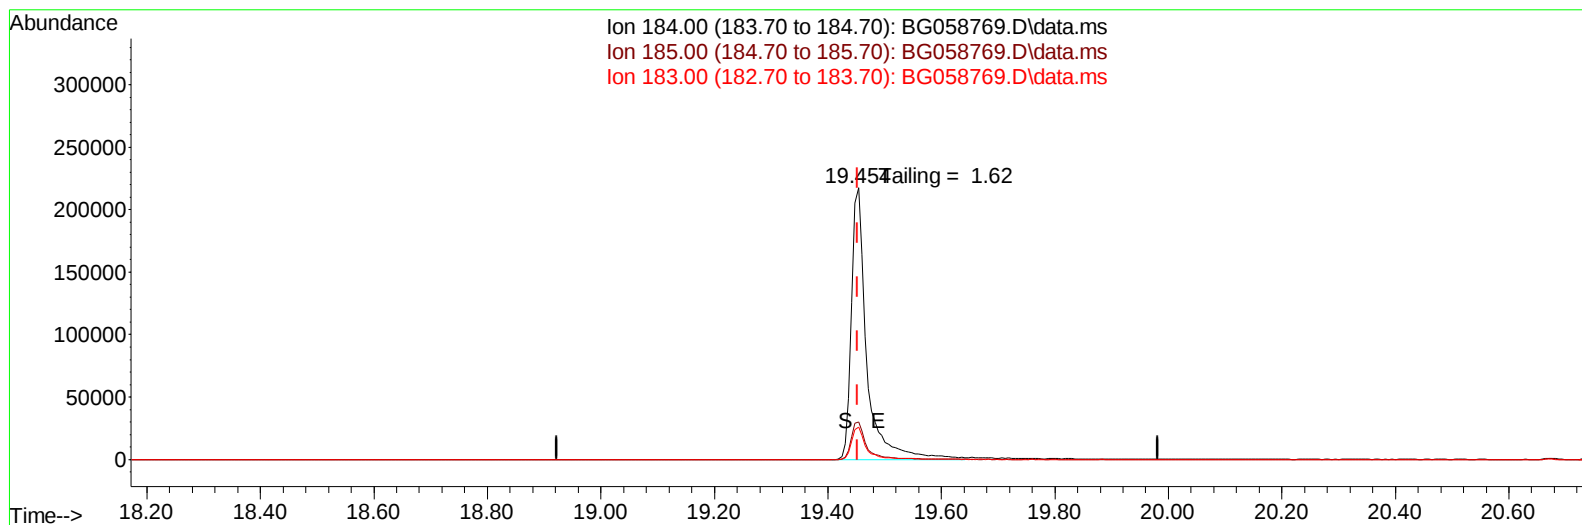

TIC: BG058769.D\data.ms

(77) Benzidine

19.454min (+ 0.002) 299332.90 ng

response 411060

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.81
183.00	12.50	11.87
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/18/2023	BNA_G	<u>BG058769.D</u>
Compound Name	Response	Retention Time
DDT	210277	20.676
DDD	2760	20.282
DDE	300	19.736
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3060	213337	1.43

Instrument :
BNA_G
ClientSampleId :
DFTPP