

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG082121\  
 Data File : BG049915.D  
 Acq On : 20 Aug 2021 18:39  
 Operator : CG/JU  
 Sample : PB138447BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 PB138447BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG080321.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049915.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.529       | 417           | 424         | 434          | rBV      | 532582         | 864898        | 35.20%          | 9.097%        |
| 2         | 7.145       | 692           | 699         | 717          | rBV      | 541934         | 915890        | 37.27%          | 9.633%        |
| 3         | 7.979       | 834           | 841         | 849          | rBV      | 102207         | 168075        | 6.84%           | 1.768%        |
| 4         | 9.148       | 1032          | 1040        | 1051         | rBV      | 329332         | 604066        | 24.58%          | 6.354%        |
| 5         | 10.798      | 1314          | 1321        | 1330         | rVB      | 126786         | 229880        | 9.36%           | 2.418%        |
| 6         | 13.254      | 1732          | 1739        | 1746         | rBV      | 880048         | 1367549       | 55.65%          | 14.384%       |
| 7         | 14.634      | 1968          | 1974        | 1982         | rBV      | 211736         | 316598        | 12.88%          | 3.330%        |
| 8         | 16.126      | 2222          | 2228        | 2239         | rBV      | 726067         | 1124744       | 45.77%          | 11.830%       |
| 9         | 17.384      | 2436          | 2442        | 2450         | rBV      | 254960         | 400118        | 16.28%          | 4.208%        |
| 10        | 19.998      | 2881          | 2887        | 2895         | rVB      | 1874420        | 2457276       | 100.00%         | 25.846%       |
| 11        | 21.660      | 3163          | 3170        | 3180         | rBV2     | 287920         | 476904        | 19.41%          | 5.016%        |
| 12        | 23.939      | 3549          | 3558        | 3563         | rBV7     | 9027           | 27315         | 1.11%           | 0.287%        |
| 13        | 24.885      | 3708          | 3719        | 3732         | rVB2     | 169142         | 489970        | 19.94%          | 5.154%        |
| 14        | 26.013      | 3902          | 3911        | 3920         | rVB9     | 11961          | 34227         | 1.39%           | 0.360%        |
| 15        | 27.352      | 4135          | 4139        | 4150         | rVB9     | 10957          | 29876         | 1.22%           | 0.314%        |




Sum of corrected areas: 9507386

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG082121\  
Data File : BG049915.D  
Acq On : 20 Aug 2021 18:39  
Operator : CG/JU  
Sample : PB138447BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB138447BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG080321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

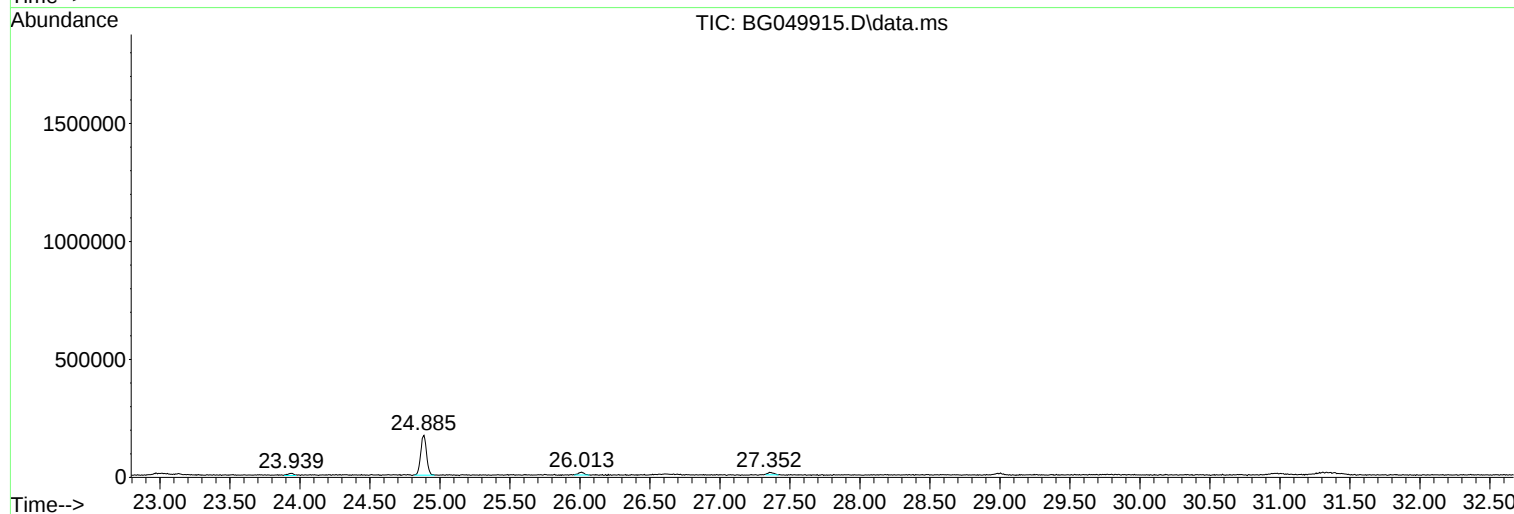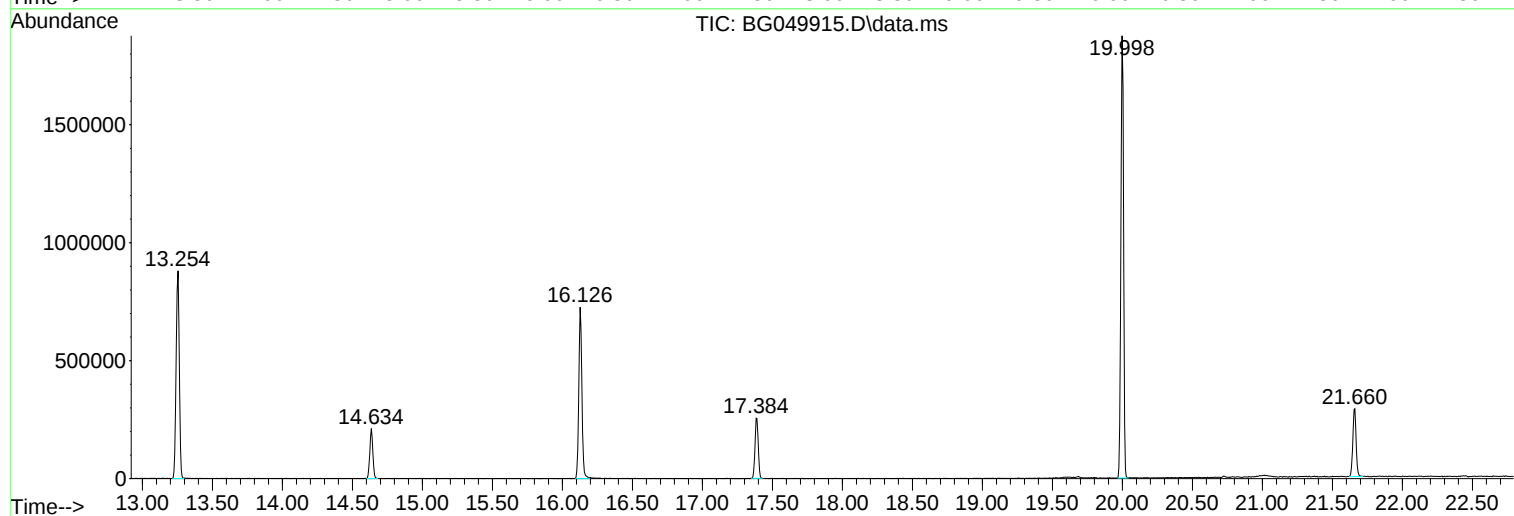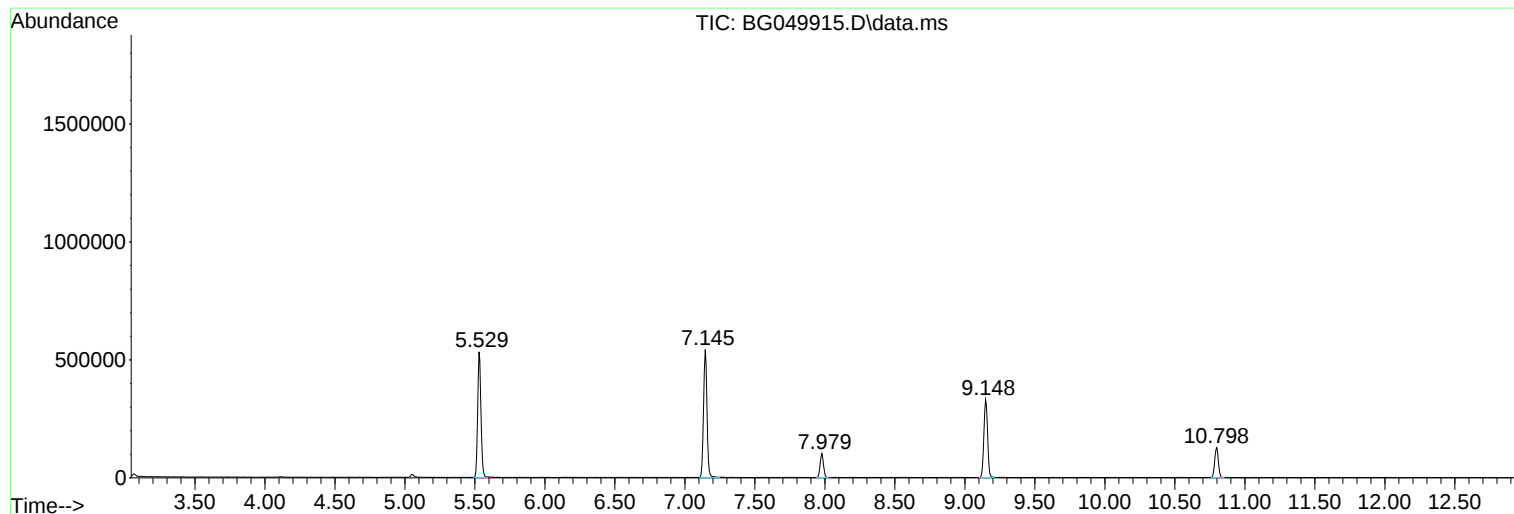

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG082121\  
Data File : BG049915.D  
Acq On : 20 Aug 2021 18:39  
Operator : CG/JU  
Sample : PB138447BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB138447BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG080321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG082121\  
Data File : BG049915.D  
Acq On : 20 Aug 2021 18:39  
Operator : CG/JU  
Sample : PB138447BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB138447BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG080321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|