

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
 Data File : BG049916.D
 Acq On : 20 Aug 2021 19:26
 Operator : CG/JU
 Sample : M3463-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SWCS-20-0003

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG049916.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.067	3	5	15	rVB	89188	131820	10.50%	0.898%
2	5.534	418	425	435	rBV	339062	546281	43.51%	3.719%
3	7.149	692	700	710	rVB	346138	613131	48.84%	4.175%
4	7.978	833	841	847	rVB	82010	147021	11.71%	1.001%
5	9.153	1033	1041	1049	rBV	217061	384789	30.65%	2.620%
6	10.568	1276	1282	1291	rBV	32656	65318	5.20%	0.445%
7	10.797	1314	1321	1328	rVB2	112694	212828	16.95%	1.449%
8	13.253	1731	1739	1748	rBV	356098	555629	44.26%	3.783%
9	14.087	1860	1881	1882	rBV2	85468	266738	21.25%	1.816%
10	14.586	1963	1966	1969	rBV5	9892	14149	1.13%	0.096%
11	14.633	1969	1974	1981	rVB	171966	278963	22.22%	1.899%
12	16.131	2222	2229	2237	rBV	425674	684349	54.51%	4.660%
13	17.388	2437	2443	2451	rBV	235227	359902	28.67%	2.450%
14	17.870	2521	2525	2526	rBV4	10949	13397	1.07%	0.091%
15	18.281	2590	2595	2608	rVB2	310202	541486	43.13%	3.687%
16	18.434	2617	2621	2624	rBV3	23321	35852	2.86%	0.244%
17	19.450	2789	2794	2796	rBV2	55766	96261	7.67%	0.655%
18	19.492	2798	2801	2805	rVV2	134437	256129	20.40%	1.744%
19	19.550	2805	2811	2827	rVB	504223	1028754	81.94%	7.004%
20	19.997	2882	2887	2894	rVB	427792	561430	44.72%	3.823%
21	20.308	2933	2940	2947	rBV	167917	336615	26.81%	2.292%
22	21.031	3058	3063	3070	rVB	253677	390706	31.12%	2.660%
23	21.307	3105	3110	3118	rVB3	90674	192068	15.30%	1.308%
24	21.471	3133	3138	3146	rBV2	74155	124553	9.92%	0.848%
25	21.659	3165	3170	3177	rVB	243841	400687	31.92%	2.728%
26	21.794	3187	3193	3203	rVB2	200475	417161	33.23%	2.840%
27	22.440	3301	3303	3306	rVB3	30444	31459	2.51%	0.214%
28	22.499	3307	3313	3322	rVB4	129840	310888	24.76%	2.117%
29	22.658	3333	3340	3349	rVB2	211891	510801	40.69%	3.478%
30	23.216	3429	3435	3442	rBV6	44113	115613	9.21%	0.787%
31	23.662	3503	3511	3525	rVB2	191922	525521	41.86%	3.578%
32	23.938	3552	3558	3565	rVB3	69711	156874	12.50%	1.068%
33	24.038	3569	3575	3585	rVV5	67679	196974	15.69%	1.341%
34	24.150	3587	3594	3604	rVB3	93138	222865	17.75%	1.517%
35	24.843	3703	3712	3713	rBV2	159049	357421	28.47%	2.434%
36	25.154	3759	3765	3776	rVB9	44821	137765	10.97%	0.938%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049916.D
Acq On : 20 Aug 2021 19:26
Operator : CG/JU
Sample : M3463-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-20-0003

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	26.235	3941	3949	3959	rVB4	130149	447079	35.61%	3.044%
38	26.335	3960	3966	3974	rVB4	57651	156331	12.45%	1.064%
39	26.605	4003	4012	4024	rVB6	94948	305241	24.31%	2.078%
40	27.910	4225	4234	4246	rVB5	91829	367406	29.27%	2.502%
41	29.454	4483	4497	4511	rVB5	198694	933375	74.35%	6.355%
42	30.383	4642	4655	4672	rVB6	249007	1255434	100.00%	8.548%




Sum of corrected areas: 14687064

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049916.D
Acq On : 20 Aug 2021 19:26
Operator : CG/JU
Sample : M3463-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-20-0003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

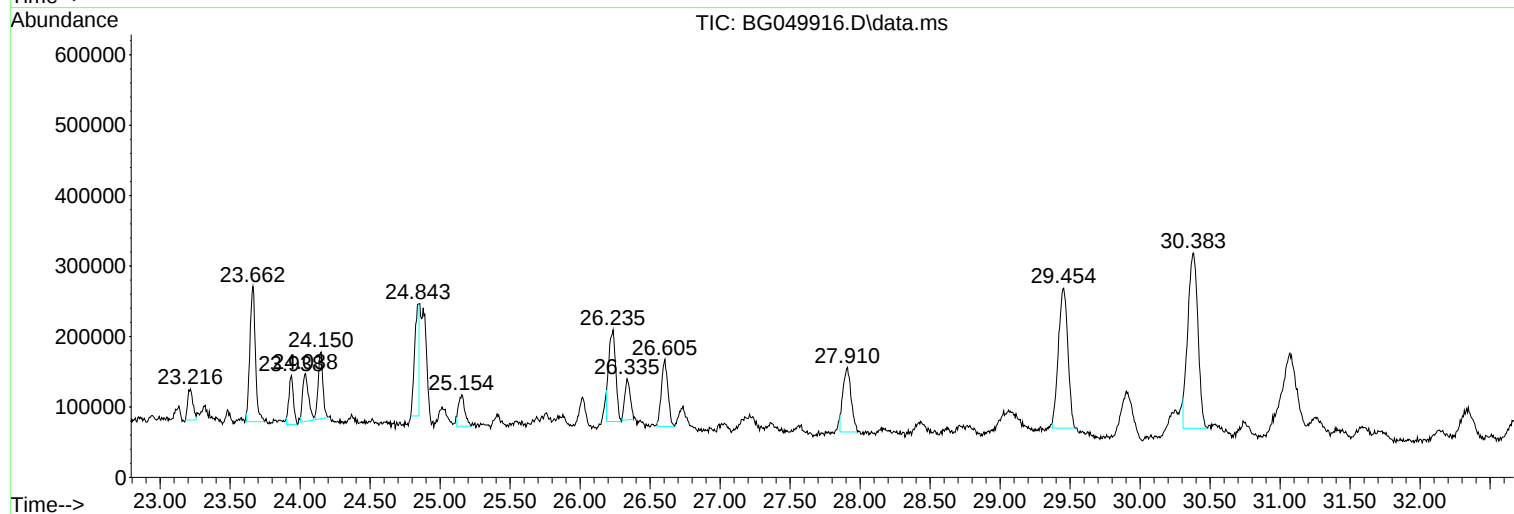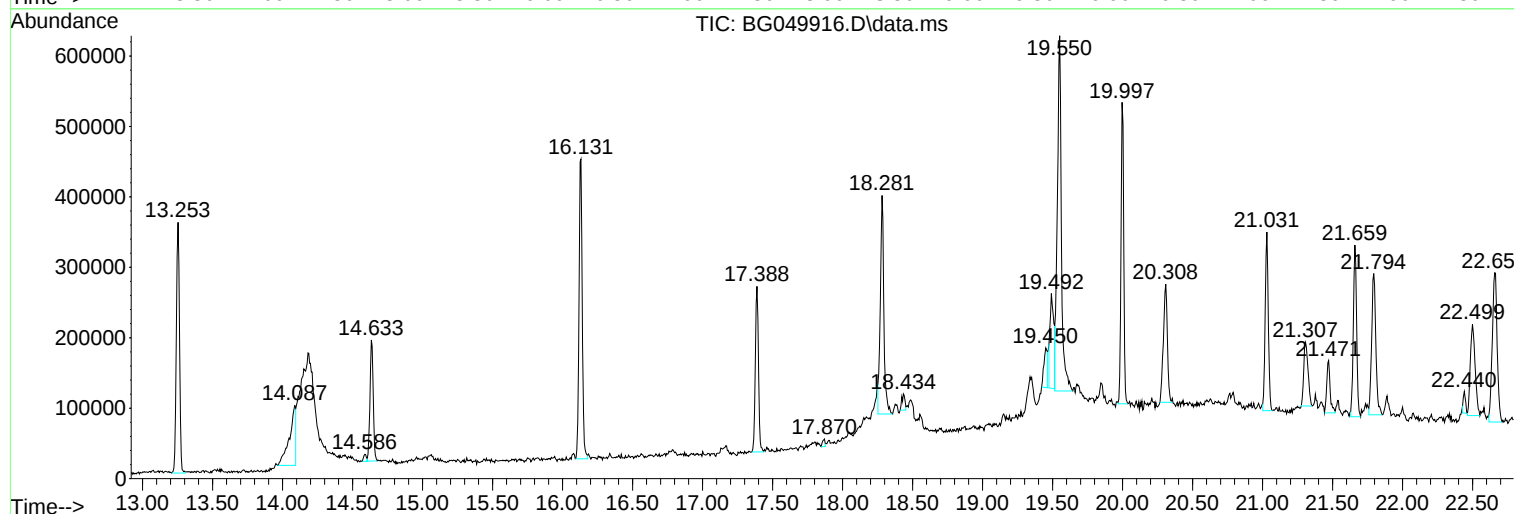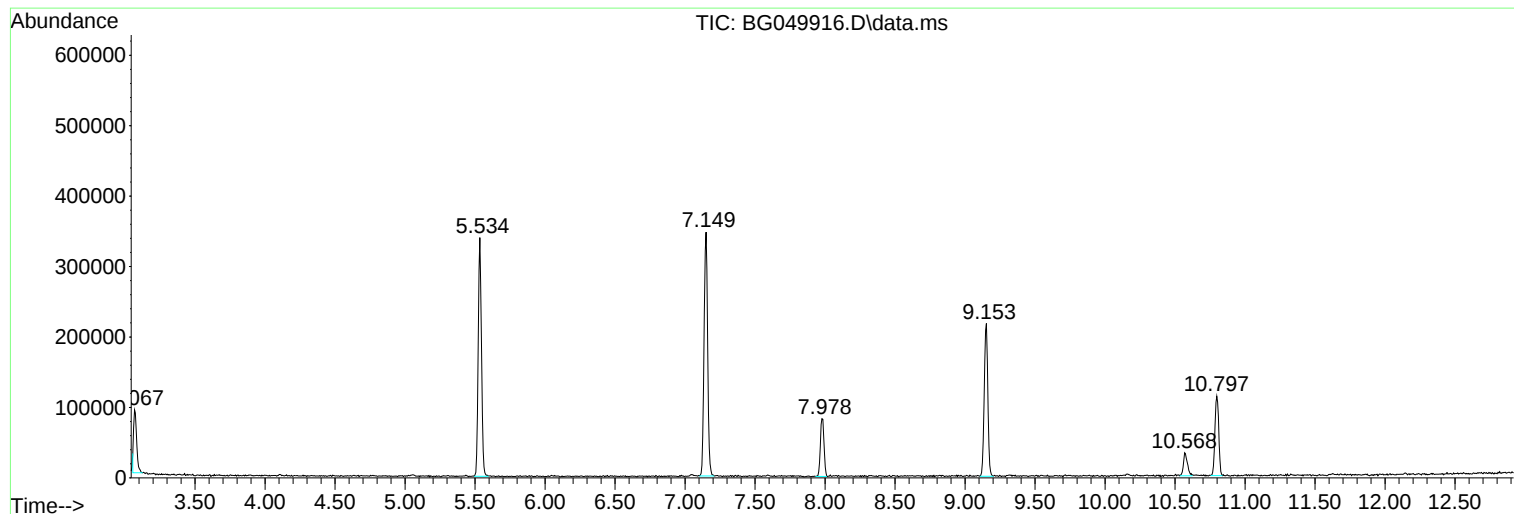

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049916.D
Acq On : 20 Aug 2021 19:26
Operator : CG/JU
Sample : M3463-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-20-0003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082121\
Data File : BG049916.D
Acq On : 20 Aug 2021 19:26
Operator : CG/JU
Sample : M3463-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SWCS-20-0003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------